




Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
Calibration Table Last Updated: Thu Jan 24 06:50:06 2019

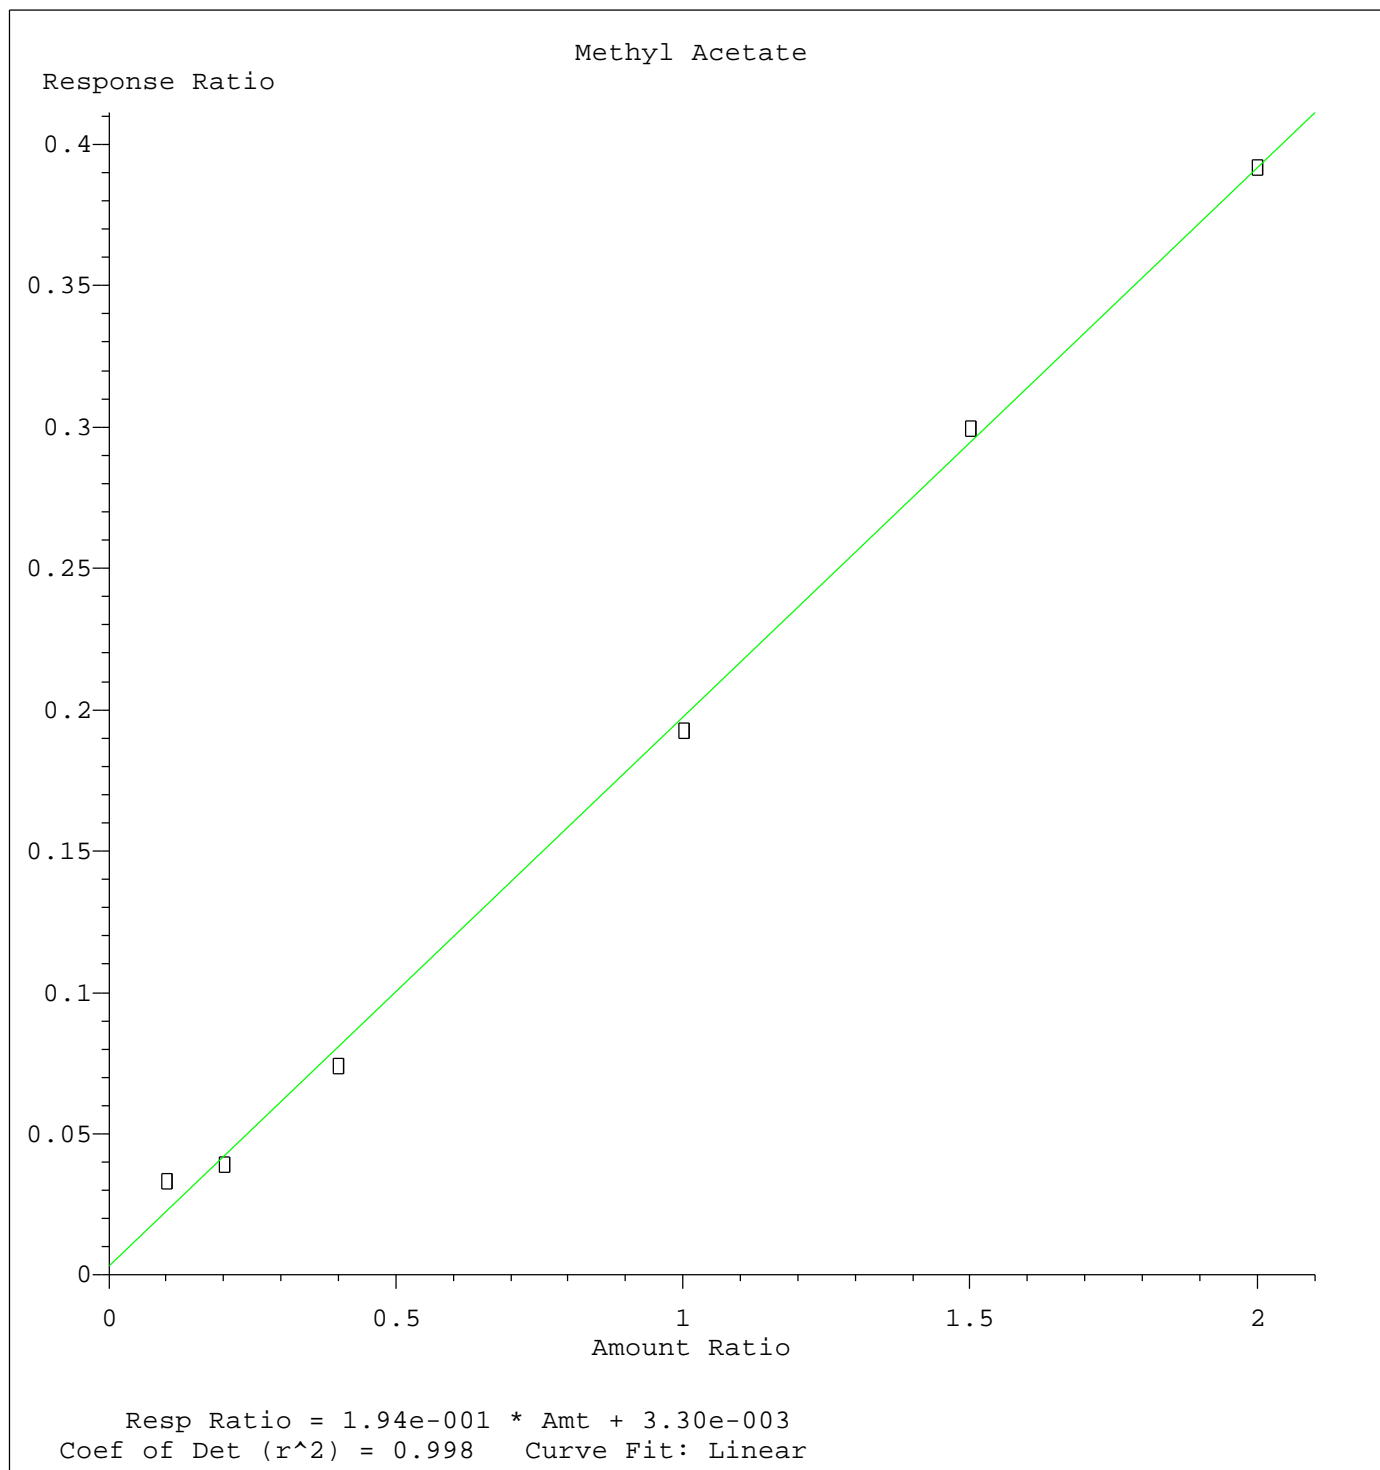


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
Calibration Table Last Updated: Thu Jan 24 06:50:06 2019

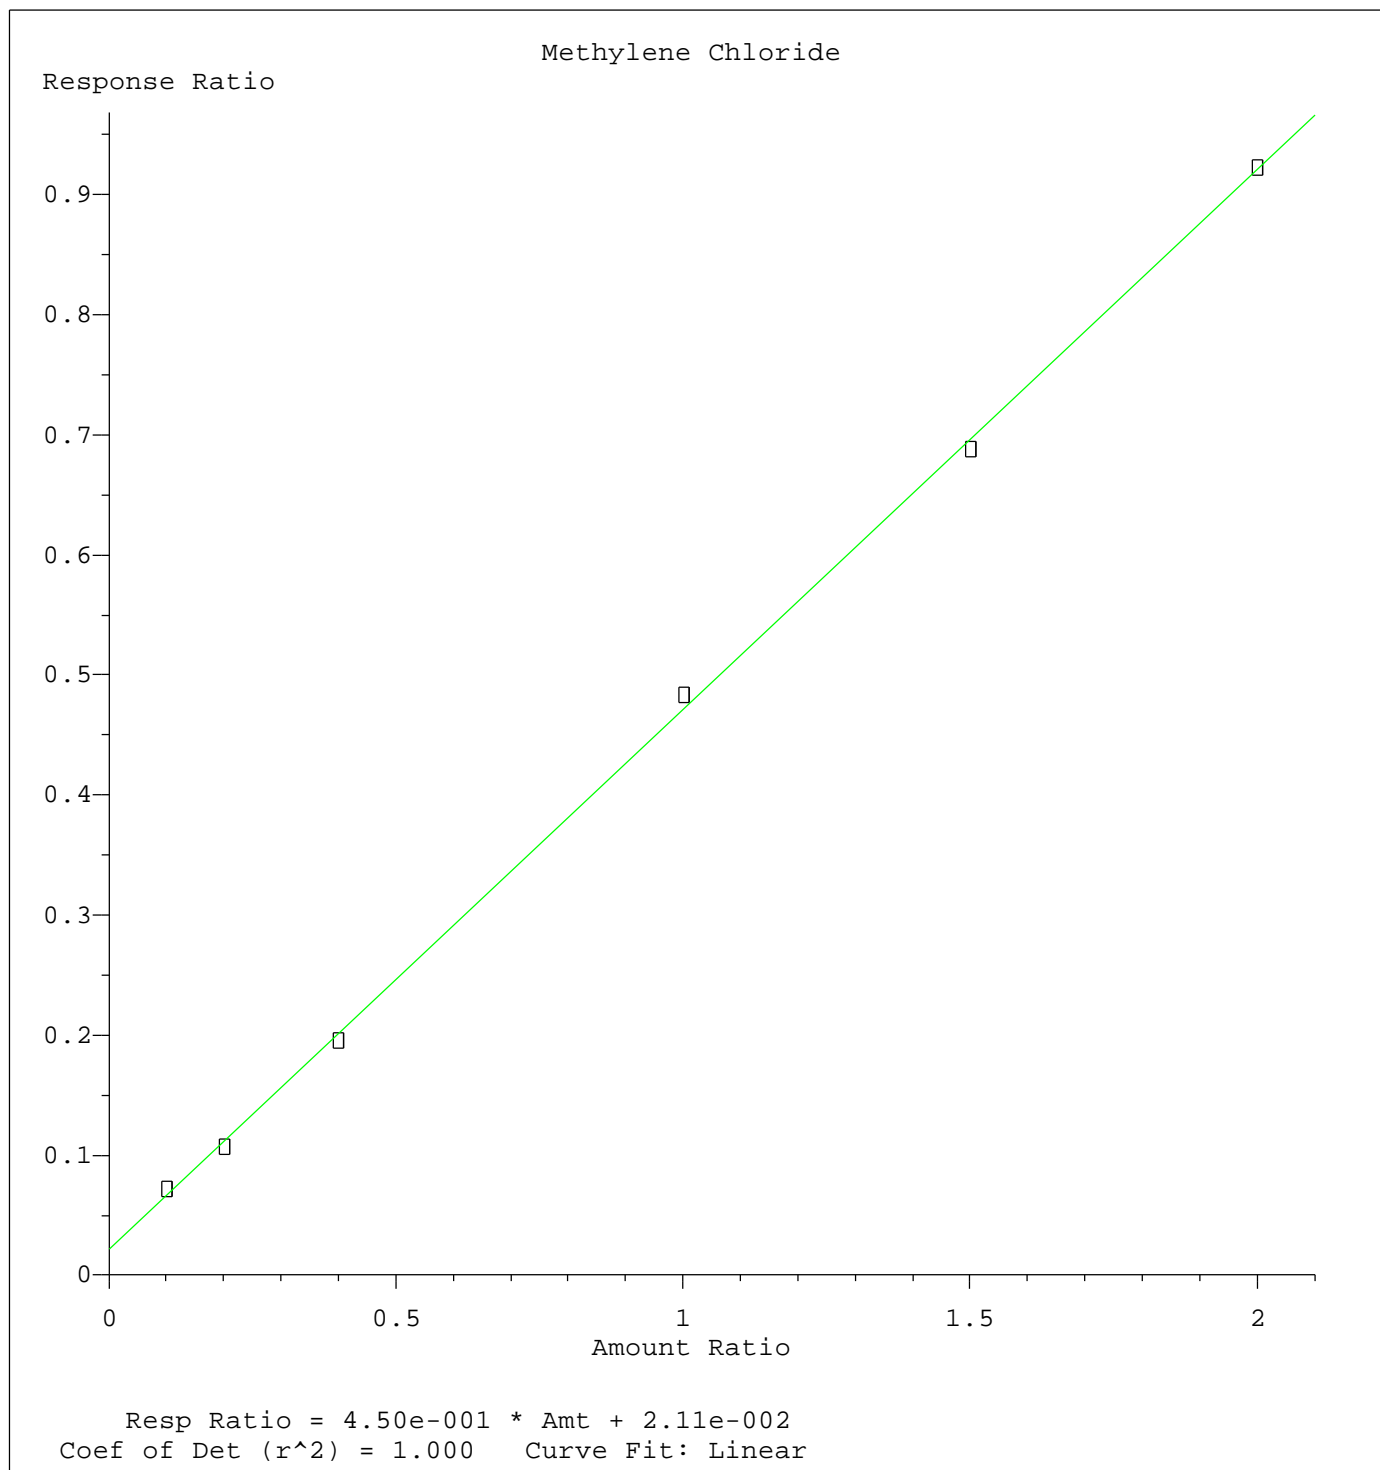


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
Calibration Table Last Updated: Thu Jan 24 06:50:06 2019

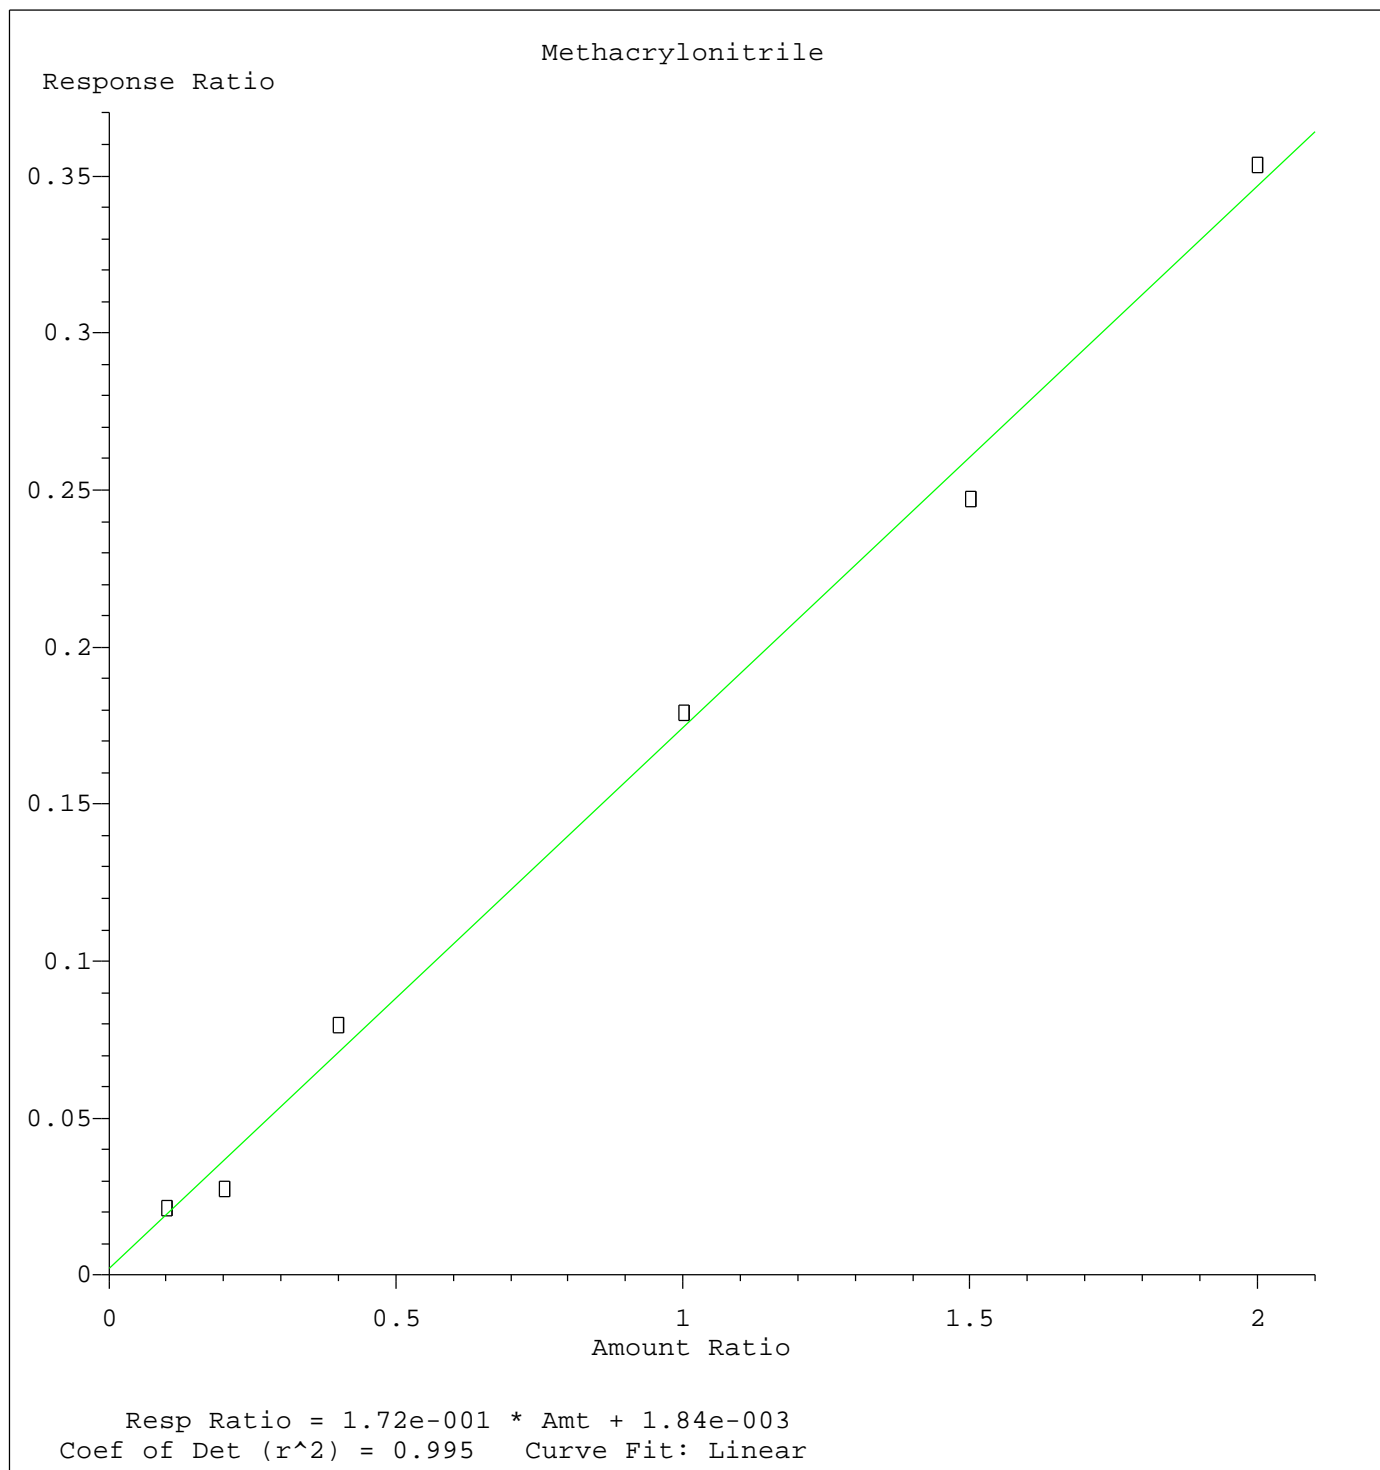

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
Calibration Table Last Updated: Thu Jan 24 06:50:06 2019

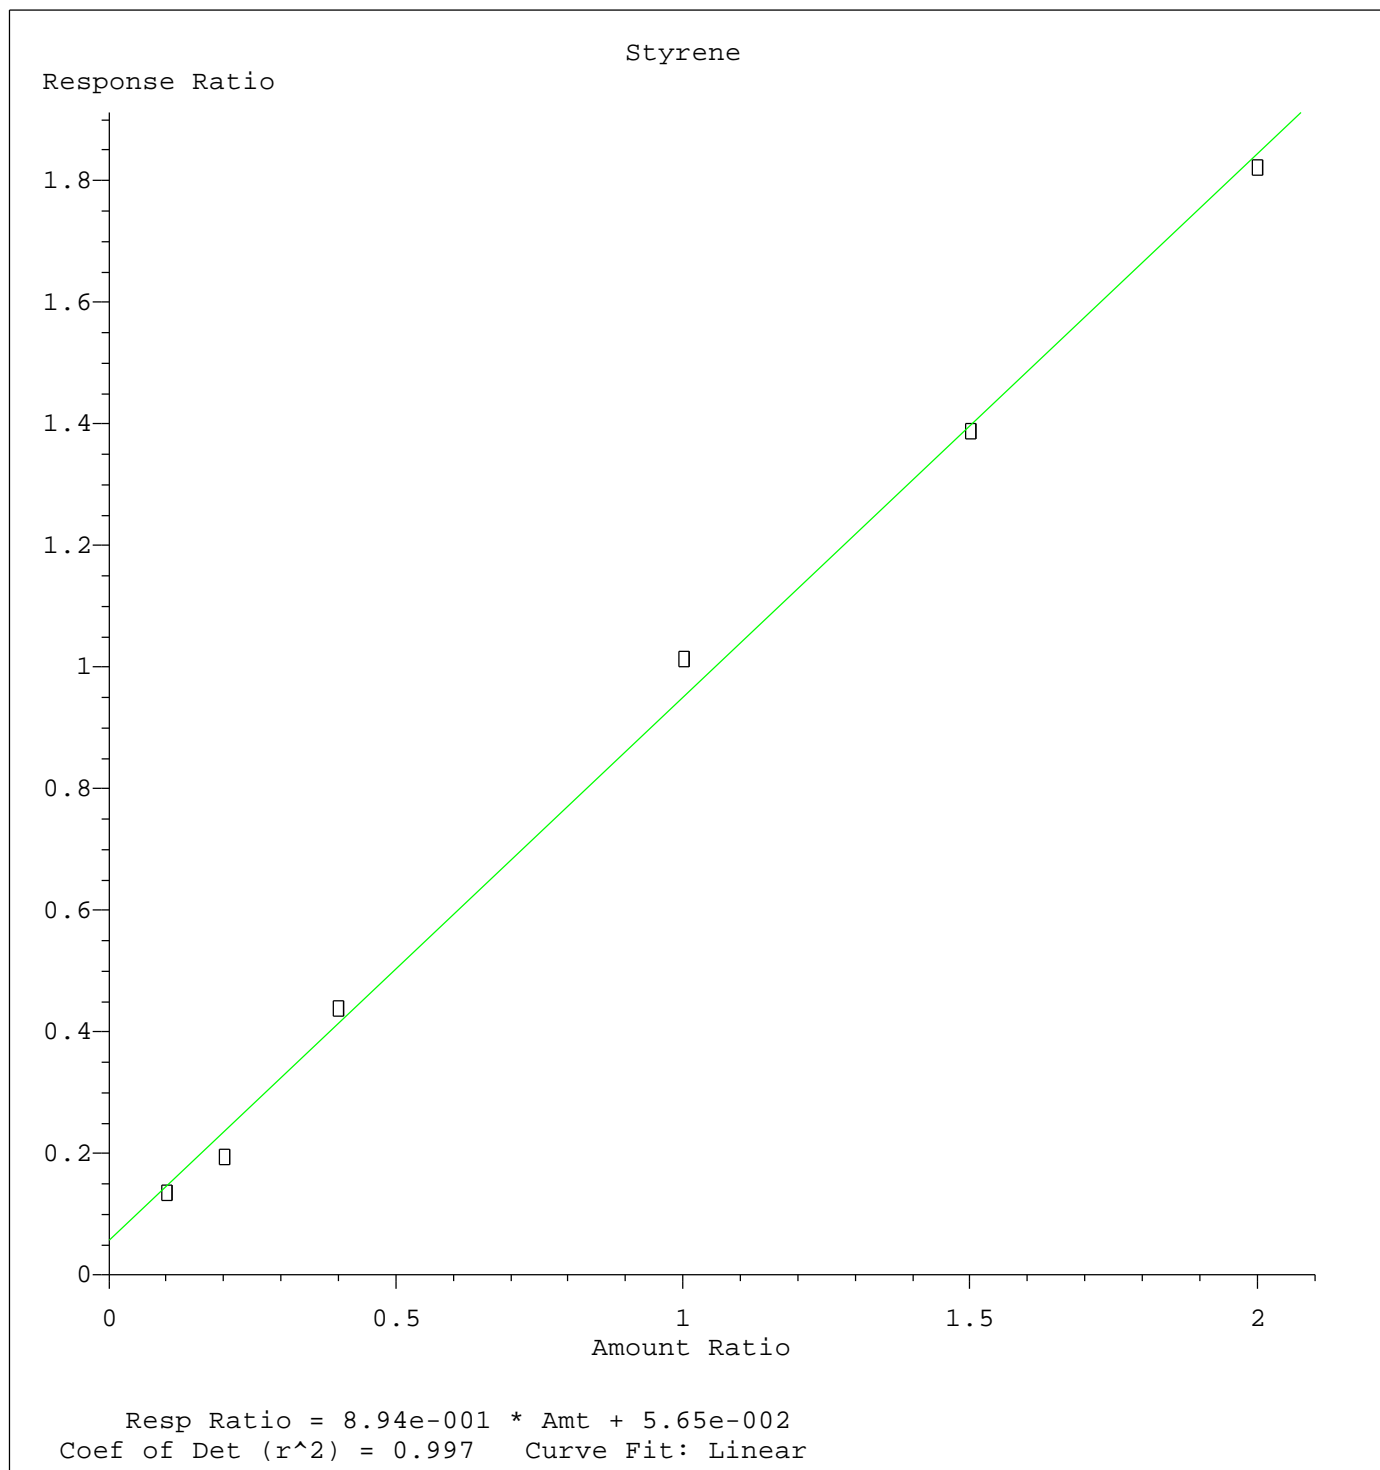

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
Calibration Table Last Updated: Thu Jan 24 06:50:06 2019

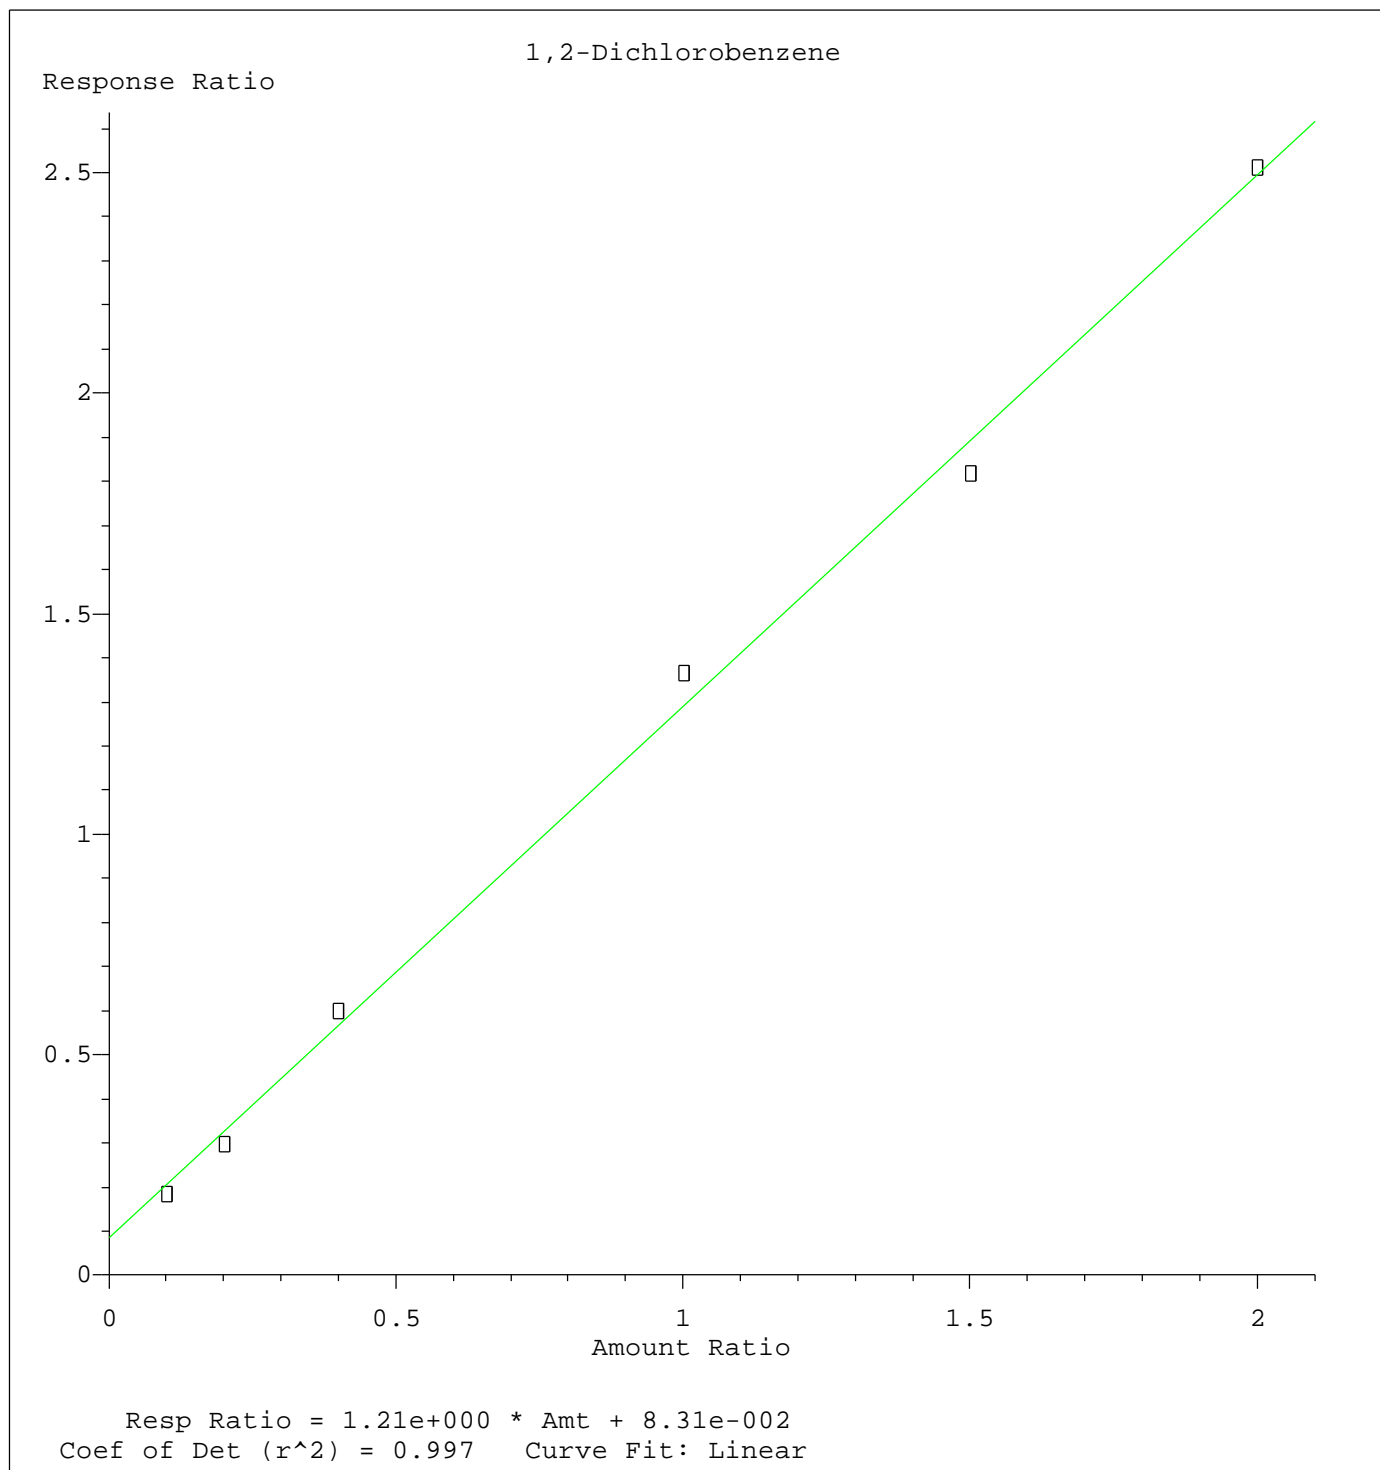

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
Calibration Table Last Updated: Thu Jan 24 06:50:06 2019