


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD012319\
 Data File : VD060782.D
 Acq On : 23 Jan 2019 13:30
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012319S.M
 Title : SW846 8260
 Last Update : Thu Jan 24 06:50:06 2019

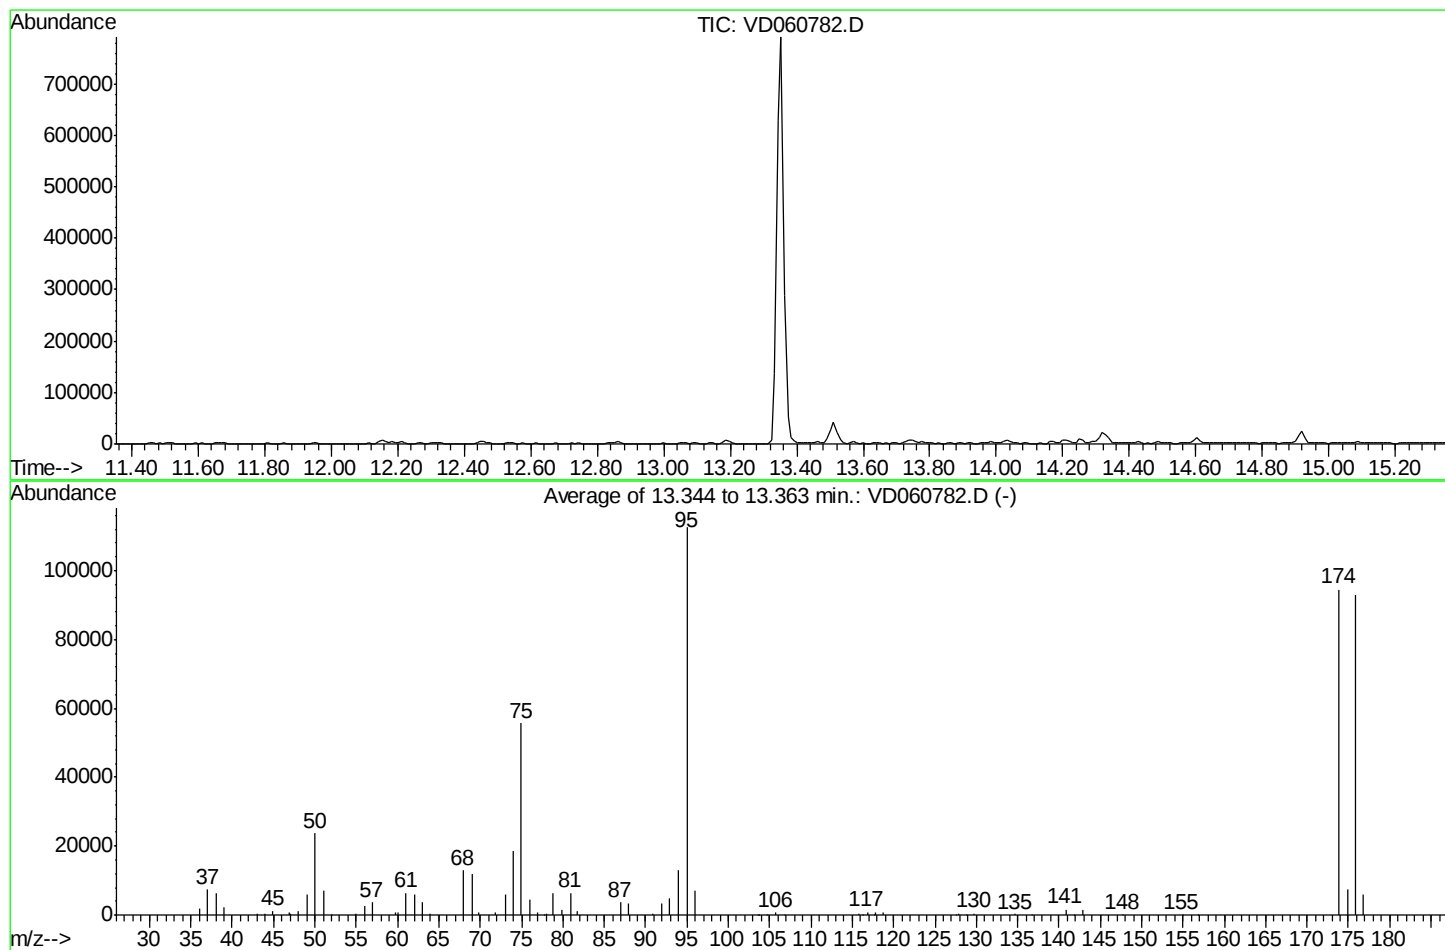

AutoFind: Scans 1251, 1252, 1253; Background Corrected with Scan 1246

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	23750	PASS
75	95	30	60	49.4	55632	PASS
95	95	100	100	100.0	112546	PASS
96	95	5	9	6.4	7166	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.9	94421	PASS
175	174	5	9	7.7	7274	PASS
176	174	95	101	98.6	93061	PASS
177	176	5	9	6.5	6023	PASS