


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D012320S.M  
Calibration Table Last Updated: Thu Jan 23 13:45:59 2020

Methylene Chloride

Response Ratio

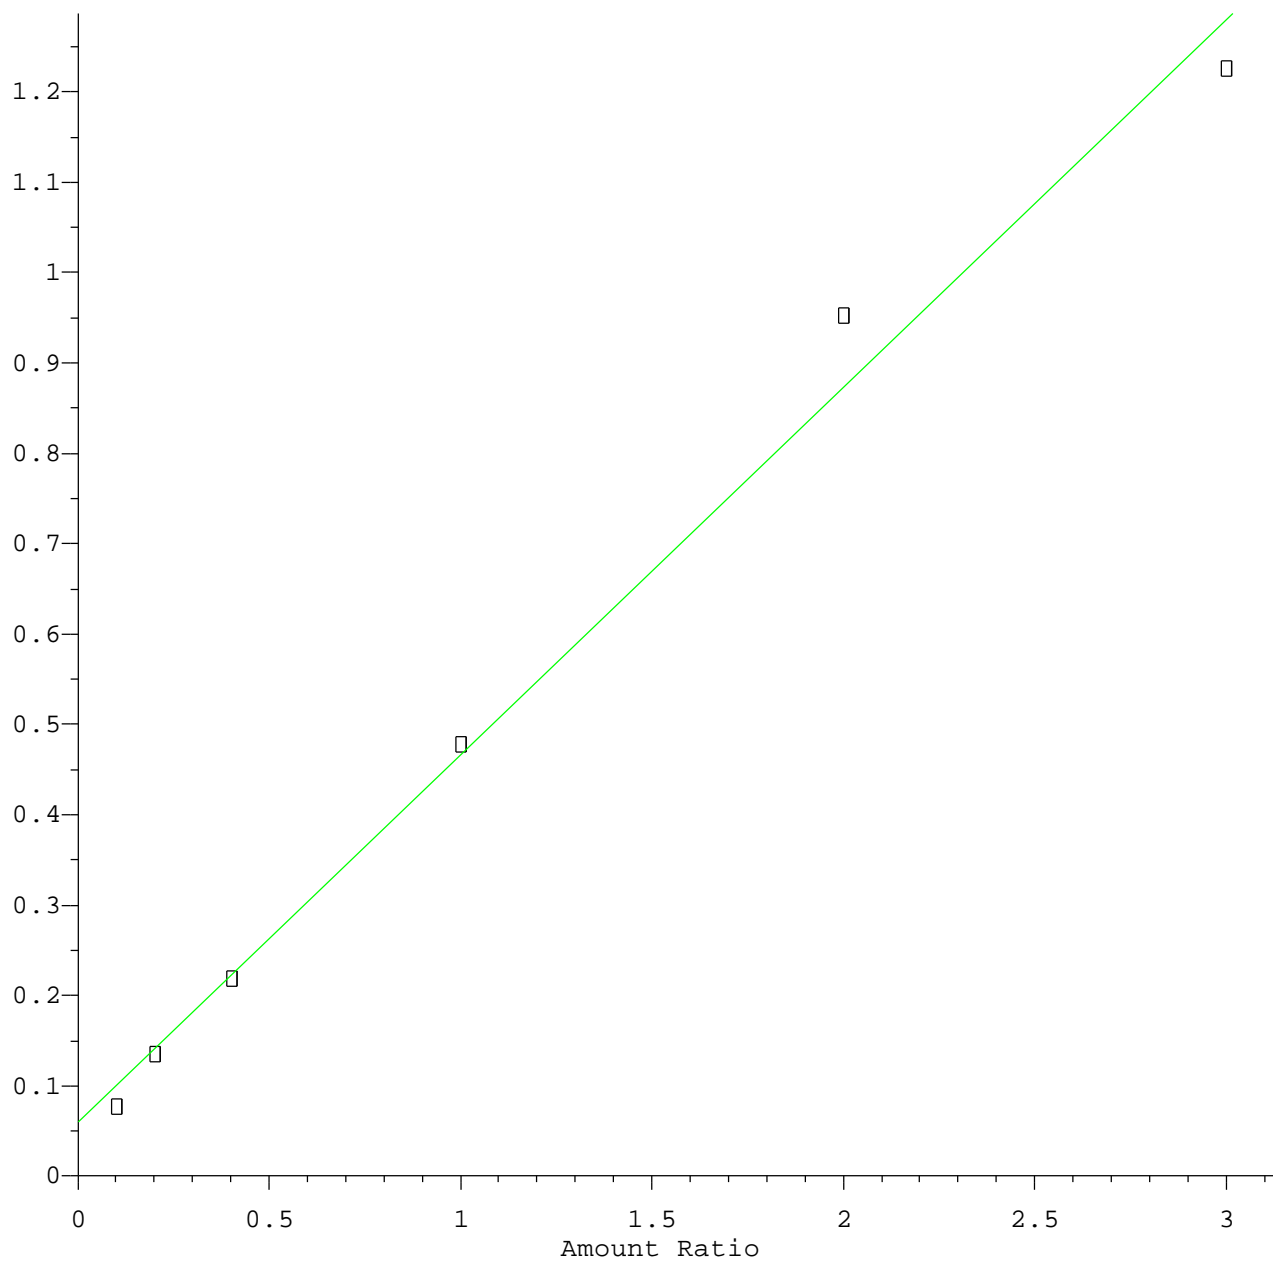

Resp Ratio =  $4.07 \times 10^{-1} \times \text{Amt} + 5.97 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.991    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D012320S.M  
Calibration Table Last Updated: Thu Jan 23 13:45:59 2020