

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012323\
 Data File : VD075173.D
 Acq On : 23 Jan 2023 14:04
 Operator : KP/SY
 Sample : 01233-03
 Misc : 5.06G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 B-P34B

Quant Time: Jan 23 14:11:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 19 01:32:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	49085	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	95032	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.587	117	93578	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	41757	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	33237	66.358	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	132.720%
35) Dibromofluoromethane	7.804	113	30709	53.477	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.960%
50) Toluene-d8	10.269	98	119243	52.738	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	105.480%
62) 4-Bromofluorobenzene	12.575	95	40309	56.173	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	112.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012323\
Data File : VD075173.D
Acq On : 23 Jan 2023 14:04
Operator : KP/SY
Sample : 01233-03
Misc : 5.06G/5.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
B-P34B

Quant Time: Jan 23 14:11:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 19 01:32:27 2023
Response via : Initial Calibration



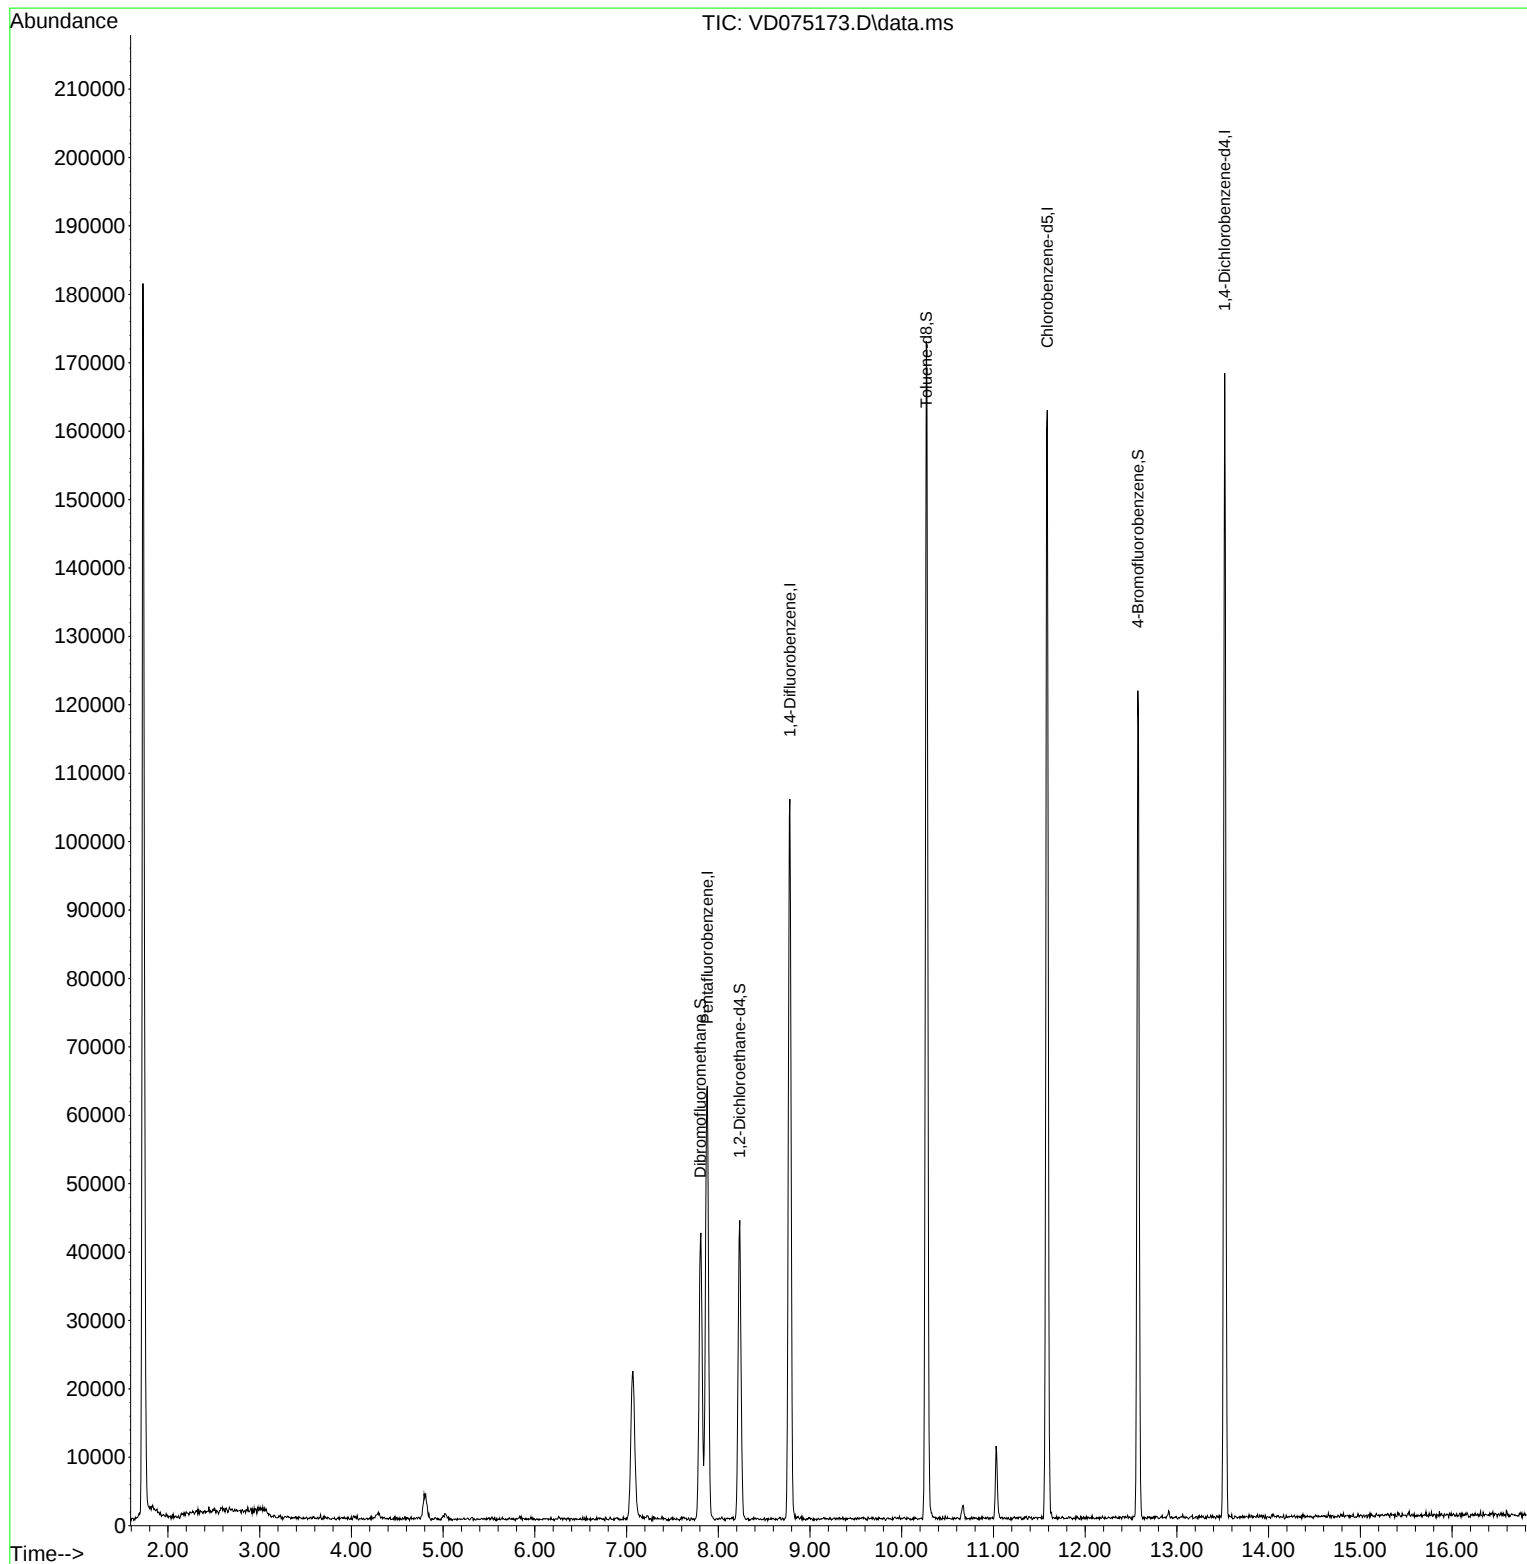


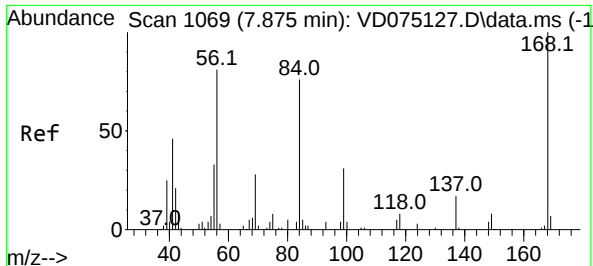

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04




Instrument :
MSVOA_D
ClientSampleId :
B-P34B


Tgt Ion:168 Resp: 49085
Ion Ratio Lower Upper
168 100
99 54.1 45.2 67.8

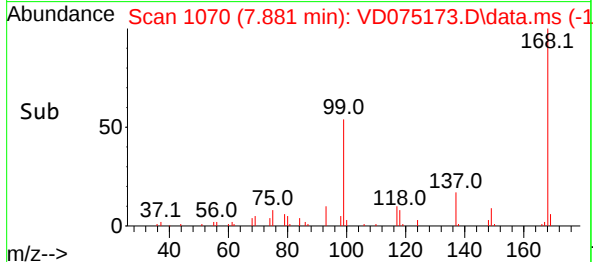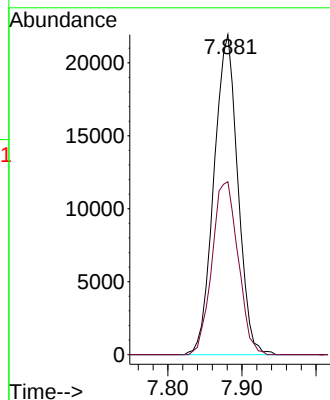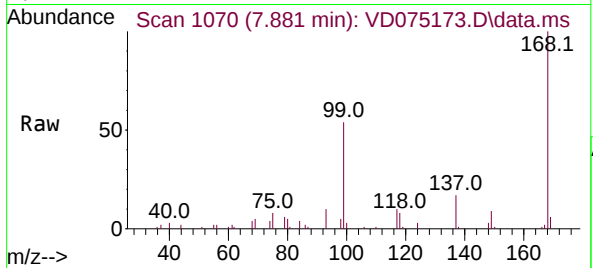

#33
1,2-Dichloroethane-d4
Concen: 66.358 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04

Tgt Ion: 65 Resp: 33237
Ion Ratio Lower Upper
65 100
67 54.3 0.0 105.2


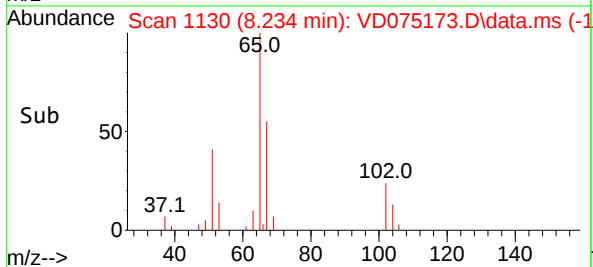
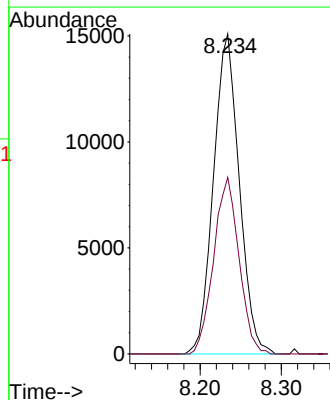
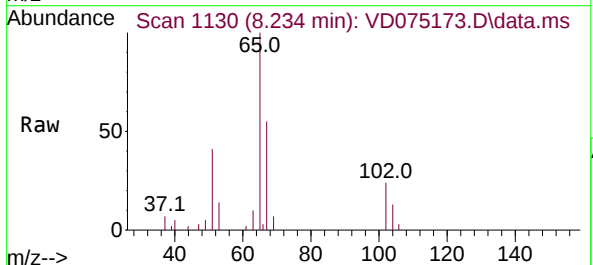


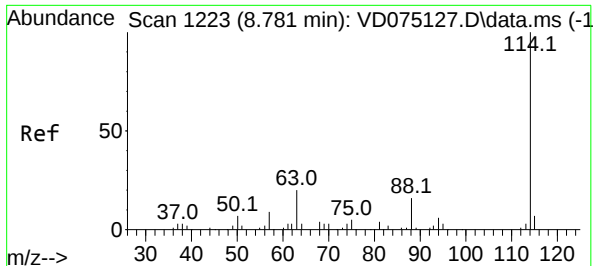

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.781 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04




Instrument :
MSVOA_D
ClientSampleId :
B-P34B

Tgt Ion:114 Resp: 95032
Ion Ratio Lower Upper
114 100
63 17.9 0.0 40.2
88 15.2 0.0 32.2

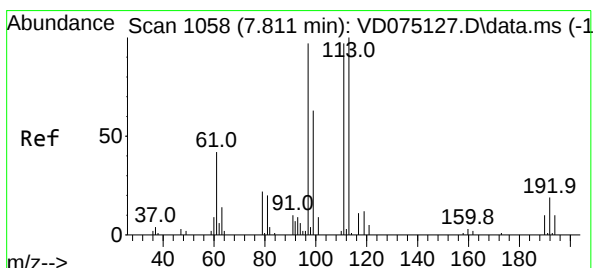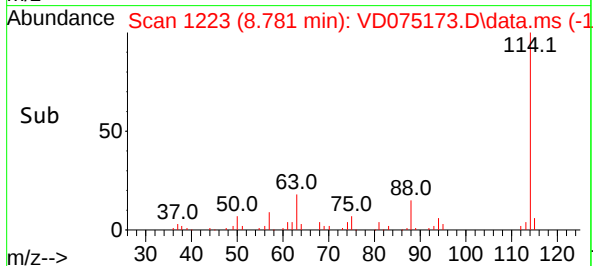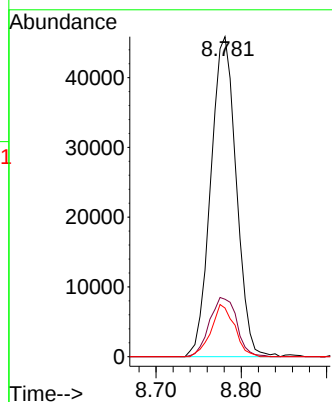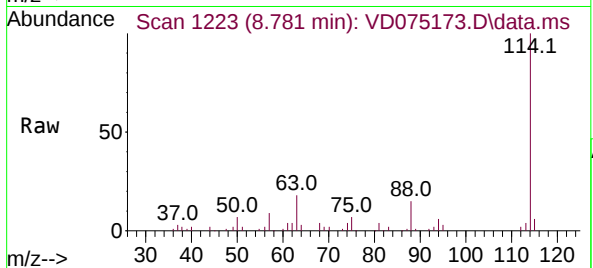

#35
Dibromofluoromethane
Concen: 53.477 ug/l
RT: 7.804 min Scan# 1057
Delta R.T. -0.006 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04

Tgt Ion:113 Resp: 30709
Ion Ratio Lower Upper
113 100
111 103.9 80.1 120.1
192 16.8 15.4 23.0


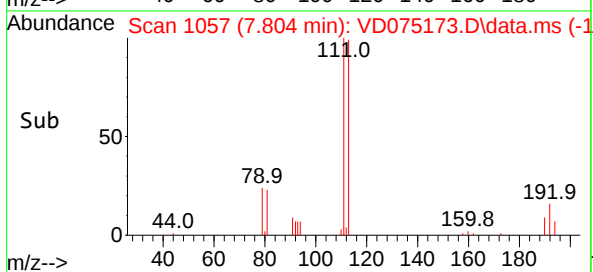
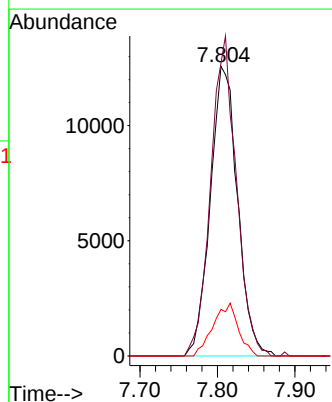
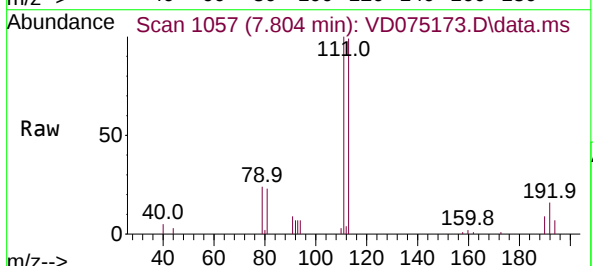




#50
Toluene-d8
Concen: 52.738 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04




Instrument :
MSVOA_D
ClientSampleId :
B-P34B


Tgt Ion: 98 Resp: 119243
Ion Ratio Lower Upper
98 100
100 64.6 52.7 79.1

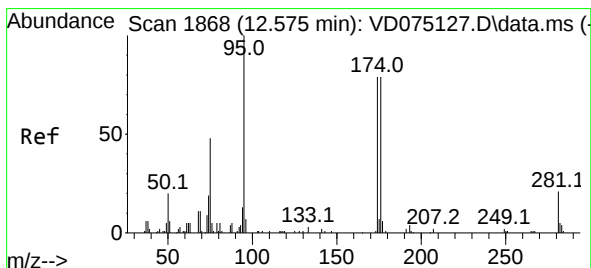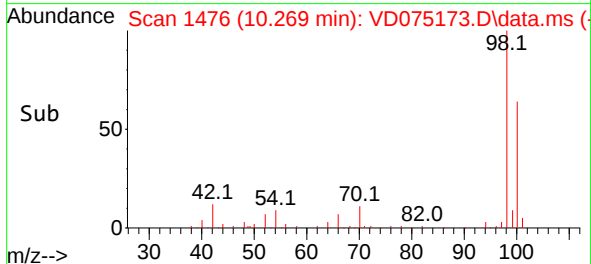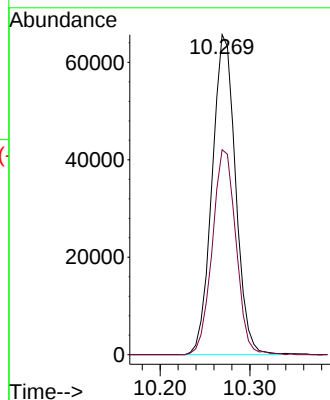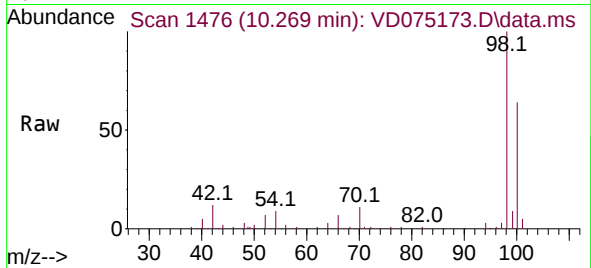

#62
4-Bromofluorobenzene
Concen: 56.173 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04

Tgt Ion: 95 Resp: 40309
Ion Ratio Lower Upper
95 100
174 75.1 0.0 161.2
176 74.7 0.0 160.2


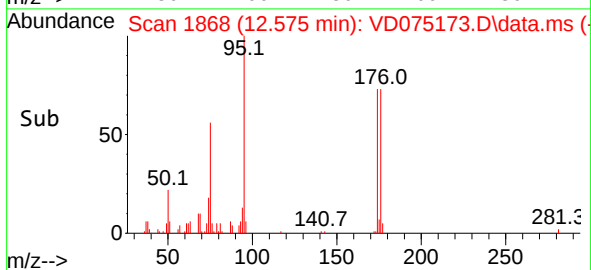
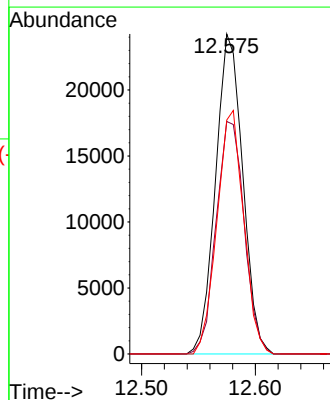
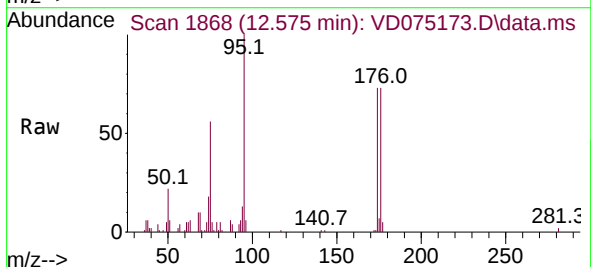


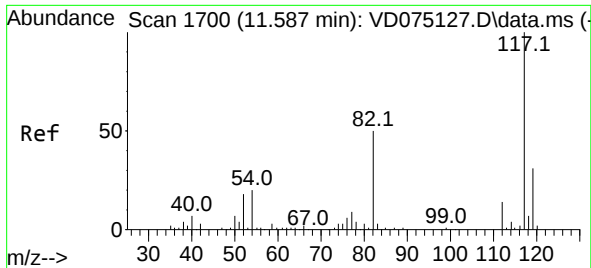

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.587 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04

Instrument :
MSVOA_D
ClientSampleId :
B-P34B

Tgt Ion:117 Resp: 93578
Ion Ratio Lower Upper
117 100
82 54.3 39.6 59.4
119 31.1 24.6 37.0

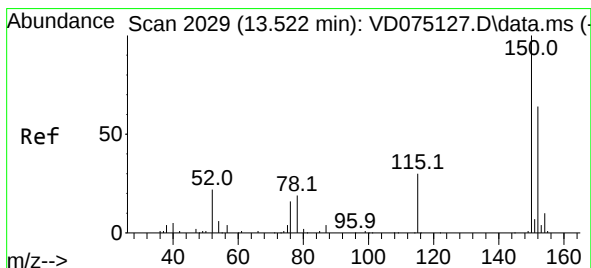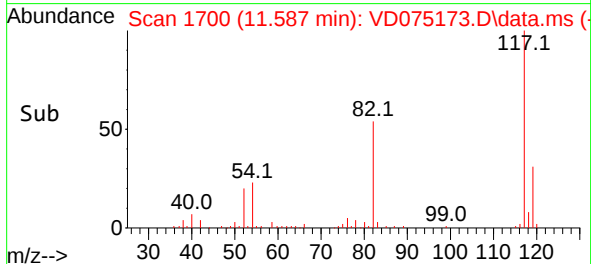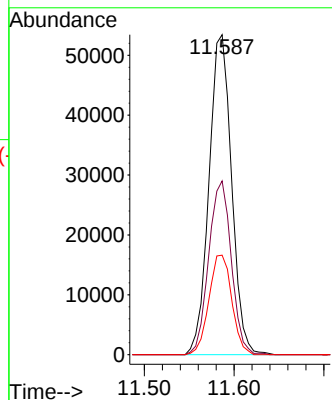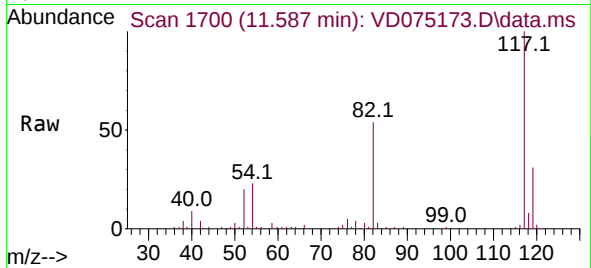

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD075173.D
Acq: 23 Jan 2023 14:04

Tgt Ion:152 Resp: 41757
Ion Ratio Lower Upper
152 100
115 60.1 28.8 86.4
150 159.8 0.0 348.6

