
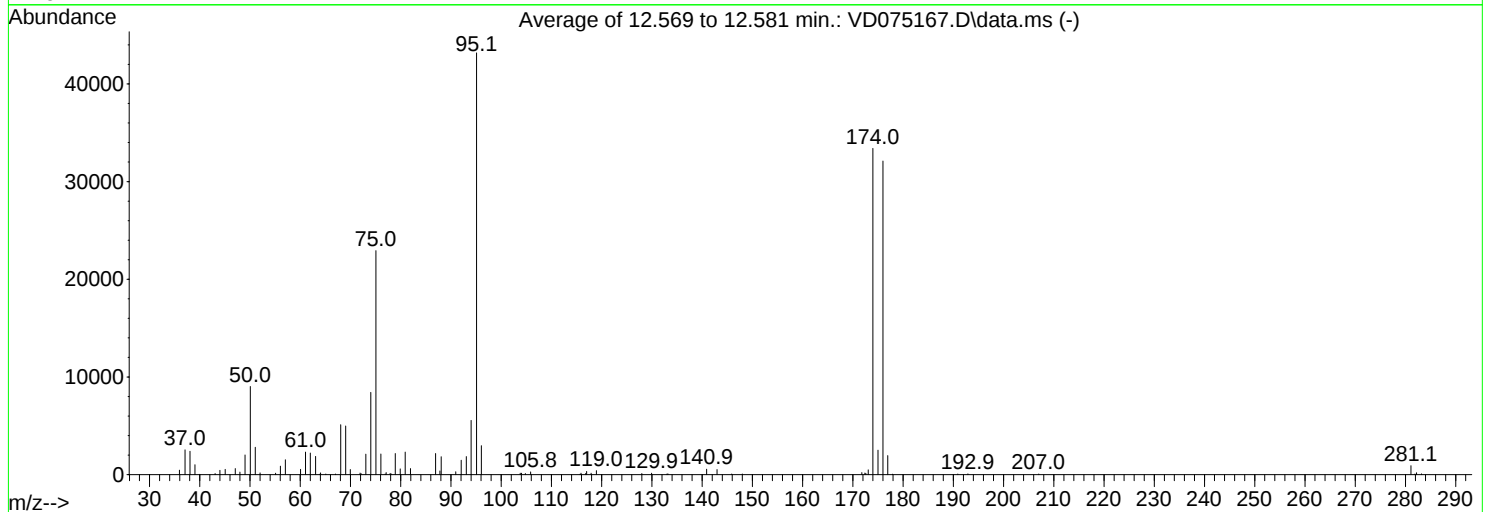


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012323\
Data File : VD075167.D
Acq On : 23 Jan 2023 09:38
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
Title : SW846 8260
Last Update : Thu Jan 19 01:32:27 2023

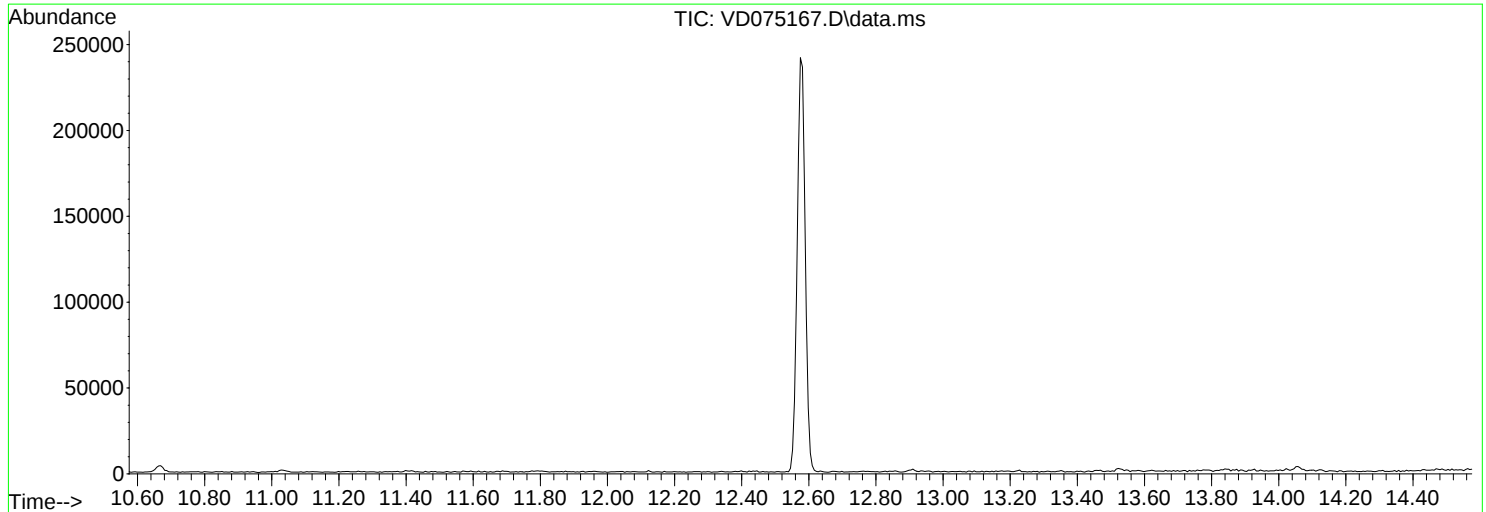

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	9034	PASS
75	95	30	60	53.1	22933	PASS
95	95	100	100	100.0	43181	PASS
96	95	5	9	6.9	2966	PASS
173	174	0.00	2	1.5	499	PASS
174	95	50	100	77.3	33392	PASS
175	174	5	9	7.5	2509	PASS
176	174	95	101	96.1	32101	PASS
177	176	5	9	6.1	1950	PASS