


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012622\
Data File : VD071782.D
Acq On : 26 Jan 2022 10:29
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Title : SW846 8260
Last Update : Thu Jan 27 06:04:38 2022

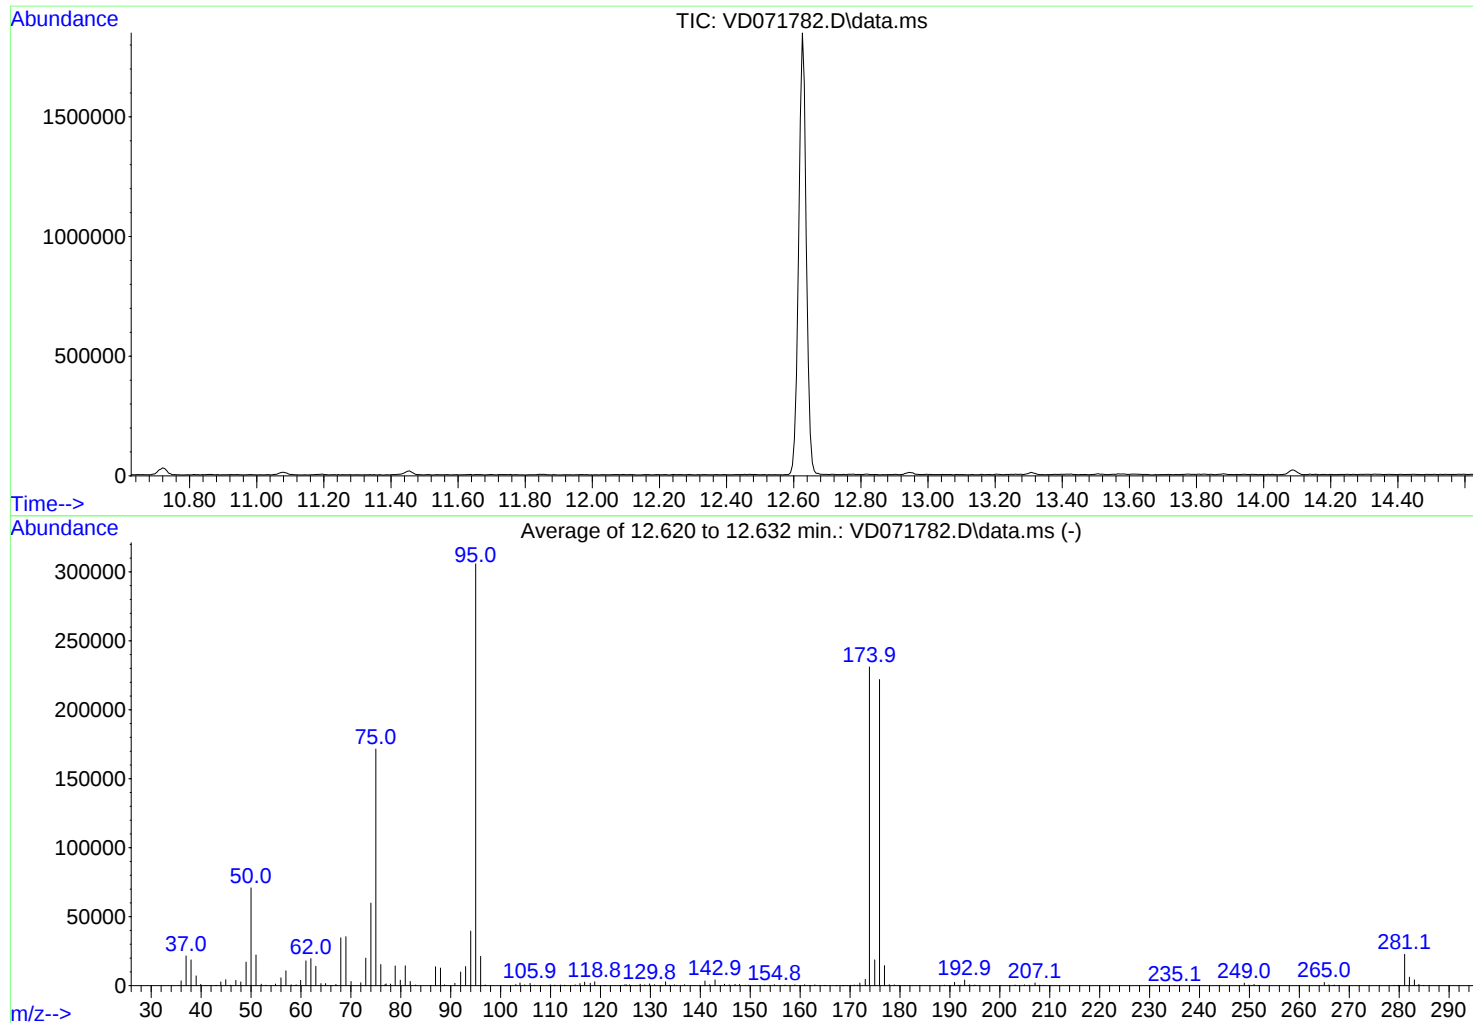

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	70920	PASS
75	95	30	60	56.1	171541	PASS
95	95	100	100	100.0	305835	PASS
96	95	5	9	7.0	21269	PASS
173	174	0.00	2	1.9	4481	PASS
174	95	50	100	75.6	231061	PASS
175	174	5	9	8.1	18630	PASS
176	174	95	101	96.0	221909	PASS
177	176	5	9	6.5	14454	PASS