
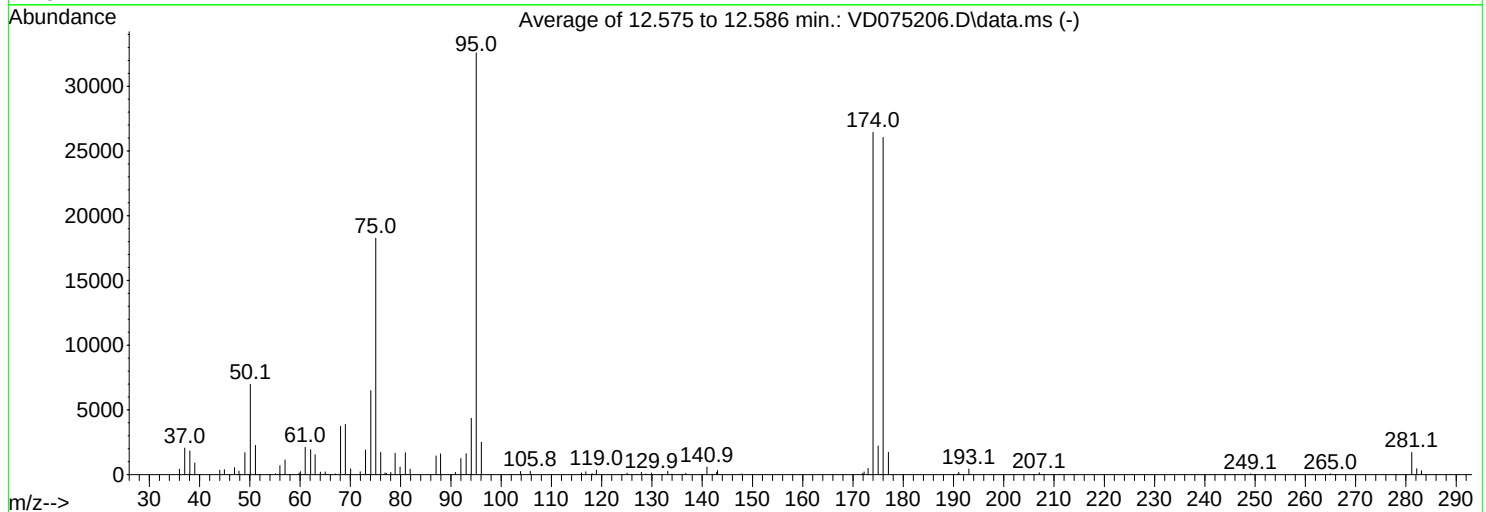


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012623\
Data File : VD075206.D
Acq On : 26 Jan 2023 10:01
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
Title : SW846 8260
Last Update : Thu Jan 19 01:32:27 2023

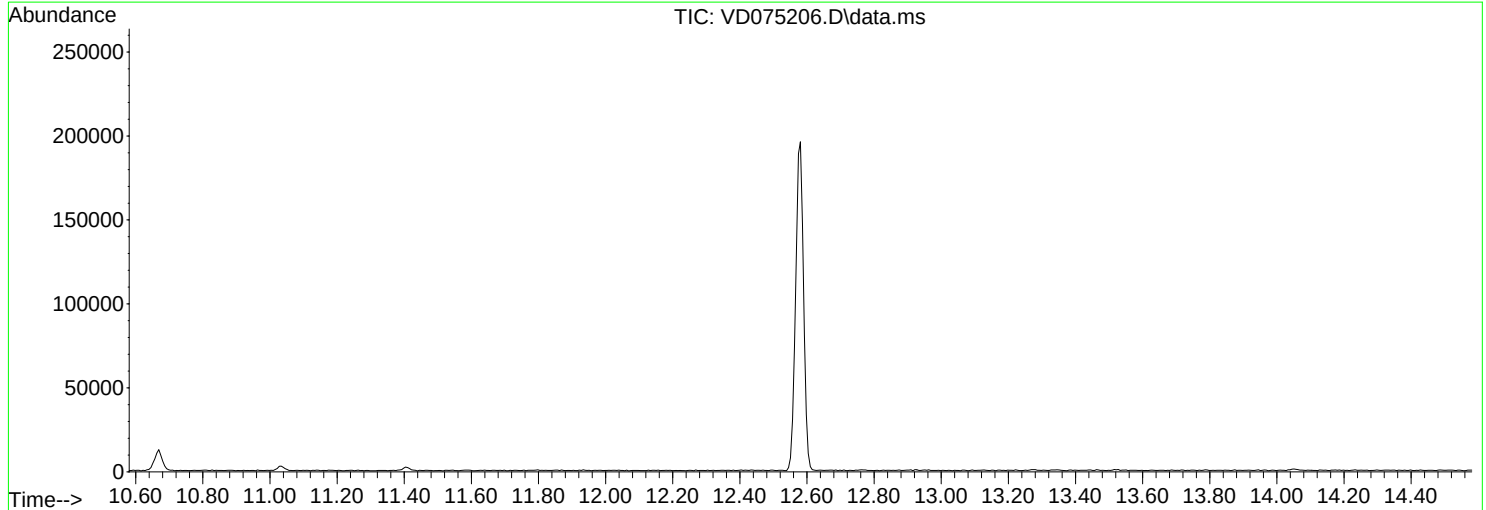

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	6984	PASS
75	95	30	60	56.1	18270	PASS
95	95	100	100	100.0	32579	PASS
96	95	5	9	7.7	2496	PASS
173	174	0.00	2	1.8	478	PASS
174	95	50	100	81.2	26440	PASS
175	174	5	9	8.4	2218	PASS
176	174	95	101	98.5	26048	PASS
177	176	5	9	6.6	1732	PASS