

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD012720\
 Data File : VD064967.D
 Acq On : 27 Jan 2020 16:54
 Operator : VA/SY
 Sample : L1242-11RE
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 20200064-AMENDED-COMP-2RE

Quant Time: Jan 27 22:45:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012320S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 23 13:45:59 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	414824	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	676454	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	623702	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	258891	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	220577	55.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.86%	
35) Dibromofluoromethane	7.92	113	85442	20.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	40.20%	
50) Toluene-d8	10.34	98	811016	49.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.86%	
62) 4-Bromofluorobenzene	12.64	95	254437	50.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.36%	
Target Compounds						
16) Acetone	4.17	43	147870	151.691	ug/l	97
17) Carbon Disulfide	4.40	76	264083	22.222	ug/l	98
25) 2-Butanone	7.22	43	36036	33.522	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD012720\
Data File : VD064967.D
Acq On : 27 Jan 2020 16:54
Operator : VA/SY
Sample : L1242-11RE
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
20200064-AMENDED-COMP-2RE

Quant Time: Jan 27 22:45:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D012320S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 23 13:45:59 2020
Response via : Initial Calibration

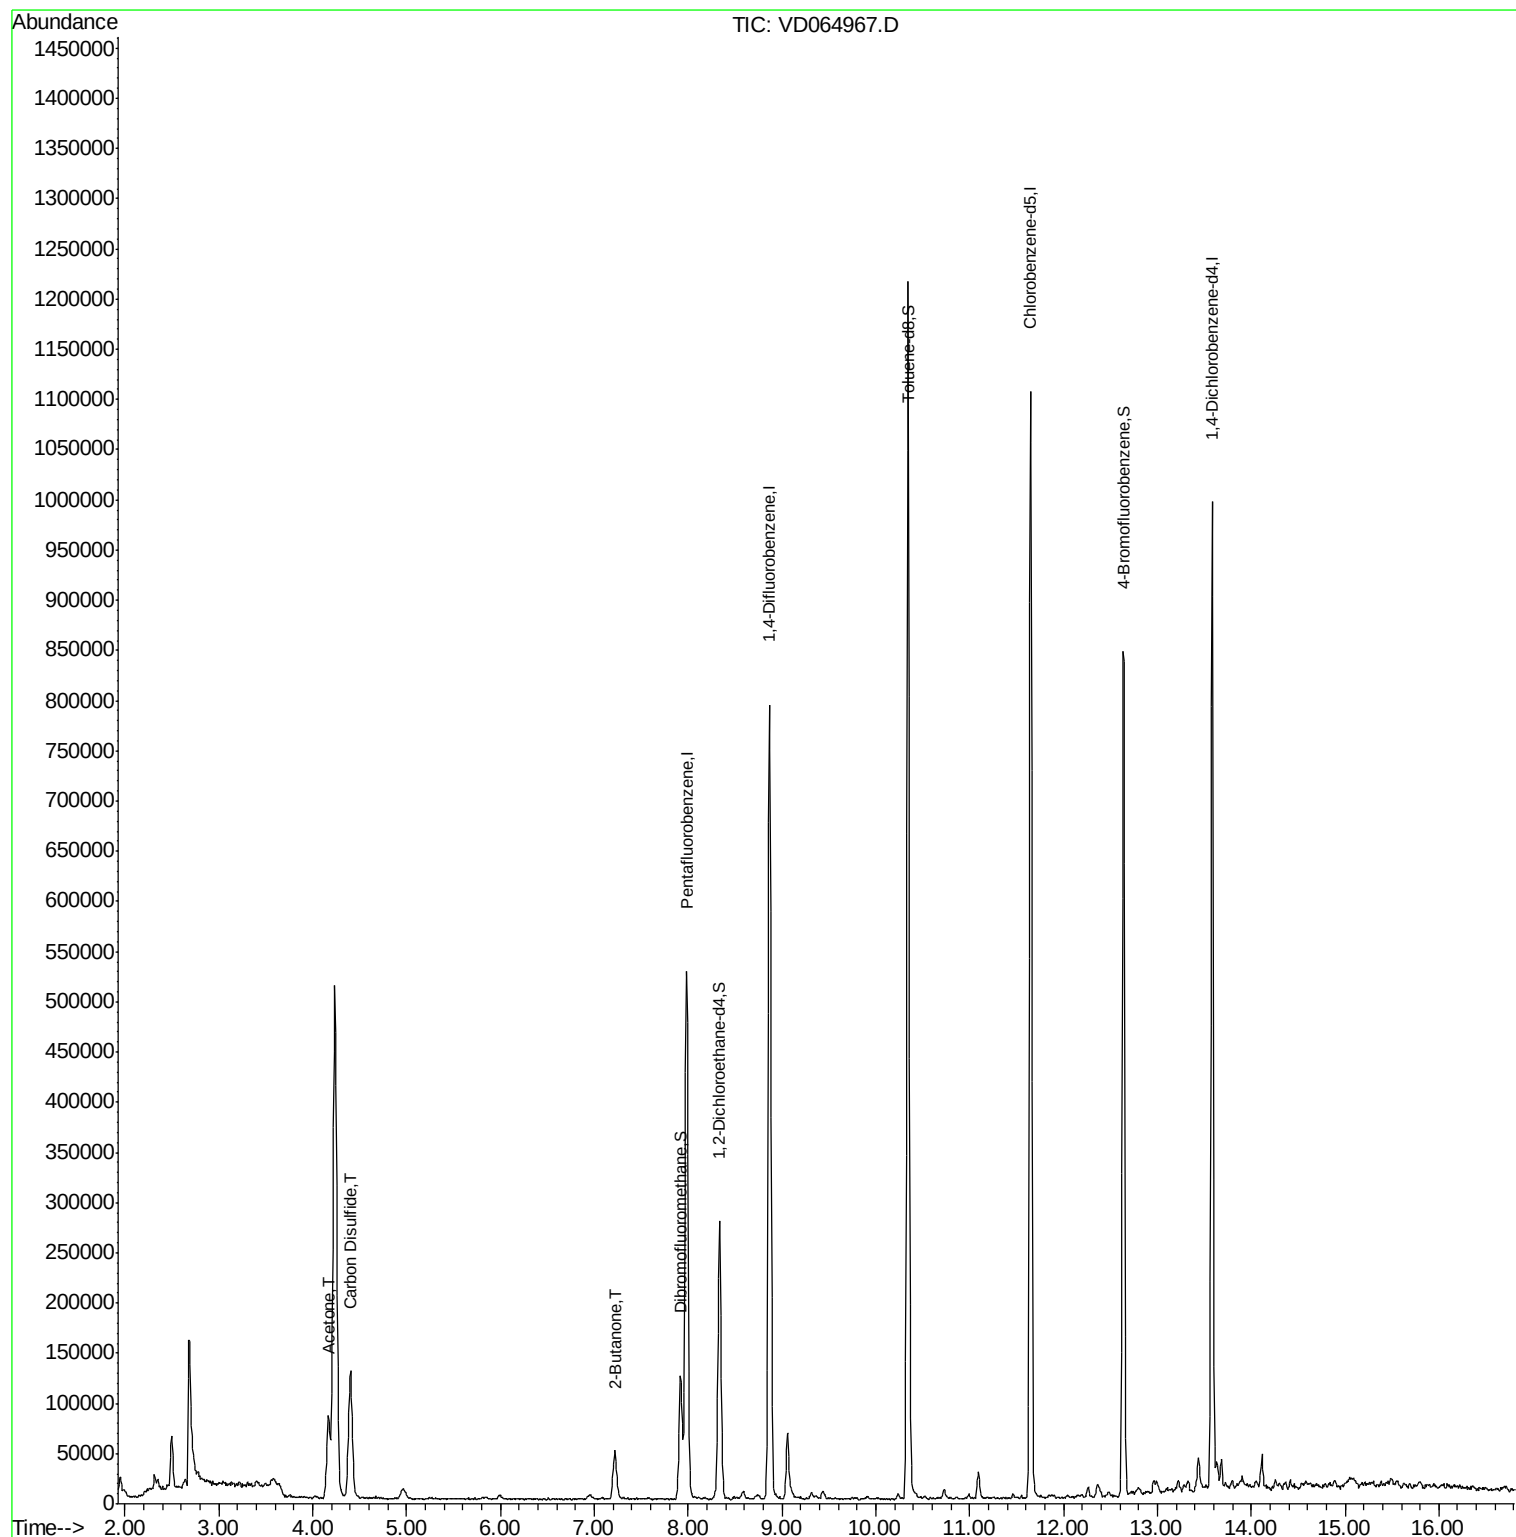

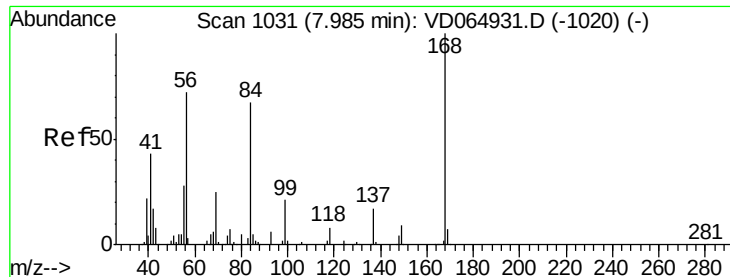

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VD064967.D

Acq: 27 Jan 2020 16:54

Instrument :

MSVOA_D

ClientSampleId :


20200064-AMENDED-COMP-2RE

Tot Ion:168 Resp: 414824

Ion Ratio Lower Upper

168 100

99 51.2 43.3 64.9

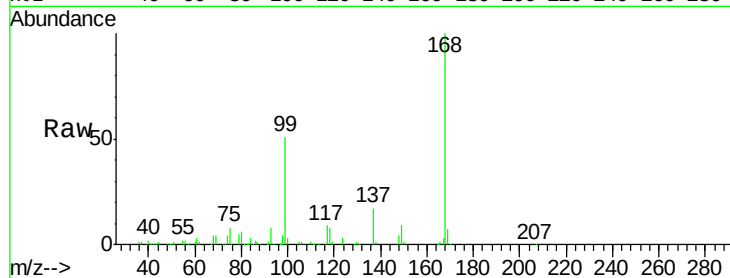

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

200000



150000

100000

50000

0

Time-->

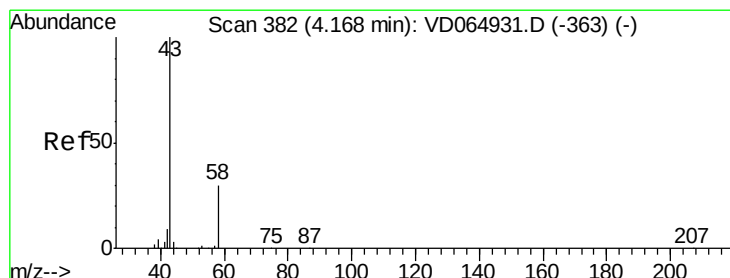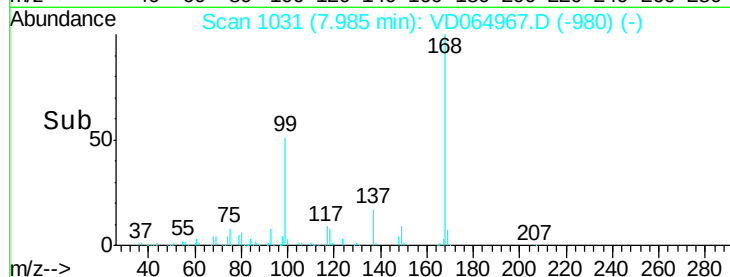

#16

Acetone

Concen: 151.691 ug/l

RT: 4.17 min Scan# 382

Delta R.T. 0.00 min

Lab File: VD064967.D


Acq: 27 Jan 2020 16:54

Tgt Ion: 43 Resp: 147870

Ion Ratio Lower Upper

43 100

58 28.1 23.8 35.8

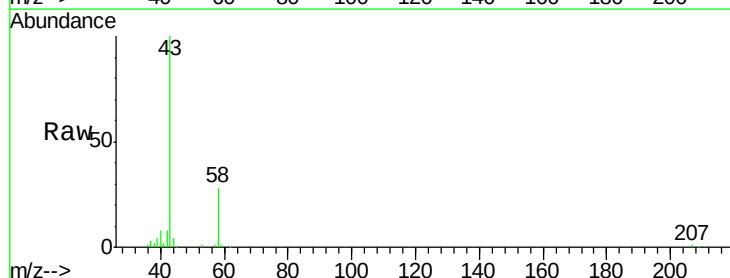

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC

4.17

60000

50000

40000


30000


20000

10000

0

Time-->

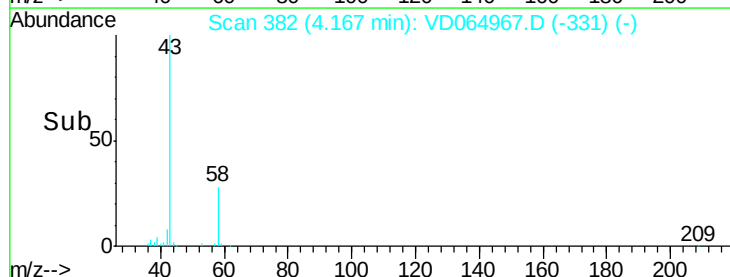

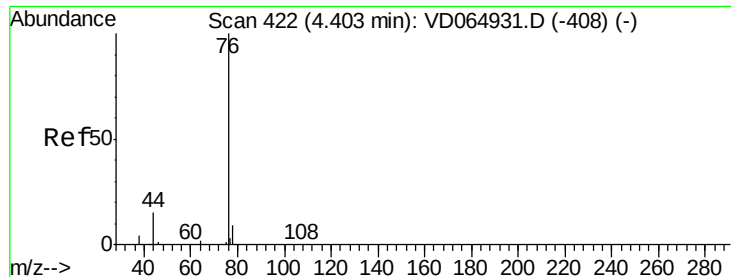

#17

Carbon Disulfide

Concen: 22.222 ug/l

RT: 4.40 min Scan# 422

Delta R.T. -0.00 min

Lab File: VD064967.D

Acq: 27 Jan 2020 16:54

Instrument :

MSVOA_D

ClientSampleId :


20200064-AMENDED-COMP-2RE

Tot Ion: 76 Resp: 264083

Ion Ratio Lower Upper

76 100

78 9.5 7.1 10.7

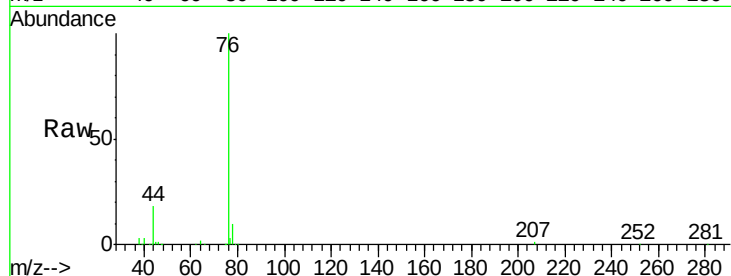

Abundance Ion 75.90 (75.60 to 76.60): VDC

Ion 77.90 (77.60 to 78.60): VDC

4.40

100000

80000



60000

40000

20000

0

Time-->

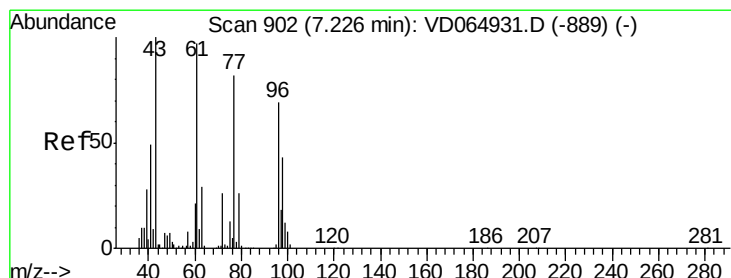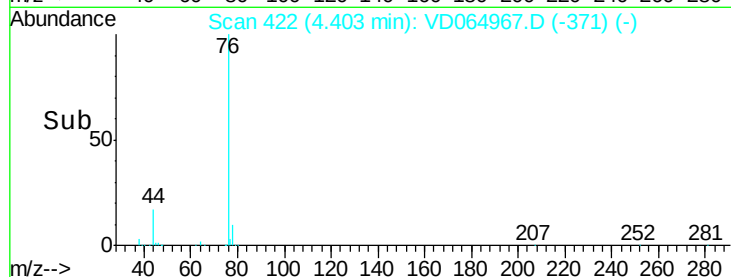

#25

2-Butanone

Concen: 33.522 ug/l

RT: 7.22 min Scan# 901

Delta R.T. -0.01 min

Lab File: VD064967.D


Acq: 27 Jan 2020 16:54

Tgt Ion: 43 Resp: 36036

Ion Ratio Lower Upper

43 100

72 27.0 20.6 31.0

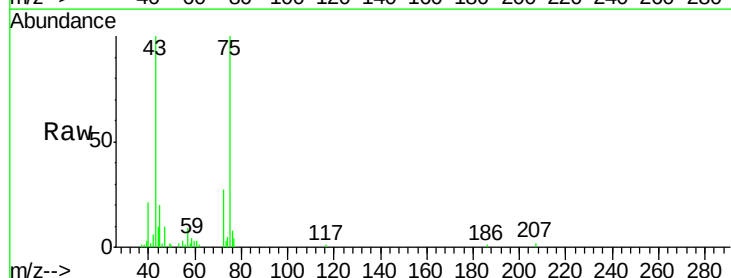

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 72.00 (71.70 to 72.70): VDC

7.22


15000


10000

5000

0

Time-->




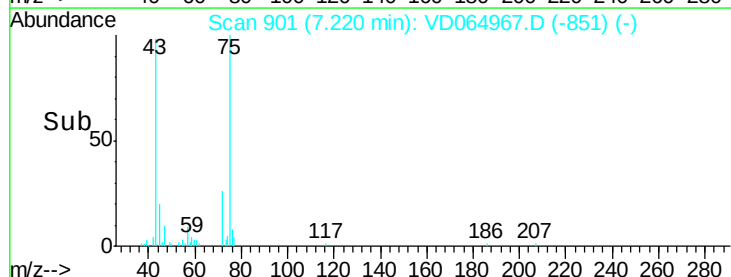


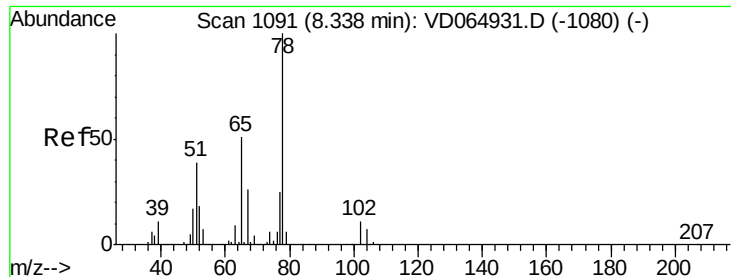

#33
 1,2-Dichloroethane-d4
 Concen: 55.434 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. -0.01 min
 Lab File: VD064967.D
 Acq: 27 Jan 2020 16:54




Instrument :
 MSVOA_D
 ClientSampleId :
 20200064-AMENDED-COMP-2RE


Tot Ion: 65 Resp: 220577
 Ion Ratio Lower Upper
 65 100
 67 50.2 0.0 103.6

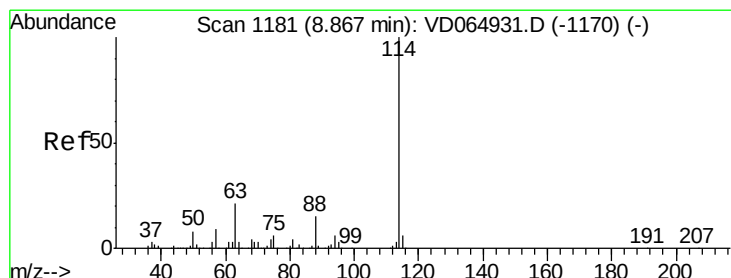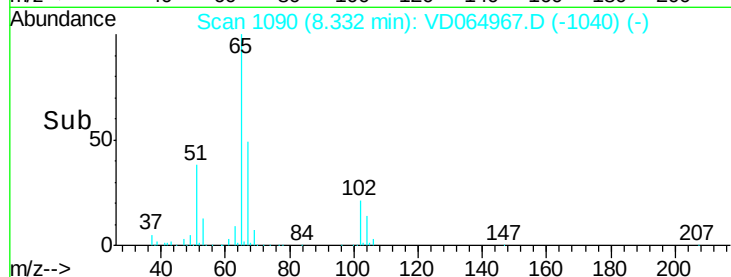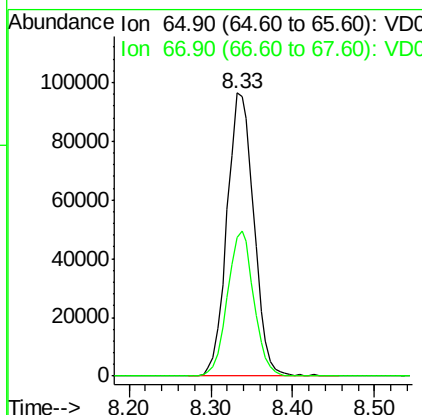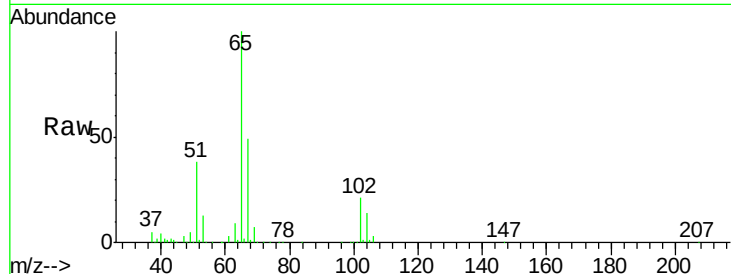

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. -0.00 min
 Lab File: VD064967.D
 Acq: 27 Jan 2020 16:54

Tgt Ion: 114 Resp: 676454
 Ion Ratio Lower Upper
 114 100
 63 20.9 0.0 42.0
 88 15.4 0.0 29.4

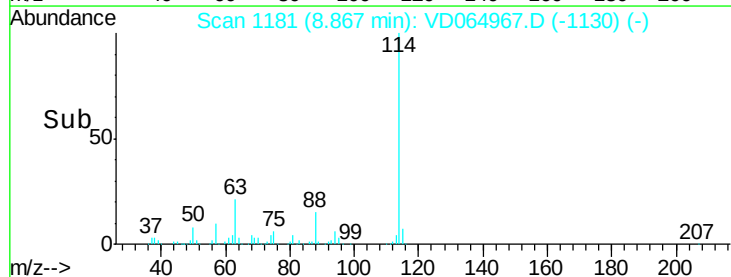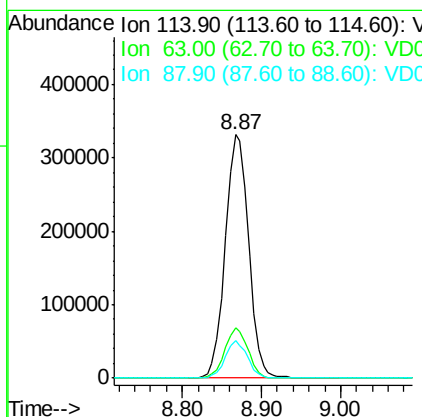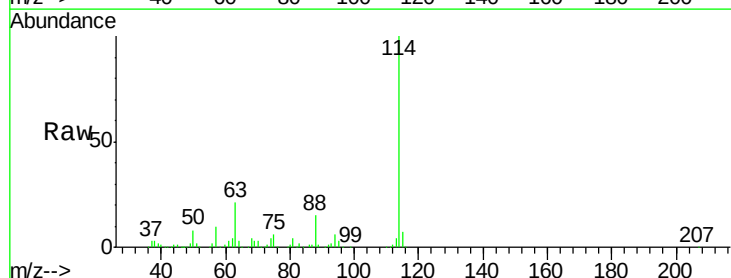

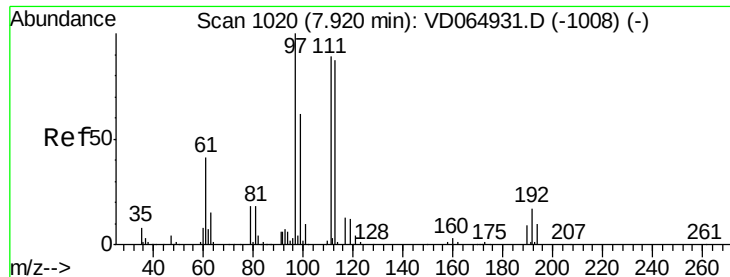

#35

Dibromofluoromethane

Concen: 20.100 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. -0.00 min

Lab File: VD064967.D

Acq: 27 Jan 2020 16:54

Instrument :

MSVOA_D

ClientSampleId :

20200064-AMENDED-COMP-2RE


Tot Ion:113 Resp: 85442

Ion Ratio Lower Upper

113 100

111 104.2 82.4 123.6




192 22.1 16.9 25.3

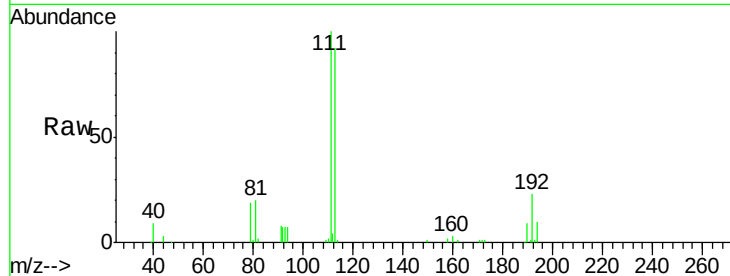

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

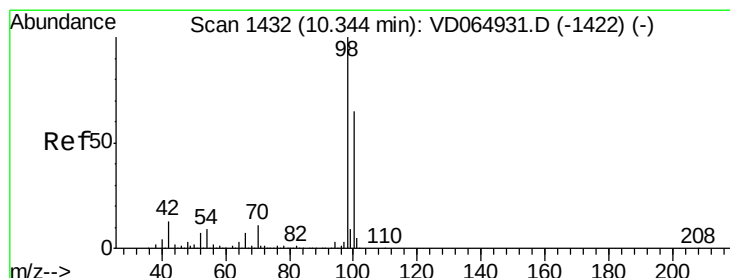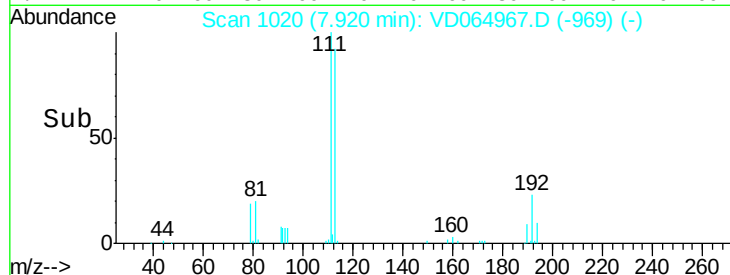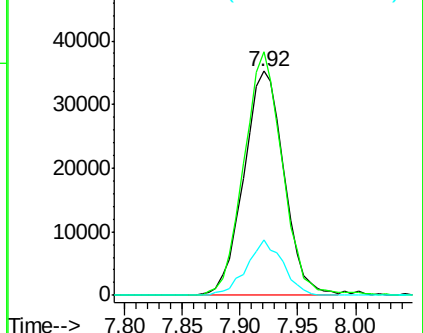

#50

Toluene-d8

Concen: 49.431 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. -0.00 min

Lab File: VD064967.D


Acq: 27 Jan 2020 16:54

Tgt Ion: 98 Resp: 811016

Ion Ratio Lower Upper



98 100


100 64.6 52.3 78.5

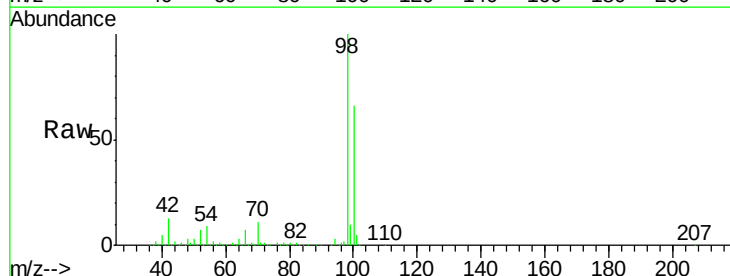

Abundance Ion 98.00 (97.70 to 98.70): V

Ion 100.00 (99.70 to 100.70): V

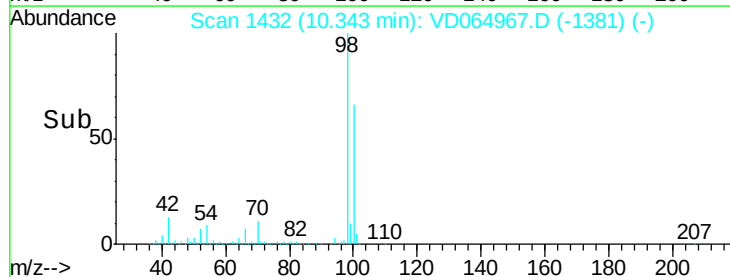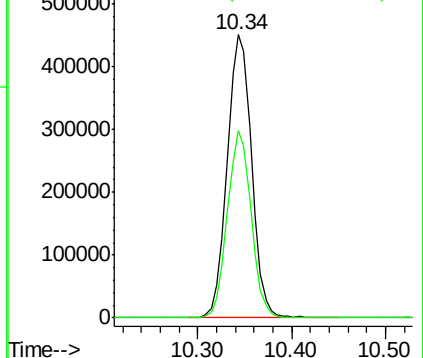

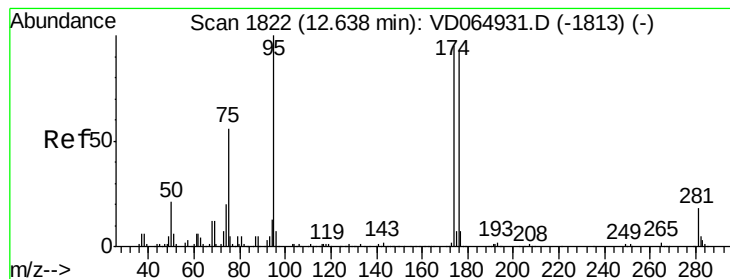

#62

4-Bromofluorobenzene

Concen: 50.676 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. -0.00 min

Lab File: VD064967.D

Acq: 27 Jan 2020 16:54

Instrument :

MSVOA_D

ClientSampleId :

20200064-AMENDED-COMP-2RE


Tot Ion: 95 Resp: 254437

Ion Ratio Lower Upper

95 100

174 93.2 0.0 186.8




176 89.9 0.0 183.4

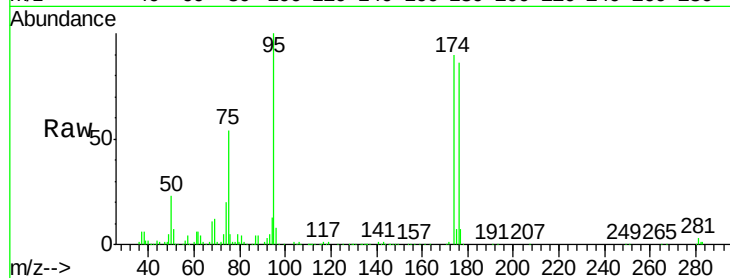

Abundance Ion 94.90 (94.60 to 95.60): V

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

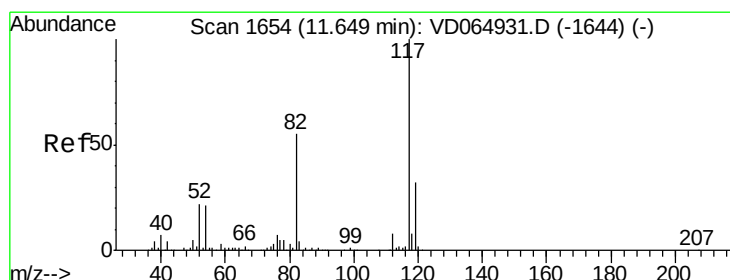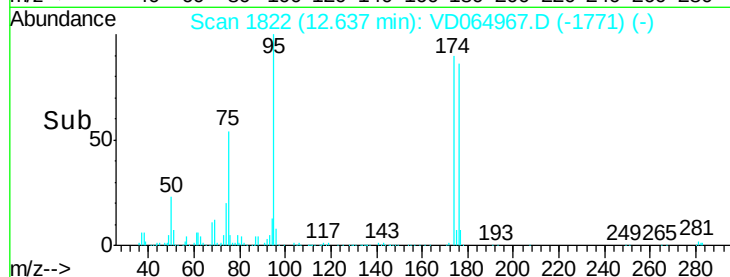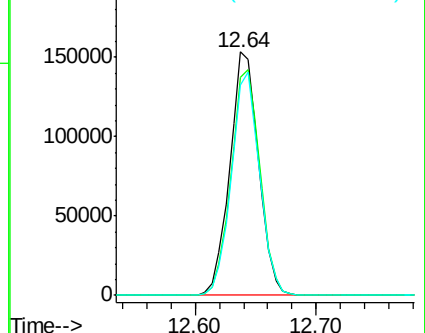

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.65 min Scan# 1654

Delta R.T. -0.00 min

Lab File: VD064967.D

Acq: 27 Jan 2020 16:54


Tgt Ion: 117 Resp: 623702

Ion Ratio Lower Upper

117 100

82 54.8 43.6 65.4



119 33.0 25.2 37.8

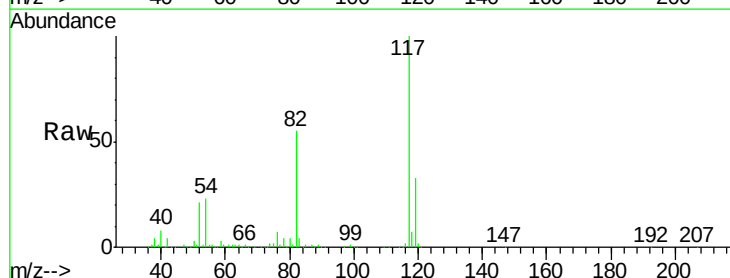


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

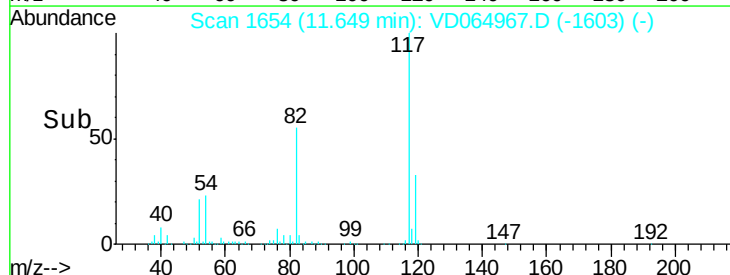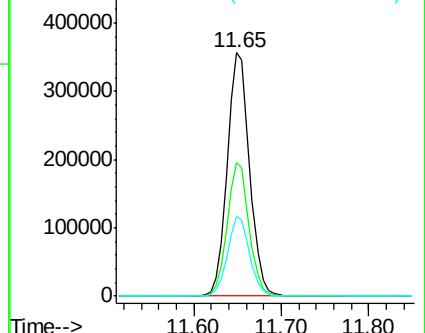

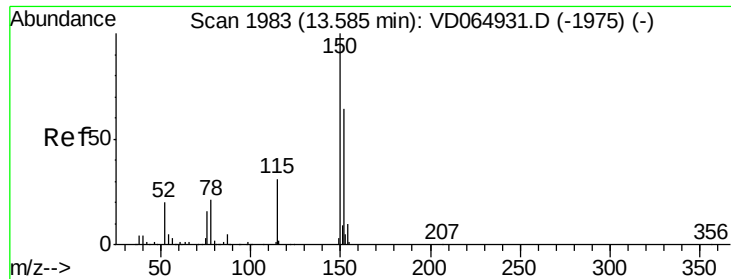

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.58 min Scan# 1983
 Delta R.T. -0.00 min
 Lab File: VD064967.D
 Acq: 27 Jan 2020 16:54

Instrument :
 MSVOA_D
 ClientSampleId :
 20200064-AMENDED-COMP-2RE

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.5	28.1	84.4
150	156.7	0.0	350.4

