


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD012720\
 Data File : VD064956.D
 Acq On : 27 Jan 2020 09:54
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012320S.M
 Title : SW846 8260
 Last Update : Thu Jan 23 13:45:59 2020

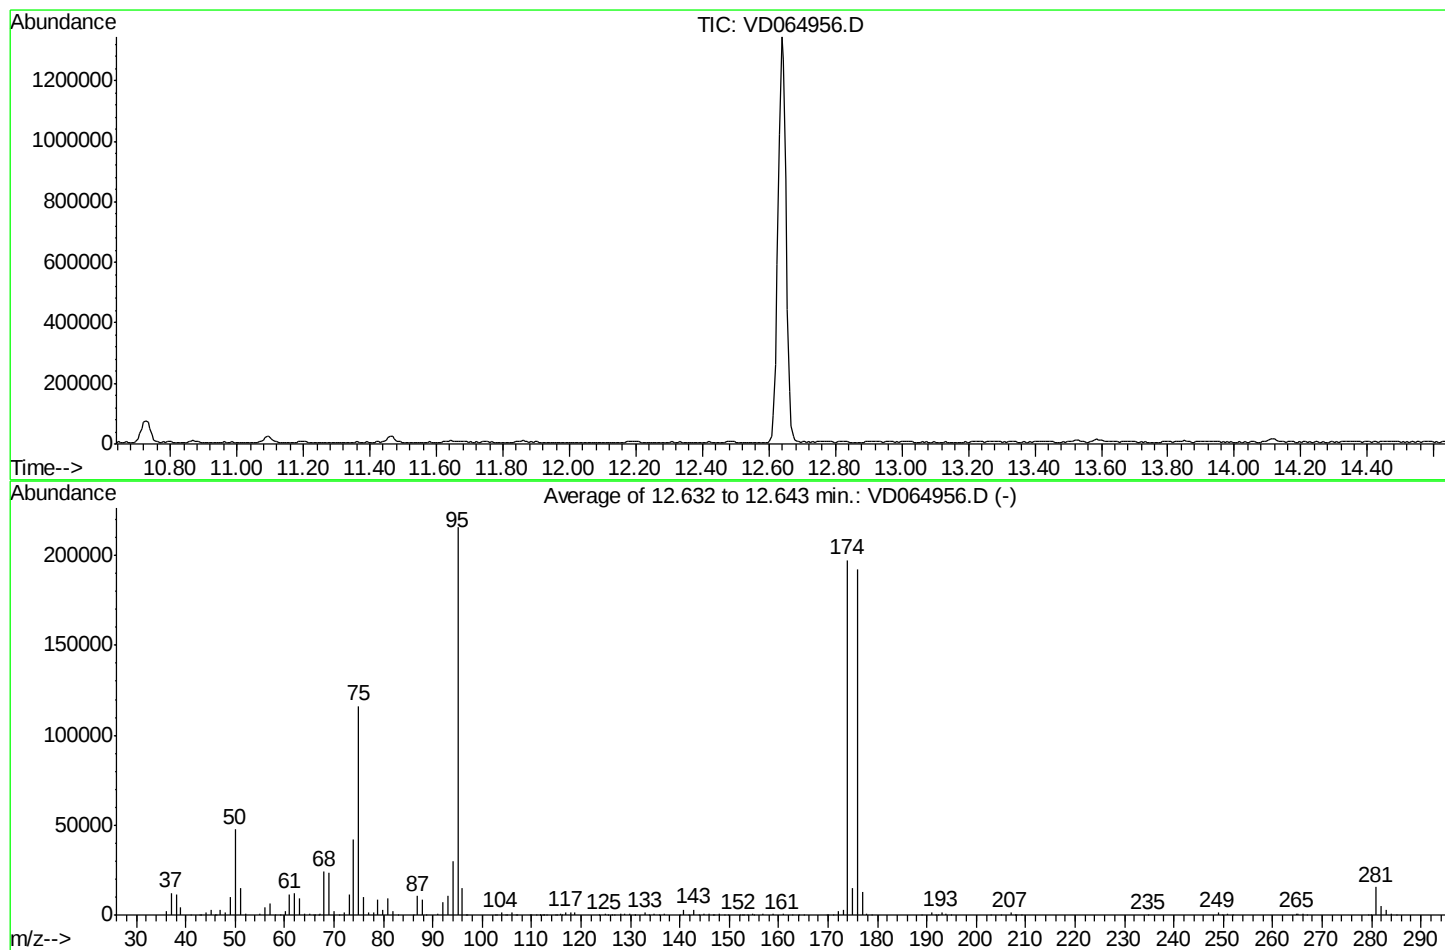

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	47421	PASS
75	95	30	60	53.8	116120	PASS
95	95	100	100	100.0	215701	PASS
96	95	5	9	7.0	15012	PASS
173	174	0.00	2	1.4	2828	PASS
174	95	50	100	91.6	197525	PASS
175	174	5	9	7.7	15168	PASS
176	174	95	101	97.4	192448	PASS
177	176	5	9	6.7	12936	PASS