


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD012819\
 Data File : VD060790.D
 Acq On : 28 Jan 2019 12:57
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012819S.M
 Title : SW846 8260
 Last Update : Tue Jan 29 13:53:55 2019

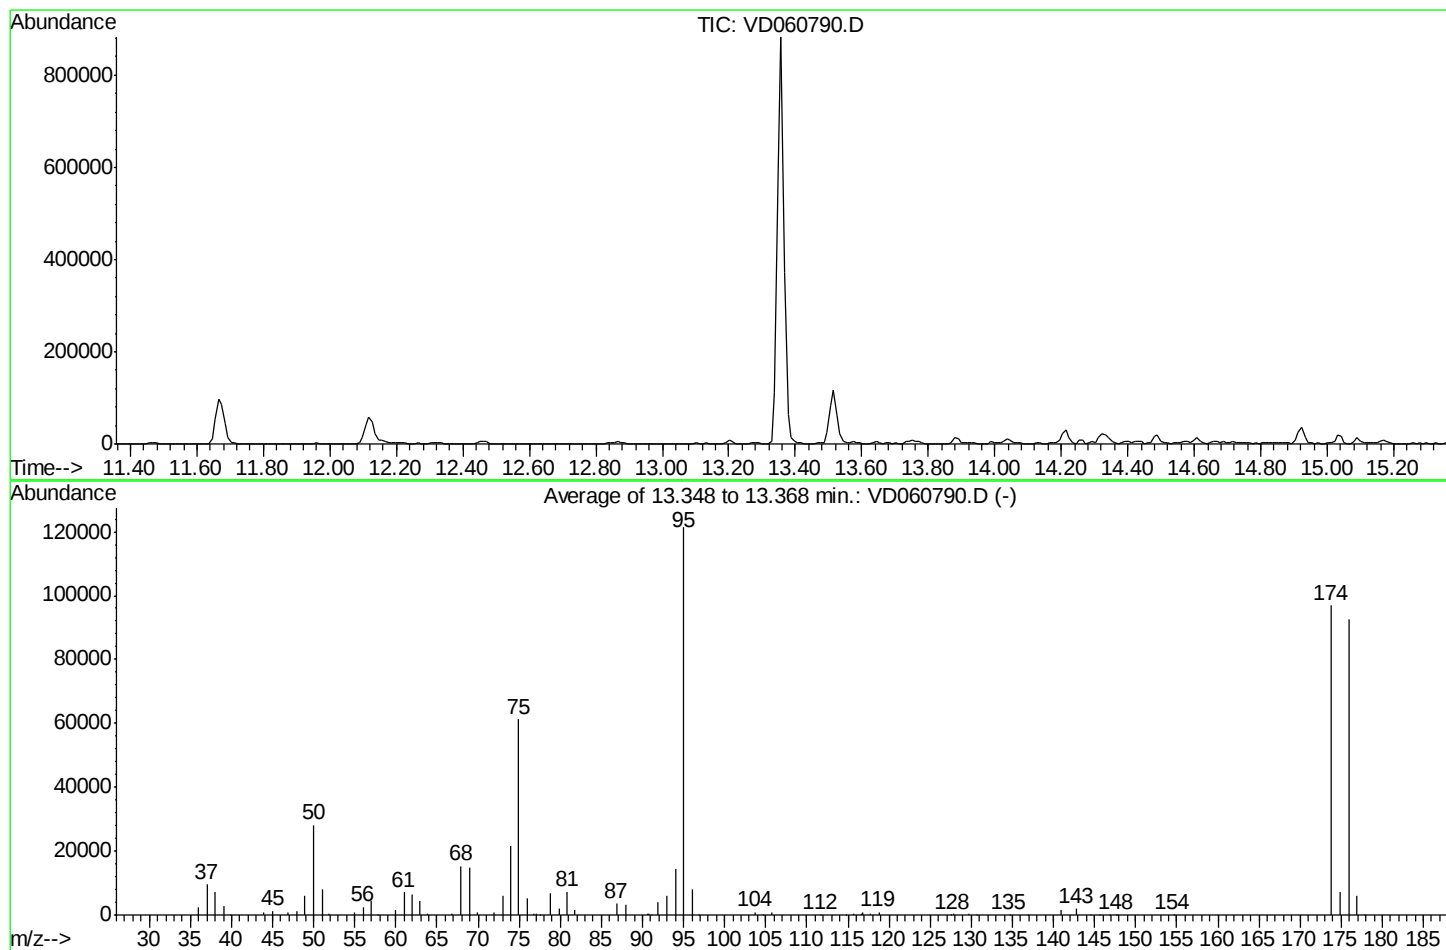

AutoFind: Scans 1252, 1253, 1254; Background Corrected with Scan 1247

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	28154	PASS
75	95	30	60	50.5	61306	PASS
95	95	100	100	100.0	121378	PASS
96	95	5	9	6.8	8198	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.9	96954	PASS
175	174	5	9	7.4	7137	PASS
176	174	95	101	95.6	92648	PASS
177	176	5	9	6.5	6038	PASS