


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD012820\
Data File : VD064972.D
Acq On : 28 Jan 2020 09:31
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012320S.M
Title : SW846 8260
Last Update : Thu Jan 23 13:45:59 2020

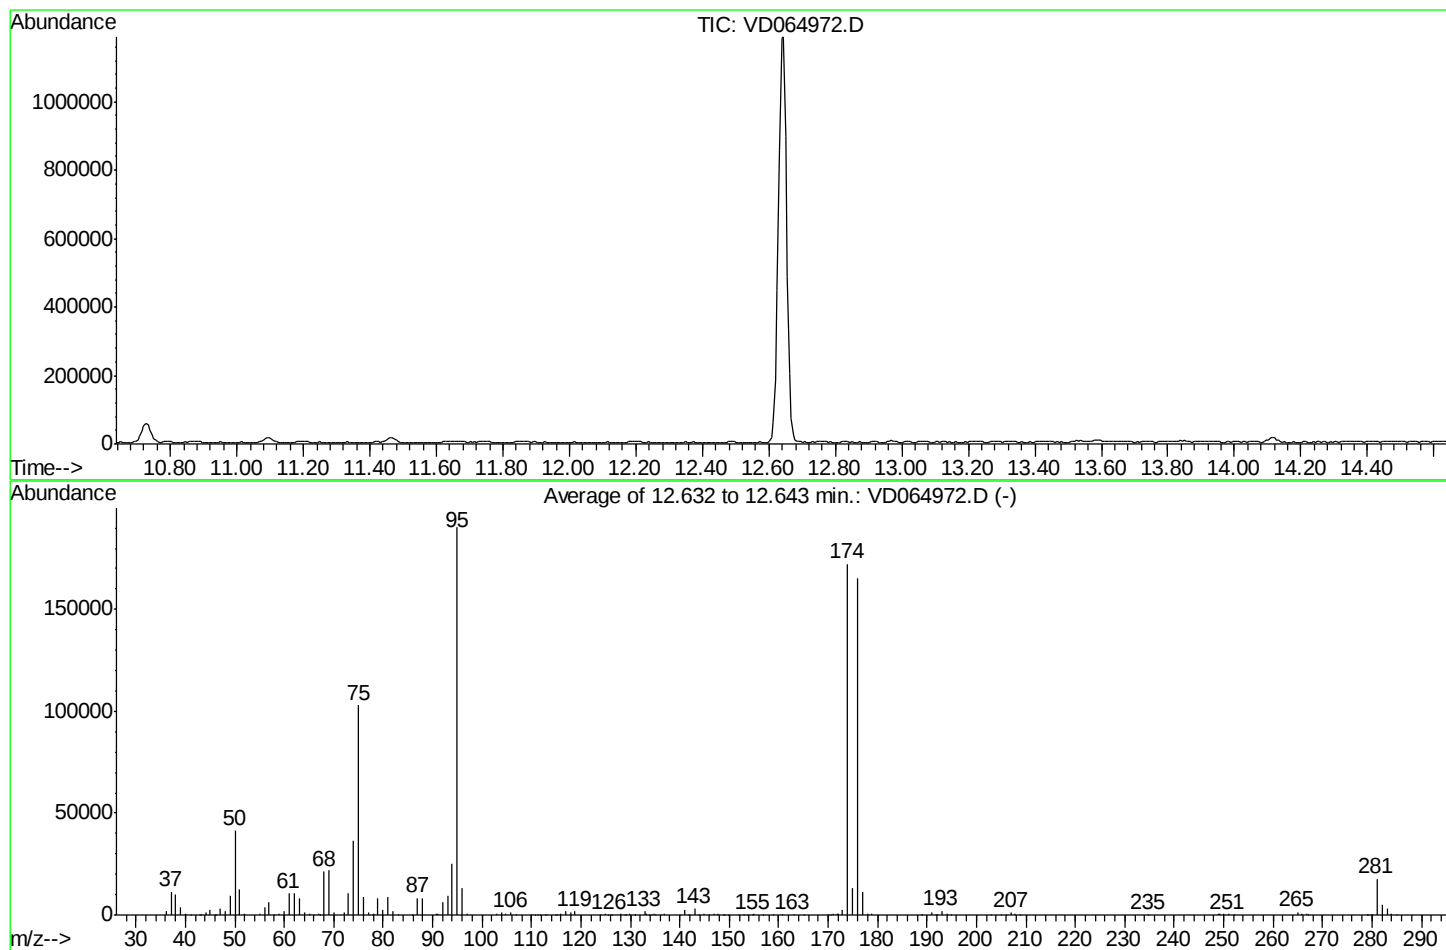

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	41464	PASS
75	95	30	60	54.0	102765	PASS
95	95	100	100	100.0	190293	PASS
96	95	5	9	7.1	13535	PASS
173	174	0.00	2	1.6	2807	PASS
174	95	50	100	90.5	172234	PASS
175	174	5	9	7.7	13282	PASS
176	174	95	101	95.9	165189	PASS
177	176	5	9	6.7	11139	PASS