


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD012920\
 Data File : VD064987.D
 Acq On : 29 Jan 2020 10:09
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012320S.M
 Title : SW846 8260
 Last Update : Thu Jan 23 13:45:59 2020

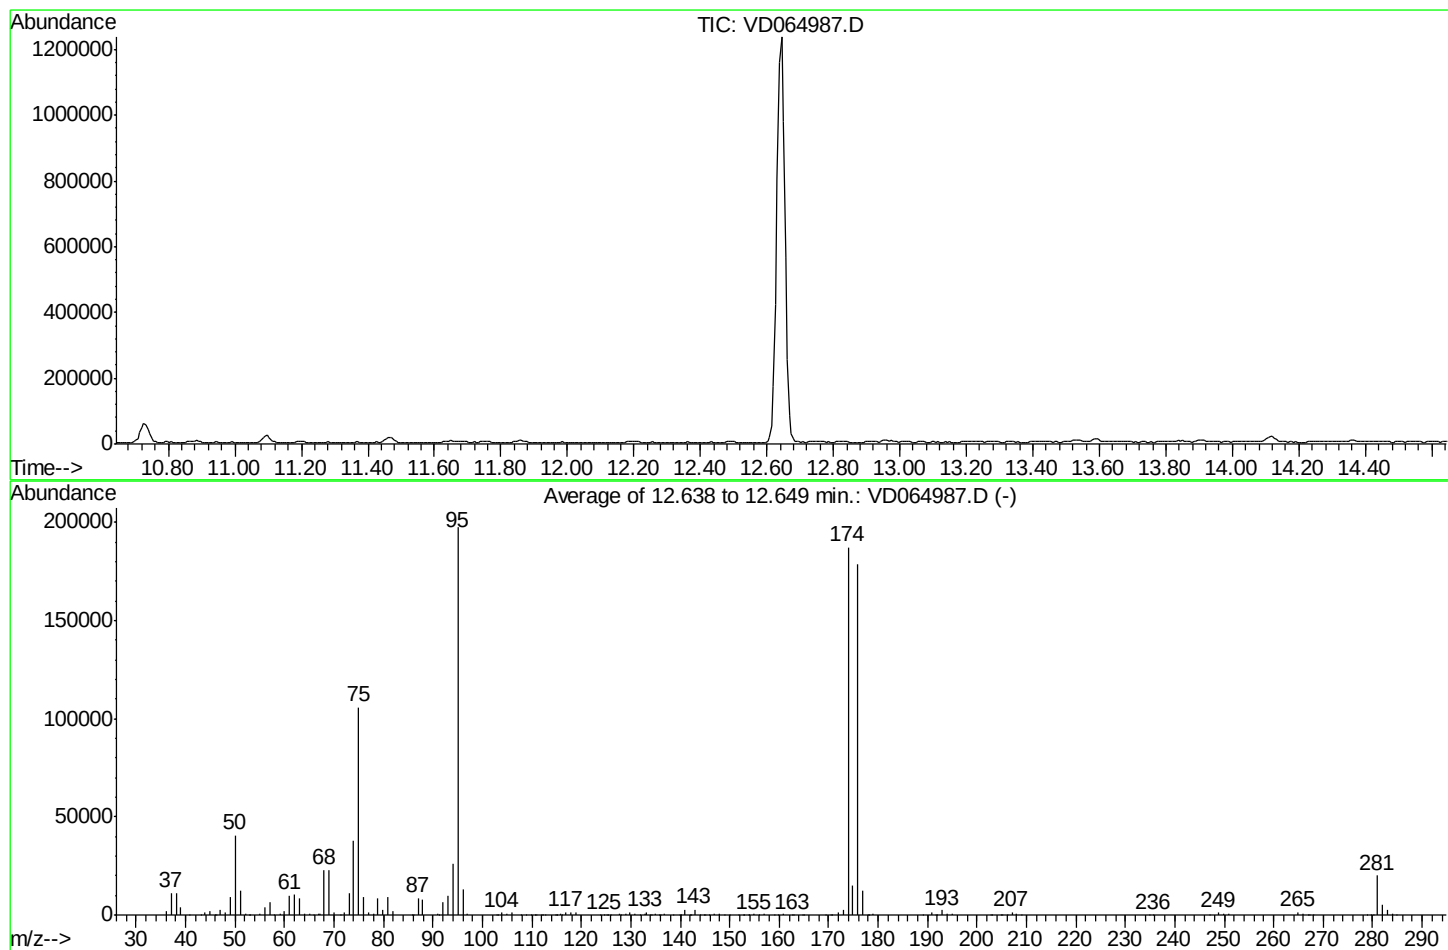

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	40584	PASS
75	95	30	60	53.5	105696	PASS
95	95	100	100	100.0	197418	PASS
96	95	5	9	6.6	13091	PASS
173	174	0.00	2	1.5	2765	PASS
174	95	50	100	94.8	187221	PASS
175	174	5	9	8.1	15226	PASS
176	174	95	101	95.3	178474	PASS
177	176	5	9	7.0	12541	PASS