
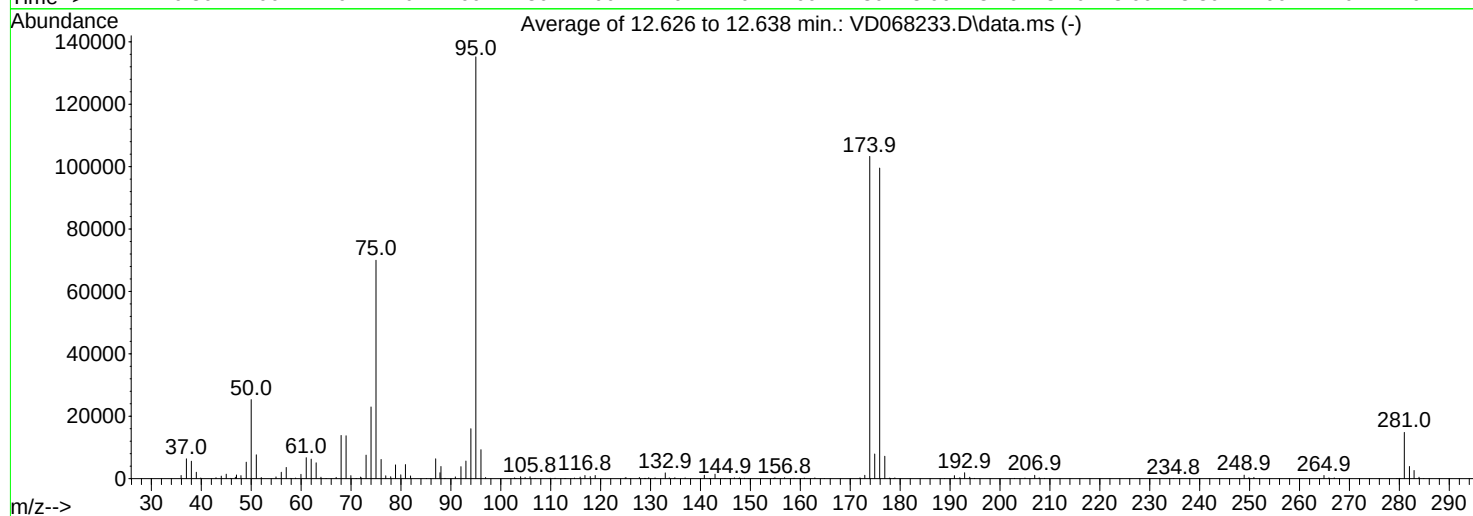


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012921\
 Data File : VD068233.D
 Acq On : 29 Jan 2021 10:42
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
 Title : SW846 8260
 Last Update : Tue Jan 19 13:19:08 2021

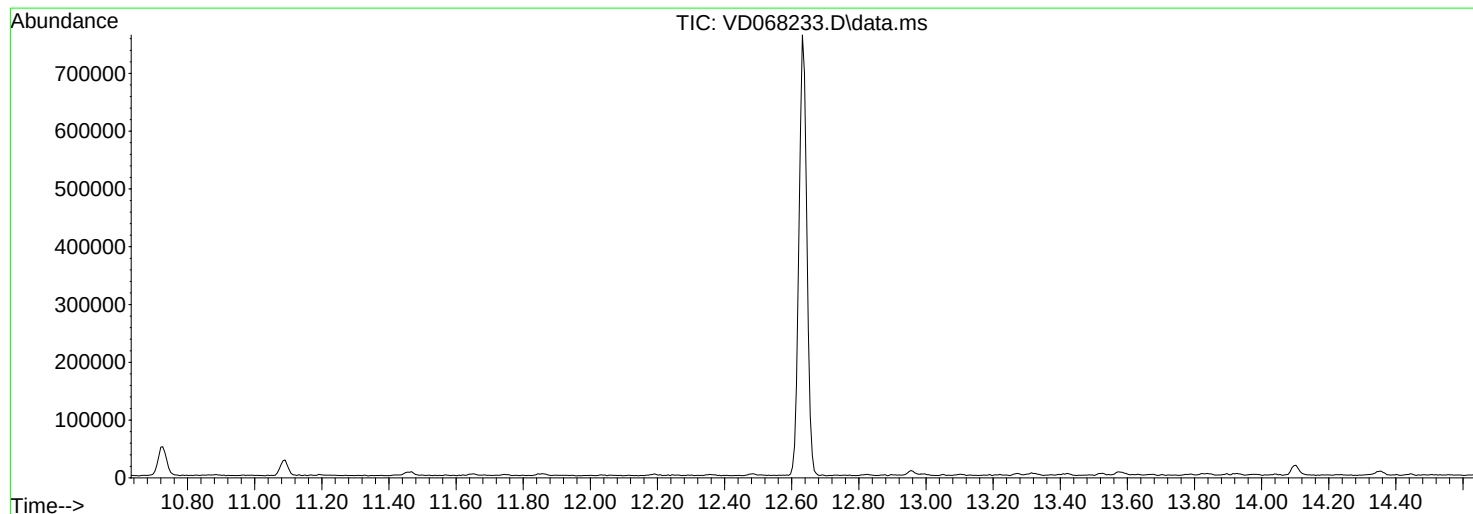

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	25357	PASS
75	95	30	60	51.8	70029	PASS
95	95	100	100	100.0	135208	PASS
96	95	5	9	6.9	9291	PASS
173	174	0.00	2	1.1	1095	PASS
174	95	50	100	76.4	103283	PASS
175	174	5	9	7.7	7908	PASS
176	174	95	101	96.4	99541	PASS
177	176	5	9	7.2	7178	PASS