
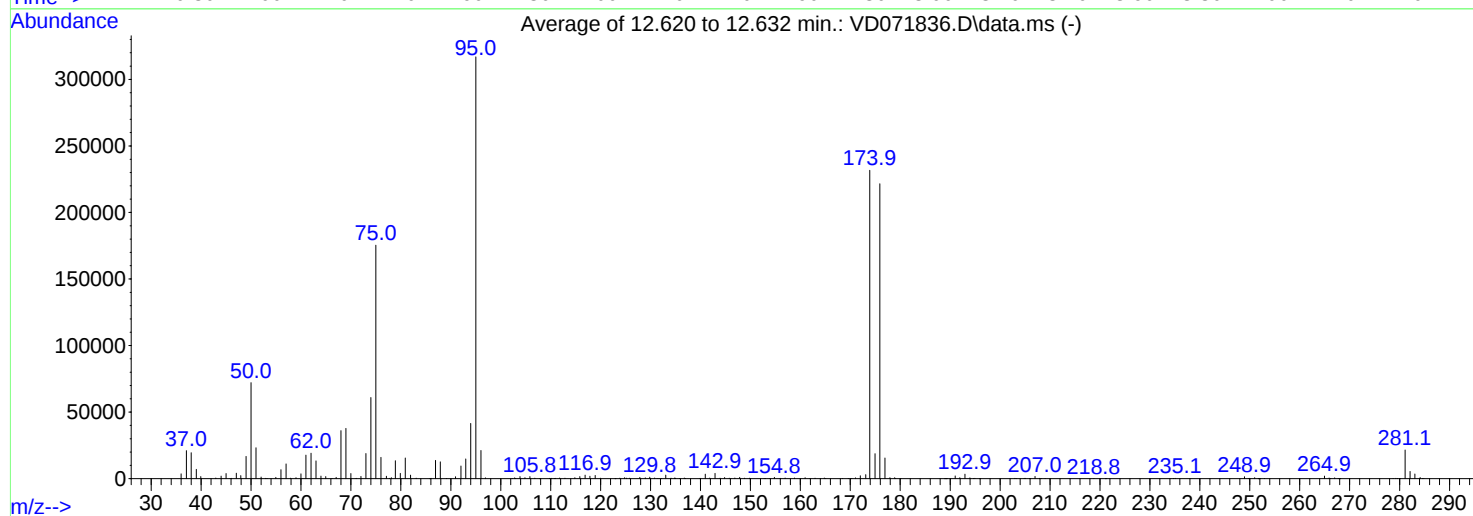


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD013122\  
 Data File : VD071836.D  
 Acq On : 31 Jan 2022 10:00  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D012622S.M  
 Title : SW846 8260  
 Last Update : Thu Jan 27 06:04:38 2022

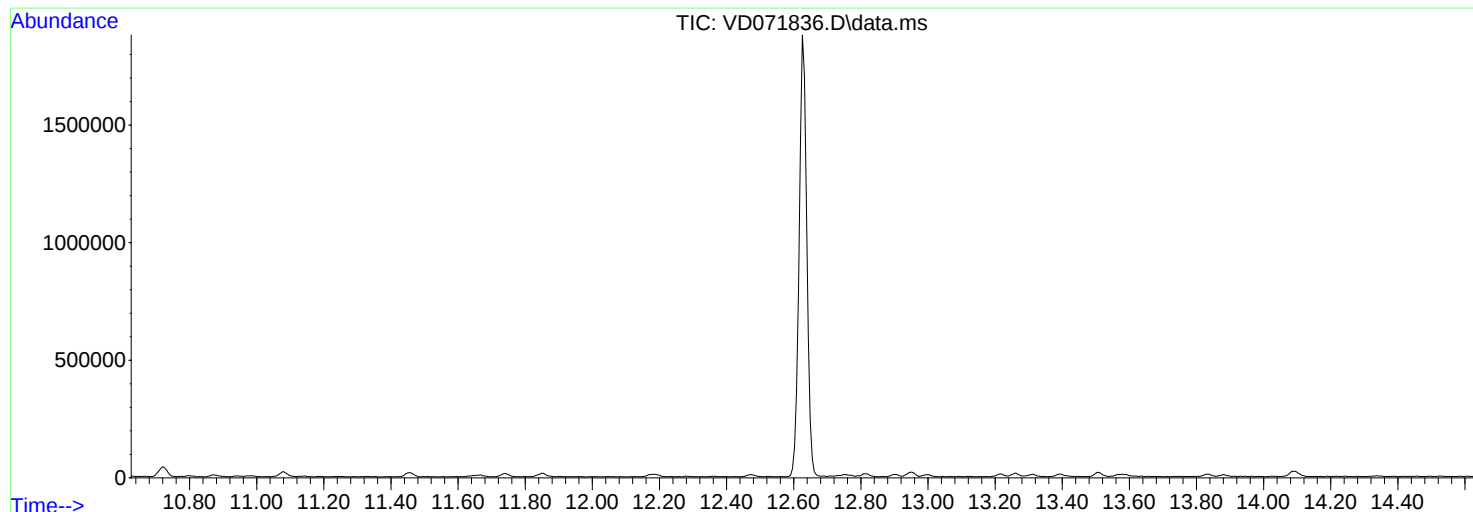

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 22.8         | 72107      | PASS                |
| 75             | 95              | 30              | 60              | 55.3         | 175424     | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 316949     | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 21147      | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 2971       | PASS                |
| 174            | 95              | 50              | 100             | 73.1         | 231680     | PASS                |
| 175            | 174             | 5               | 9               | 8.1          | 18719      | PASS                |
| 176            | 174             | 95              | 101             | 95.7         | 221611     | PASS                |
| 177            | 176             | 5               | 9               | 7.0          | 15521      | PASS                |