


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD071860.D
Data File : VD071860.D
Acq On : 01 Feb 2022 08:46
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Title : SW846 8260
Last Update : Thu Jan 27 06:04:38 2022

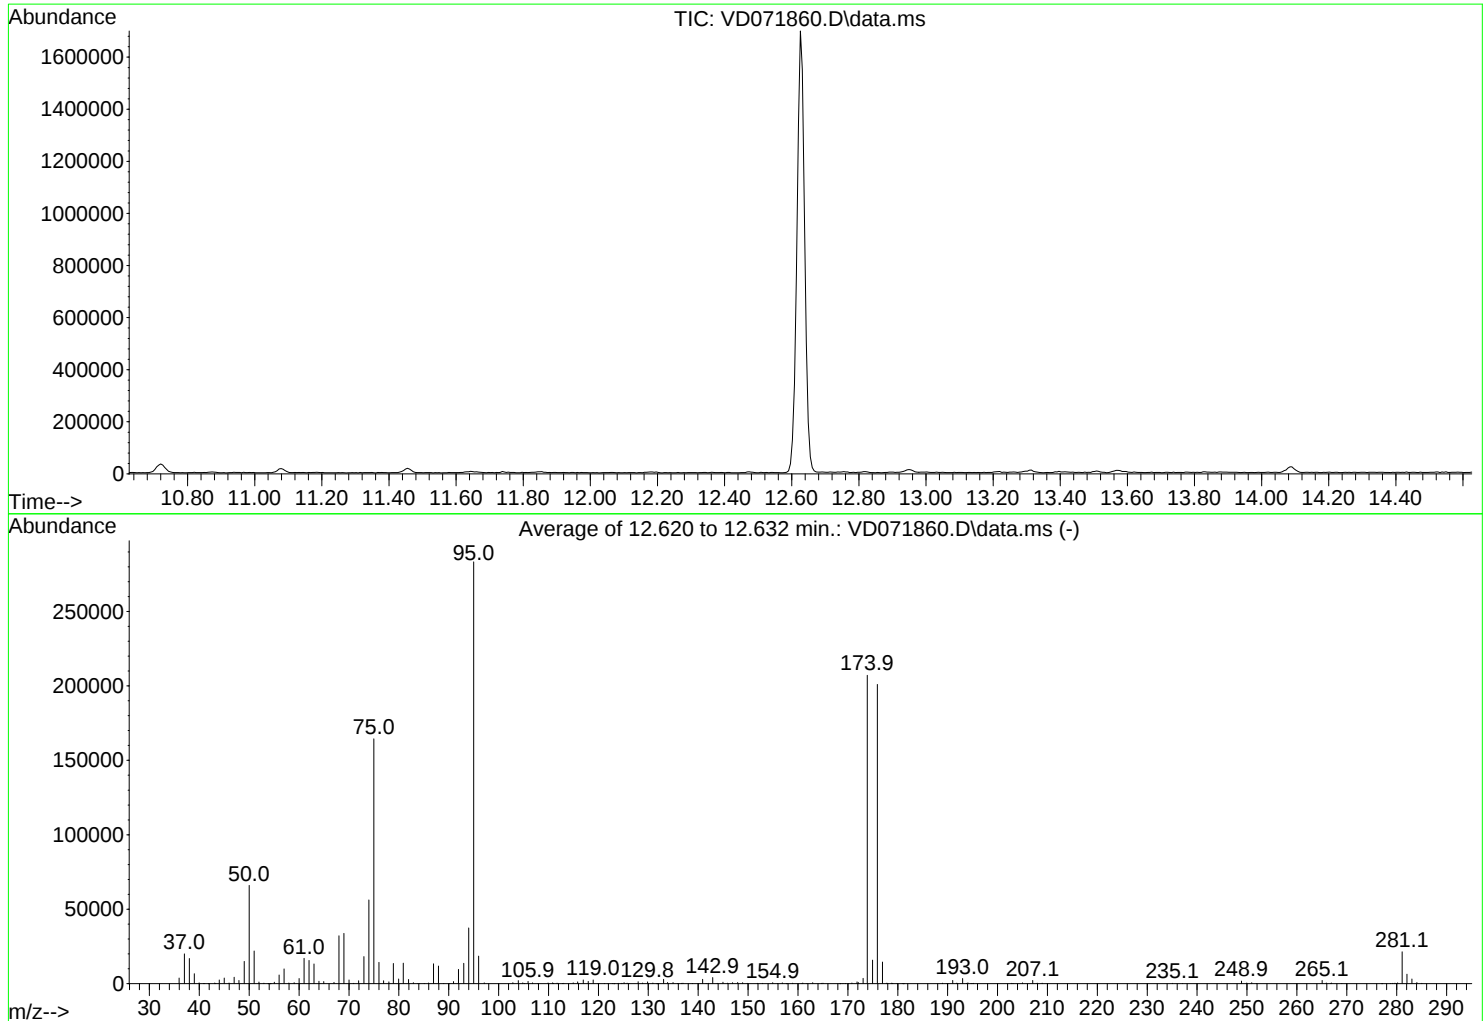

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.3	65987	PASS
75	95	30	60	58.0	164480	PASS
95	95	100	100	100.0	283349	PASS
96	95	5	9	6.5	18454	PASS
173	174	0.00	2	1.7	3536	PASS
174	95	50	100	73.1	207125	PASS
175	174	5	9	7.6	15821	PASS
176	174	95	101	97.0	201003	PASS
177	176	5	9	7.2	14572	PASS