


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD020320\
 Data File : VD065043.D
 Acq On : 03 Feb 2020 09:32
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012320S.M
 Title : SW846 8260
 Last Update : Thu Jan 23 13:45:59 2020

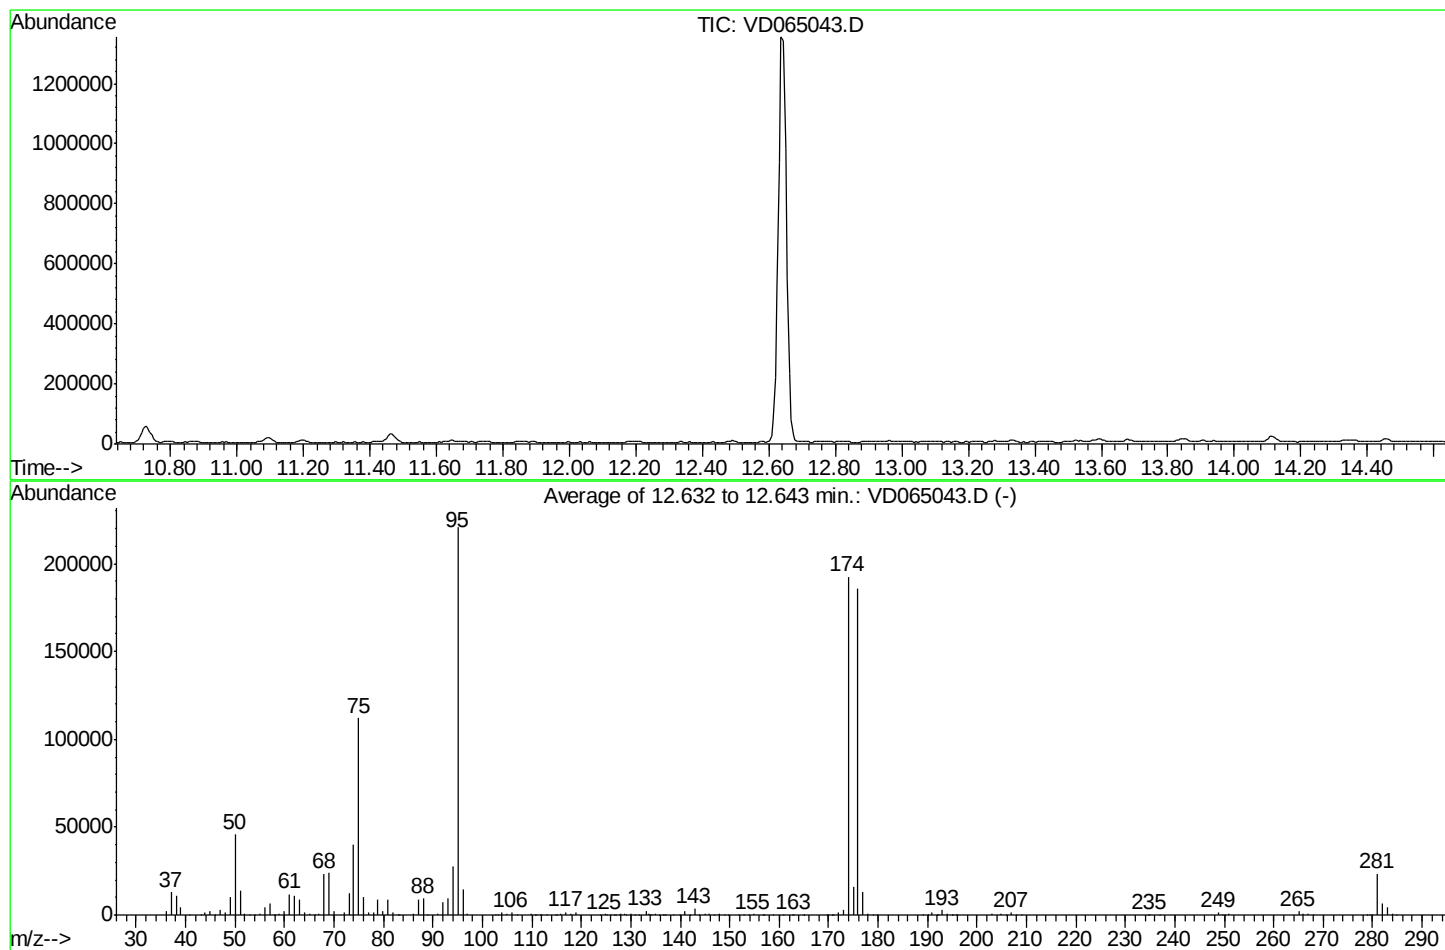

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	45637	PASS
75	95	30	60	50.7	112008	PASS
95	95	100	100	100.0	220714	PASS
96	95	5	9	6.6	14474	PASS
173	174	0.00	2	1.5	2807	PASS
174	95	50	100	87.3	192597	PASS
175	174	5	9	8.2	15799	PASS
176	174	95	101	96.6	186005	PASS
177	176	5	9	6.9	12812	PASS