
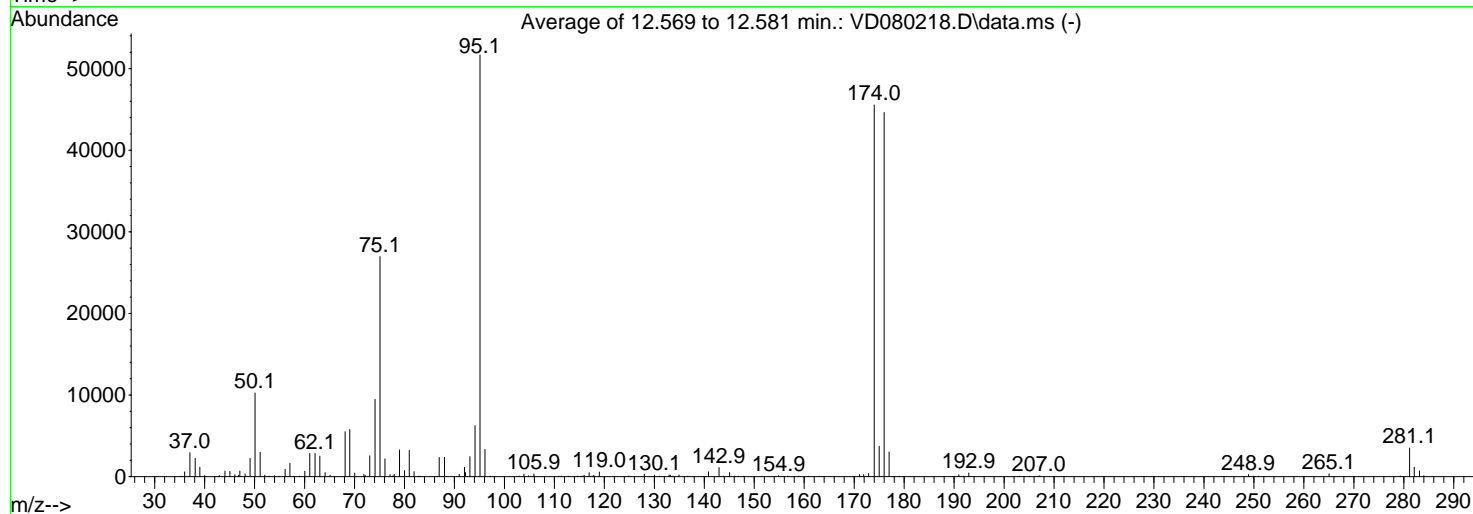


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020325\
 Data File : VD080218.D
 Acq On : 03 Feb 2025 09:37
 Operator : RP/MD
 Sample : BFB
 Misc : 5.00G/10ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020325S.M
 Title : SW846 8260
 Last Update : Tue Feb 04 05:44:14 2025

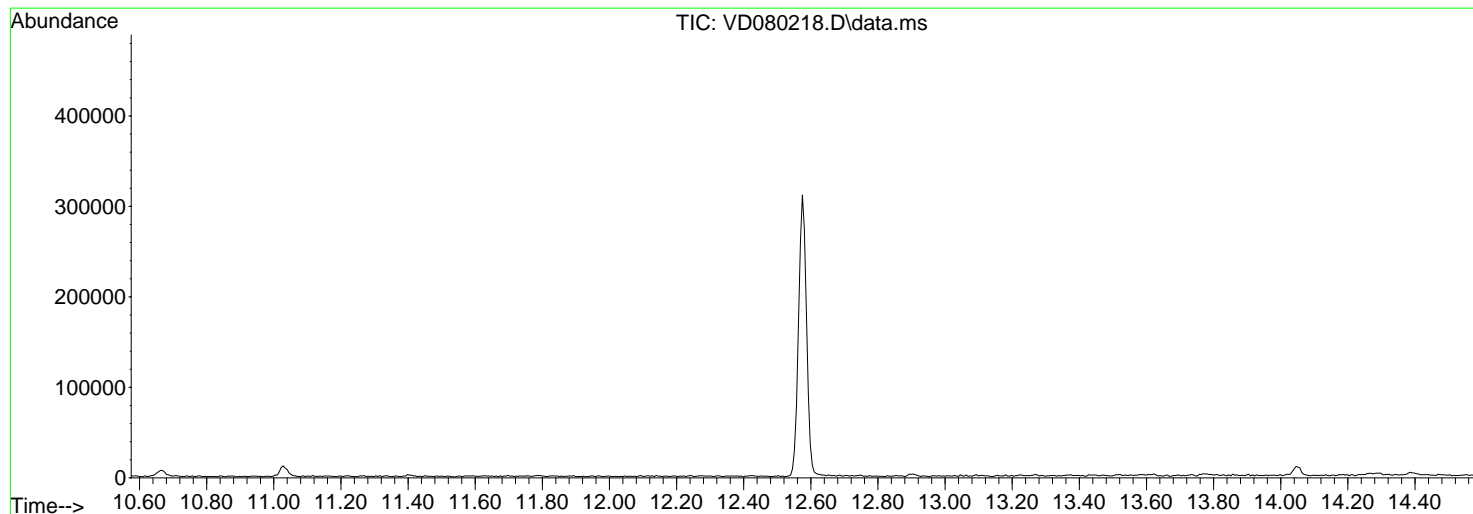

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	10262	PASS
75	95	30	60	52.2	26973	PASS
95	95	100	100	100.0	51680	PASS
96	95	5	9	6.4	3332	PASS
173	174	0.00	2	0.9	403	PASS
174	95	50	100	88.1	45541	PASS
175	174	5	9	8.2	3716	PASS
176	174	95	101	98.0	44629	PASS
177	176	5	9	6.8	3026	PASS