


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD020520\
 Data File : VD065058.D
 Acq On : 05 Feb 2020 09:39
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D020520S.M
 Title : SW846 8260
 Last Update : Wed Feb 05 15:53:00 2020

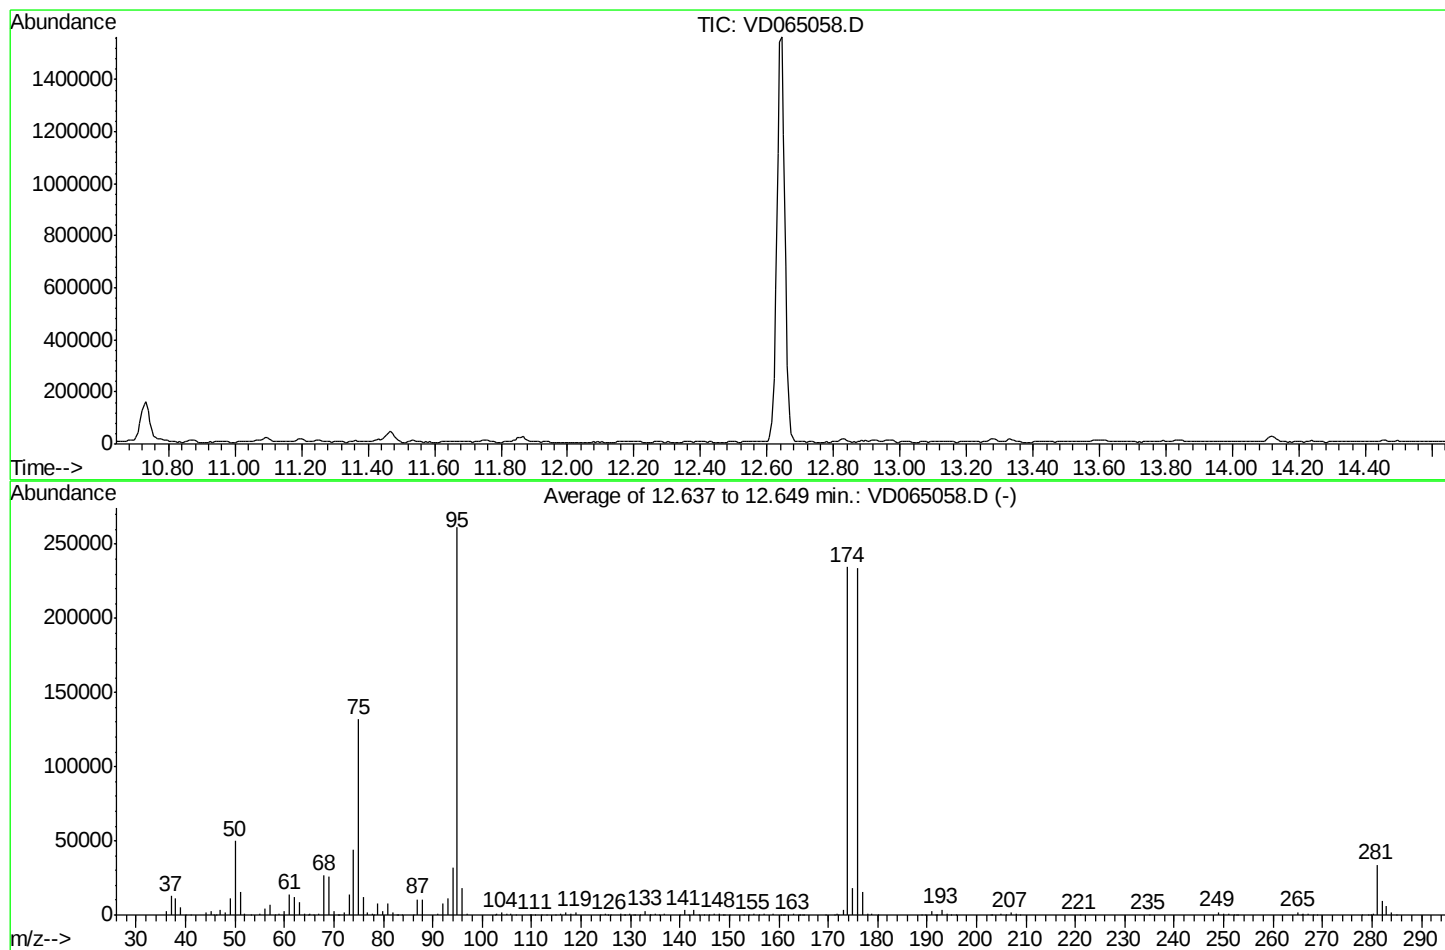

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	49877	PASS
75	95	30	60	50.4	131866	PASS
95	95	100	100	100.0	261461	PASS
96	95	5	9	7.0	18412	PASS
173	174	0.00	2	1.3	3127	PASS
174	95	50	100	89.7	234560	PASS
175	174	5	9	7.8	18214	PASS
176	174	95	101	99.7	233898	PASS
177	176	5	9	6.5	15261	PASS