

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020521\
 Data File : VD068299.D
 Acq On : 05 Feb 2021 14:03
 Operator : VA/SY
 Sample : M1317-01
 Misc : 9.82G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 R-A

Quant Time: Feb 05 21:41:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 13:19:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.979	168	416523	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	792029	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	584303	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.579	152	134311	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	259419	65.11	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 130.22%			
35) Dibromofluoromethane	7.920	113	249757	57.04	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 114.08%			
50) Toluene-d8	10.344	98	877899	50.12	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 100.24%			
62) 4-Bromofluorobenzene	12.632	95	220693	34.99	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 69.98%			
Target Compounds						Qvalue
10) Methyl Iodide	4.291	142	574	3.27	ug/l #	91
11) Tert butyl alcohol	5.226	59	263	Below Cal	#	74
16) Acetone	4.156	43	81427	114.45	ug/l	92
20) Methylene Chloride	4.979	84	1655	Below Cal	#	81
25) 2-Butanone	7.220	43	16489	15.39	ug/l	92
29) Tetrahydrofuran	7.567	42	719	1.04	ug/l #	54
31) Cyclohexane	7.985	56	13787	1.60	ug/l #	45
55) 1,1,2-Trichloroethane	10.773	97	5878	1.50	ug/l #	21
59) 2-Hexanone	10.955	43	17100	9.01	ug/l #	19
68) m/p-Xylenes	11.855	106	10885	1.25	ug/l	85
69) o-Xylene	12.179	106	8809	1.09	ug/l	65
73) Isopropylbenzene	12.479	105	47951	4.29	ug/l	91
74) N-amyl acetate	12.267	43	169470	72.95	ug/l #	51
75) 1,1,2,2-Tetrachloroethane	12.708	83	27869	15.68	ug/l #	79
76) 1,2,3-Trichloropropane	12.632	75	106253	81.82	ug/l #	100
78) n-propylbenzene	12.820	91	98473	7.45	ug/l	96
79) 2-Chlorotoluene	12.914	91	13947	1.88	ug/l #	58
80) 1,3,5-Trimethylbenzene	12.961	105	61796	6.64	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.632	75	106253	165.56	ug/l #	19
82) 4-Chlorotoluene	12.955	91	8630	1.12	ug/l #	51
83) tert-Butylbenzene	13.220	119	13790	1.75	ug/l	86
84) 1,2,4-Trimethylbenzene	13.267	105	219028	23.71	ug/l	98
85) sec-Butylbenzene	13.402	105	98497	8.93	ug/l #	74
86) p-Isopropyltoluene	13.514	119	52940	5.28	ug/l	95
89) n-Butylbenzene	13.843	91	90532	9.40	ug/l #	73
90) Hexachloroethane	14.114	117	14257	7.87	ug/l #	13
92) 1,2-Dibromo-3-Chloropr...	14.526	75	863	2.97	ug/l #	10
93) 1,2,4-Trichlorobenzene	15.167	180	3926	1.45	ug/l #	1
94) Hexachlorobutadiene	15.267	225	1682	1.12	ug/l #	75
95) Naphthalene	15.402	128	103264	20.36	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.608	180	4677	2.05	ug/l #	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020521\
Data File : VD068299.D
Acq On : 05 Feb 2021 14:03
Operator : VA/SY
Sample : M1317-01
Misc : 9.82G/5.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
R-A

Quant Time: Feb 05 21:41:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 19 13:19:08 2021
Response via : Initial Calibration




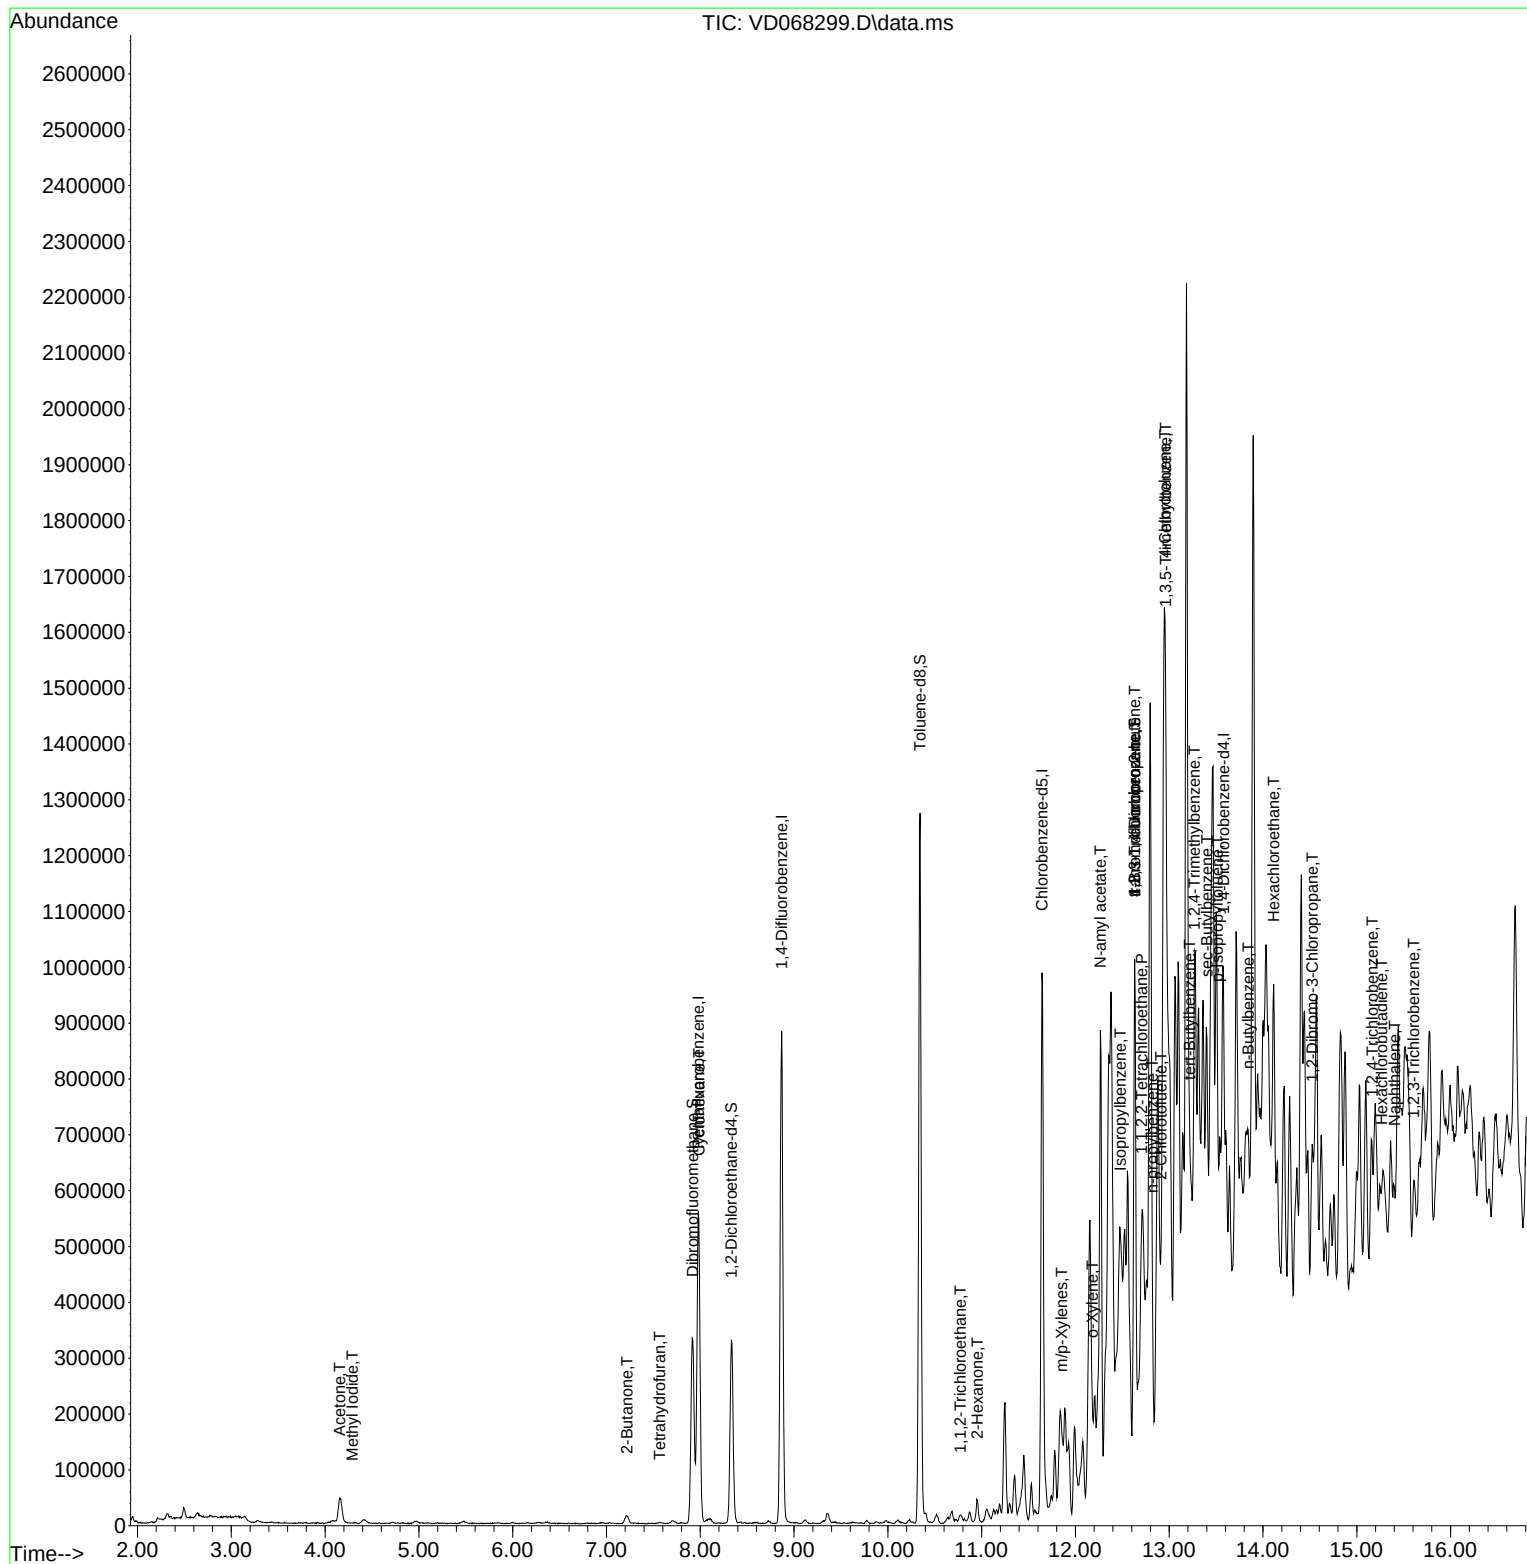


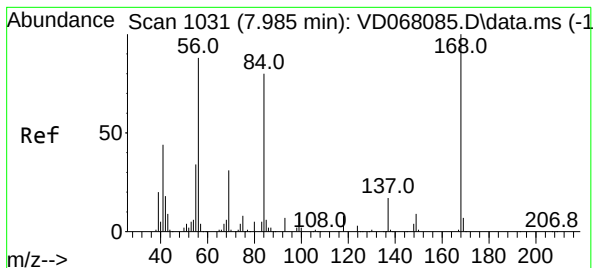

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion:168 Resp: 416523
Ion Ratio Lower Upper
168 100
99 59.6 43.5 65.3

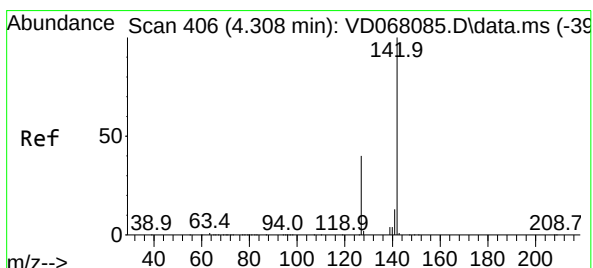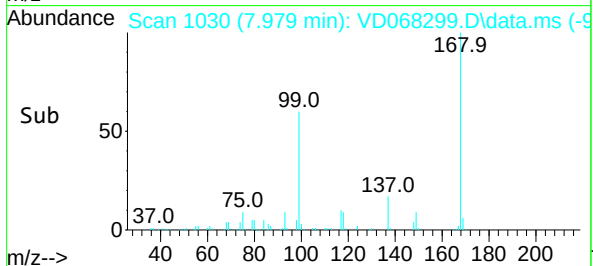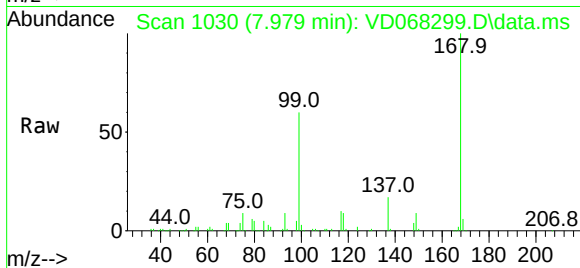

#10
Methyl Iodide
Concen: 3.27 ug/l
RT: 4.291 min Scan# 403
Delta R.T. -0.017 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03


Tgt Ion:142 Resp: 574
Ion Ratio Lower Upper
142 100
127 47.7 37.9 56.9
141 0.0 11.5 17.3#

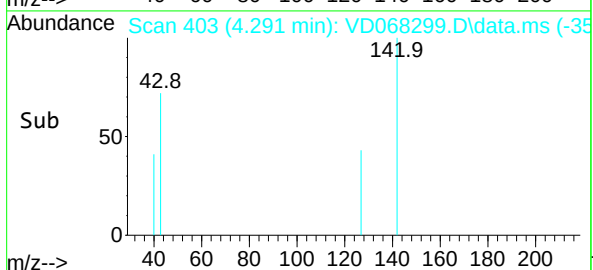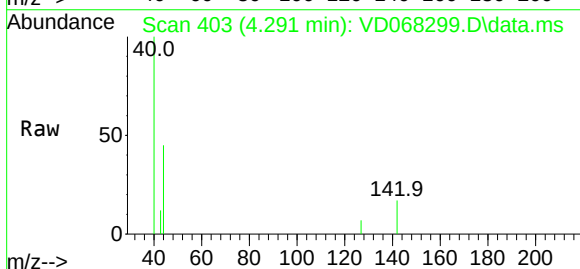






#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.226 min Scan# 562
Delta R.T. 0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Instrument :
MSVOA_D
ClientSampled :
R-A







Tgt Ion: 59 Resp: 263
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

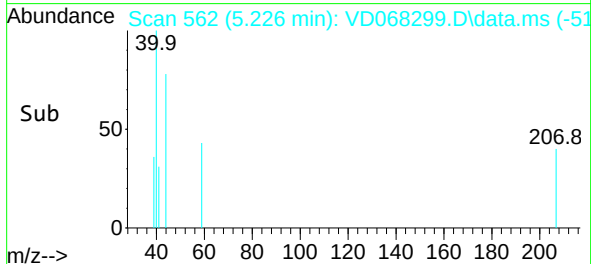

#16
Acetone
Concen: 114.45 ug/l
RT: 4.156 min Scan# 380
Delta R.T. -0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 43 Resp: 81427
Ion Ratio Lower Upper
43 100
58 34.5 24.2 36.4


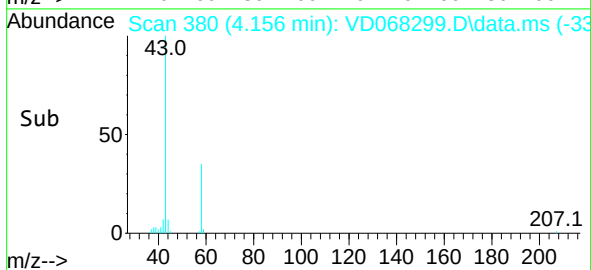

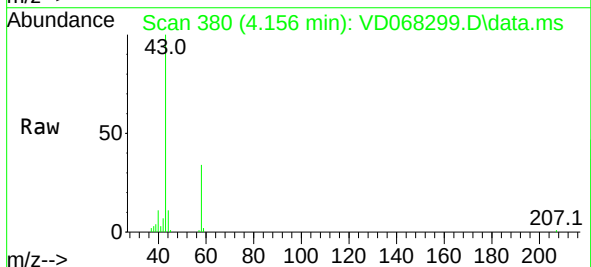




#20
Methylene Chloride
Concen: Below Cal
RT: 4.979 min Scan# 520
Delta R.T. 0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion:	84	Resp:	1655
Ion	Ratio	Lower	Upper
84	100		
49	77.2	77.4	116.2#
51	33.7	26.1	39.1
86	45.2	51.8	77.8#

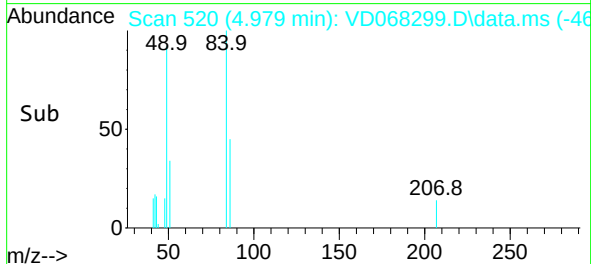

#25
2-Butanone
Concen: 15.39 ug/l
RT: 7.220 min Scan# 901
Delta R.T. 0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion:	43	Resp:	16489
Ion	Ratio	Lower	Upper
43	100		
72	26.8	25.1	37.7

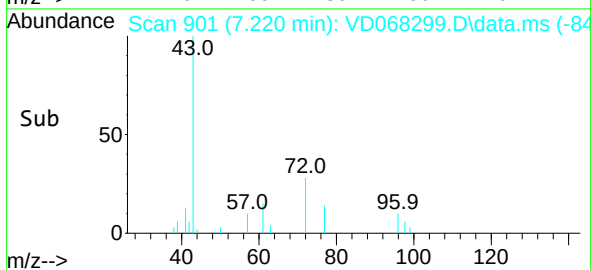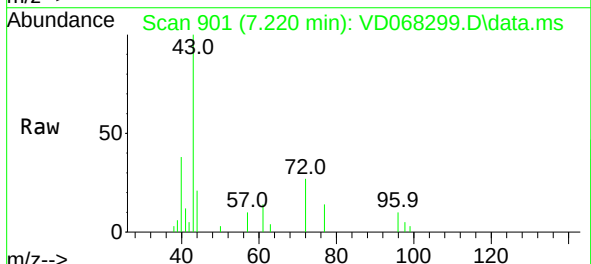



#29

Tetrahydrofuran

Concen: 1.04 ug/l

RT: 7.567 min Scan# 960

Delta R.T. 0.000 min

Lab File: VD068299.D

Acq: 05 Feb 2021 14:03





Tgt Ion: 42 Resp: 719

Ion Ratio Lower Upper

42 100

72 40.1 43.4 65.0#

71 0.0 40.8 61.2#

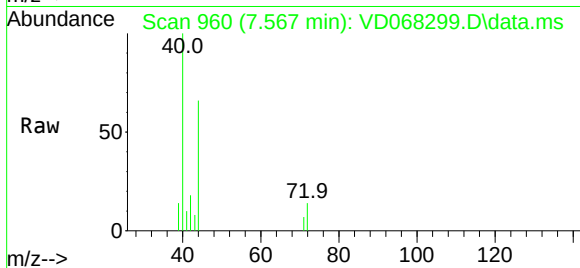

#31

Cyclohexane

Concen: 1.60 ug/l

RT: 7.985 min Scan# 1031

Delta R.T. -0.006 min

Lab File: VD068299.D

Acq: 05 Feb 2021 14:03




Tgt Ion: 56 Resp: 13787


Ion Ratio Lower Upper

56 100

69 118.0 30.1 45.1#

84 128.7 82.1 123.1#


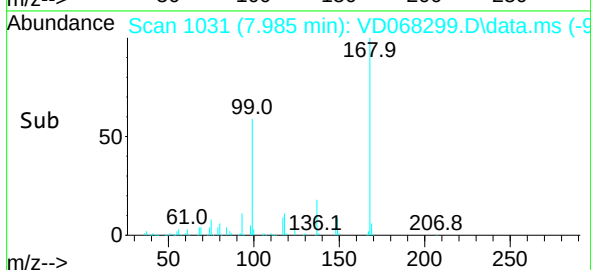

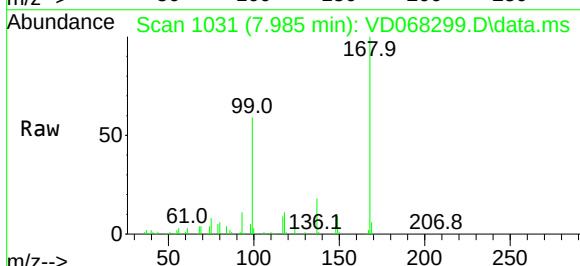




#33
 1,2-Dichloroethane-d4
 Concen: 65.11 ug/l
 RT: 8.332 min Scan# 1090
 Delta R.T. -0.006 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03




Instrument :
 MSVOA_D
 ClientSampleId :
 R-A


Tgt Ion: 65 Resp: 259419
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 105.0

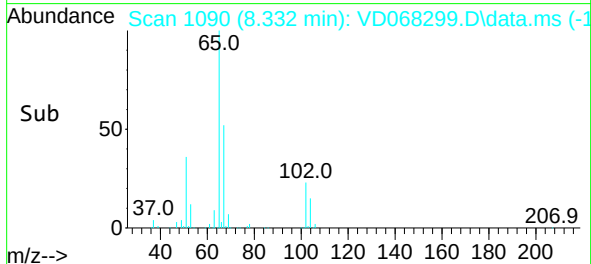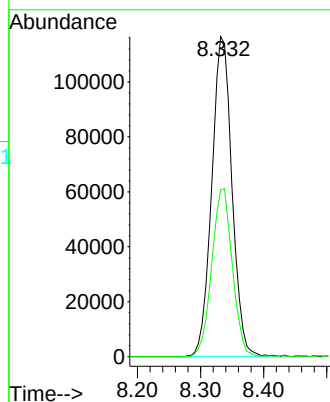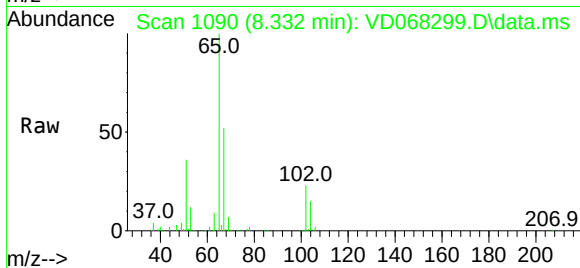

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.867 min Scan# 1181
 Delta R.T. 0.000 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03

Tgt Ion: 114 Resp: 792029
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 34.8
 88 16.5 0.0 31.6

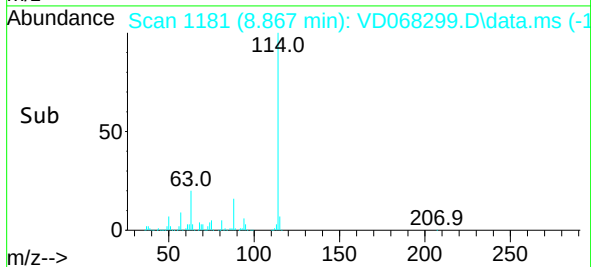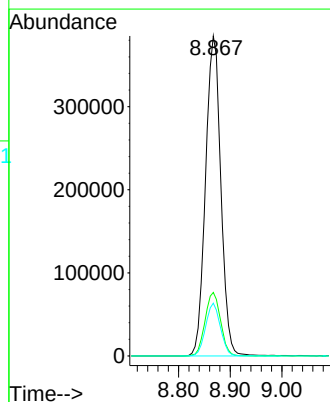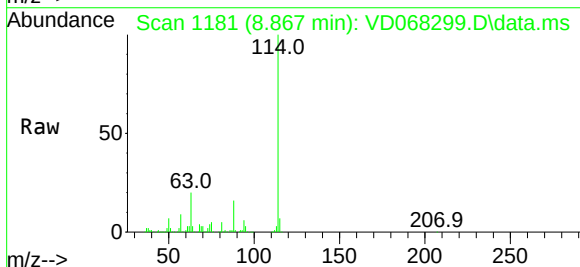

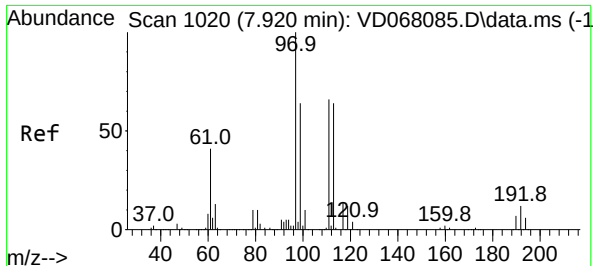

#35

Dibromofluoromethane

Concen: 57.04 ug/l

RT: 7.920 min Scan# 1020

Delta R.T. 0.000 min

Lab File: VD068299.D

Acq: 05 Feb 2021 14:03





Tgt Ion:113 Resp: 249757

Ion Ratio Lower Upper

113 100

111 101.7 81.4 122.0

192 18.2 16.1 24.1

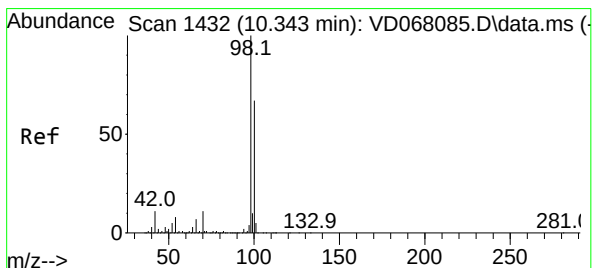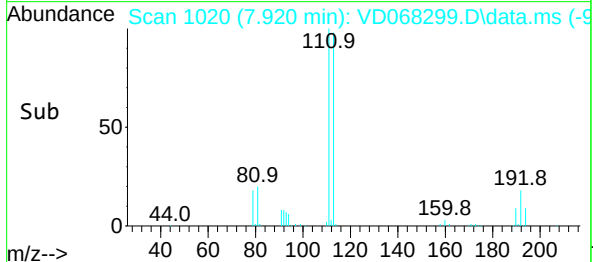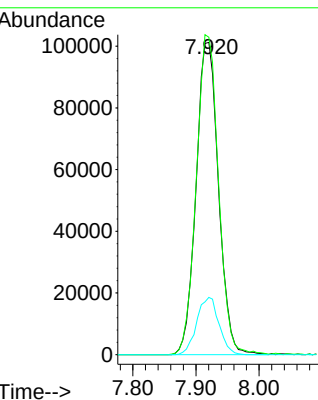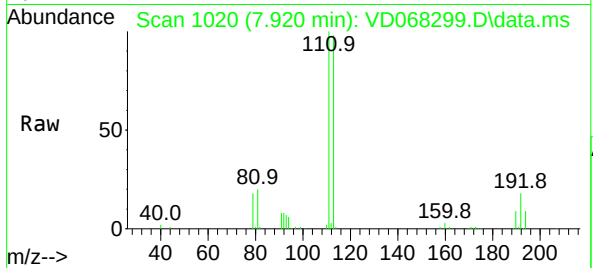

#50

Toluene-d8

Concen: 50.12 ug/l

RT: 10.344 min Scan# 1432

Delta R.T. 0.000 min

Lab File: VD068299.D




Acq: 05 Feb 2021 14:03


Tgt Ion: 98 Resp: 877899

Ion Ratio Lower Upper

98 100

100 65.1 53.0 79.4


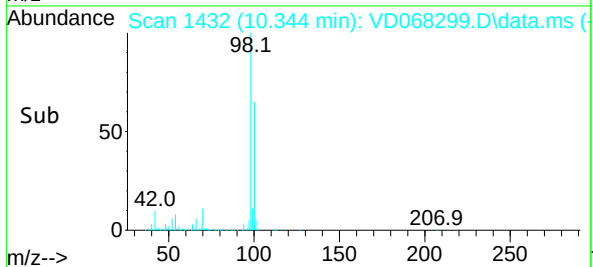
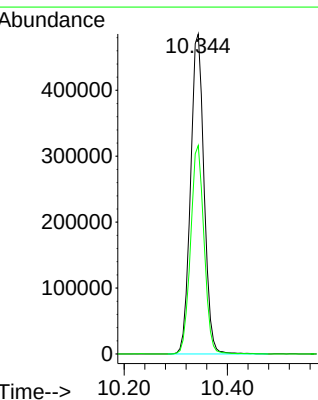
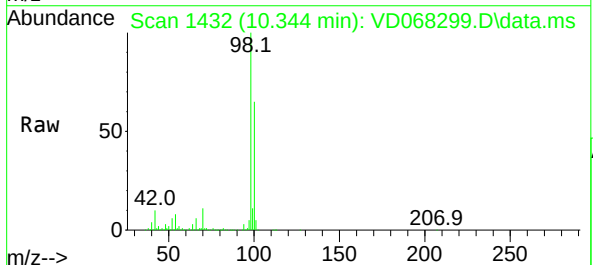




#55
1,1,2-Trichloroethane
Concen: 1.50 ug/l
RT: 10.773 min Scan# 1505
Delta R.T. -0.029 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion: 97	Resp: 5878
Ion Ratio	Lower Upper
97 100	
83 0.0	61.8 92.6#
85 7.2	42.2 63.2#
99 0.0	48.3 72.5#

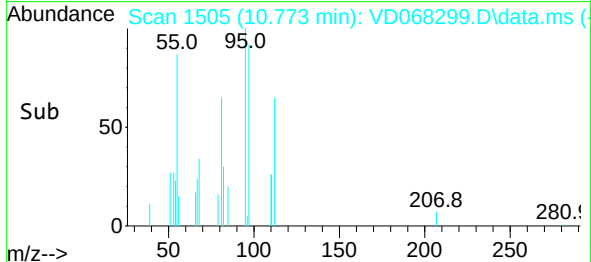

#59
2-Hexanone
Concen: 9.01 ug/l
RT: 10.955 min Scan# 1536
Delta R.T. -0.029 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 43	Resp: 17100		
Ion Ratio	Lower	Upper	
43 100			
58 0.0	31.0	93.0#	


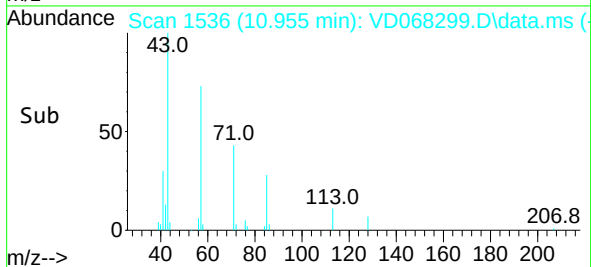

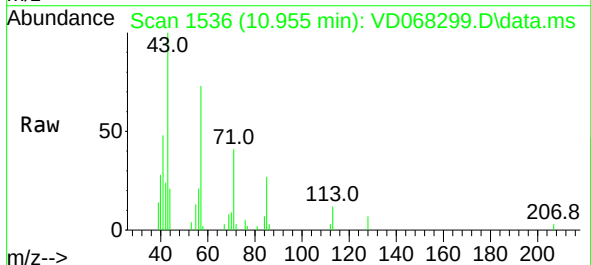




#62
4-Bromofluorobenzene
Concen: 34.99 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion: 95 Resp: 220693
Ion Ratio Lower Upper
95 100
174 73.6 0.0 172.4
176 69.8 0.0 168.4

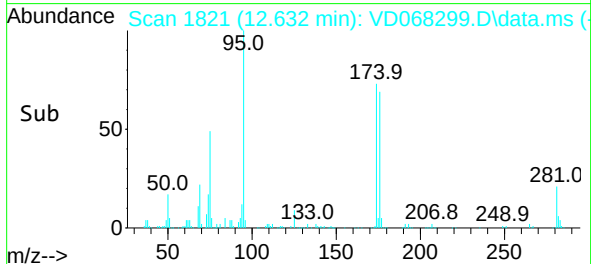

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. -0.005 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 117 Resp: 584303
Ion Ratio Lower Upper
117 100
82 54.4 41.4 62.0
119 32.0 26.1 39.1


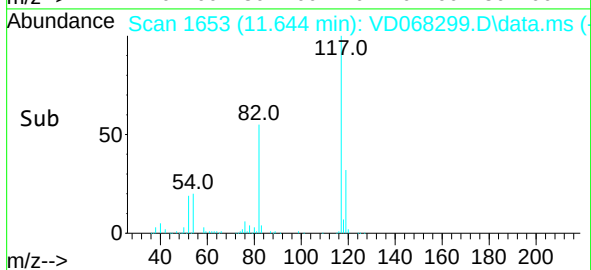

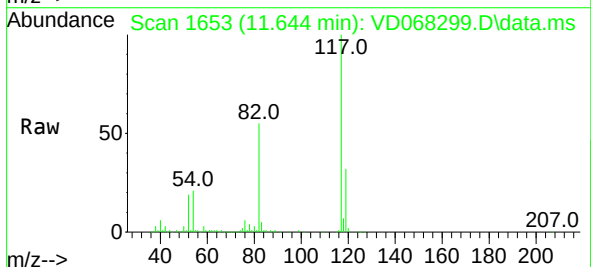


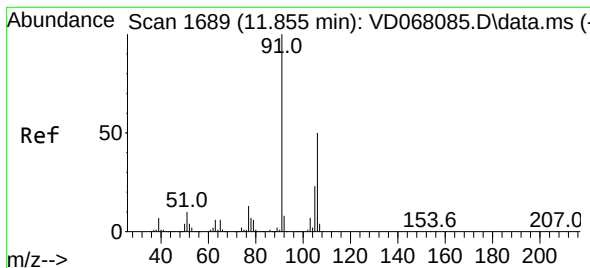

#68
m/p-Xylenes
Concen: 1.25 ug/l
RT: 11.855 min Scan# 1689
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion:106 Resp: 10885
Ion Ratio Lower Upper
106 100
91 221.4 159.1 238.7

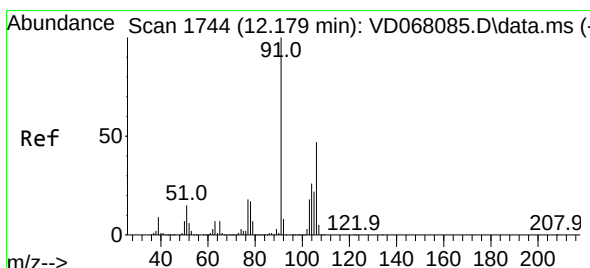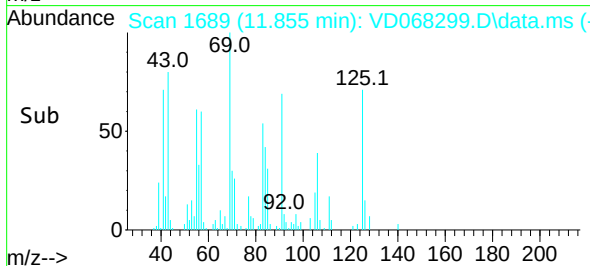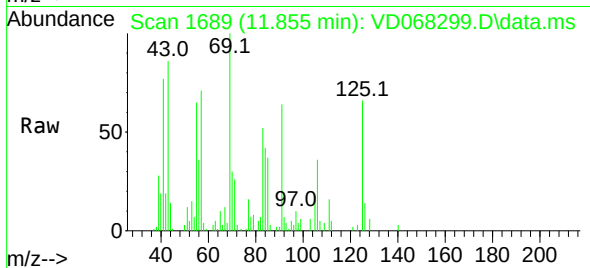

#69
o-Xylene
Concen: 1.09 ug/l
RT: 12.179 min Scan# 1744
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion:106 Resp: 8809
Ion Ratio Lower Upper
106 100
91 273.5 108.7 325.9

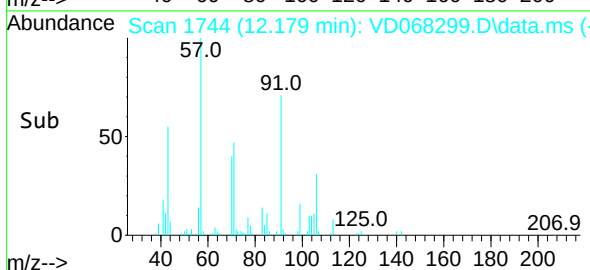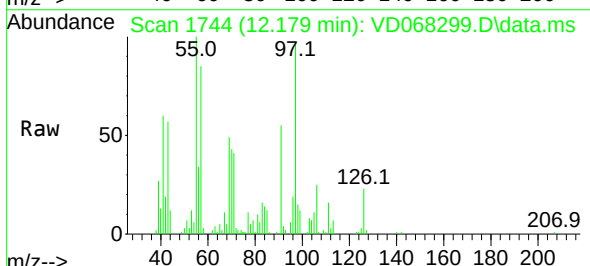



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.579 min Scan# 1982

Delta R.T. 0.006 min

Lab File: VD068299.D

Acq: 05 Feb 2021 14:03





Tgt Ion:152 Resp: 134311

Ion Ratio Lower Upper

152 100

115 58.8 28.9 86.8

150 143.5 0.0 344.4

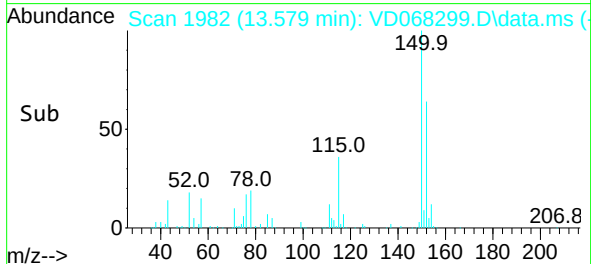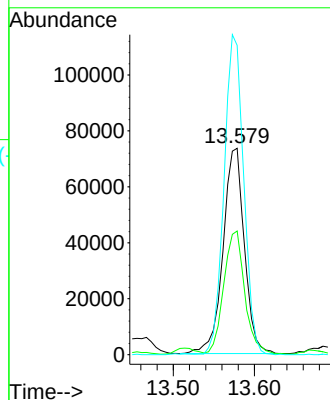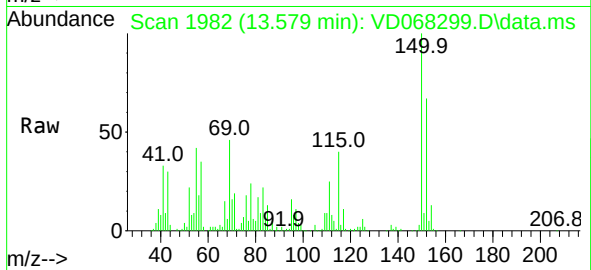

#73

Isopropylbenzene

Concen: 4.29 ug/l

RT: 12.479 min Scan# 1795

Delta R.T. 0.000 min

Lab File: VD068299.D




Acq: 05 Feb 2021 14:03


Tgt Ion:105 Resp: 47951

Ion Ratio Lower Upper

105 100


120 21.6 13.2 39.6

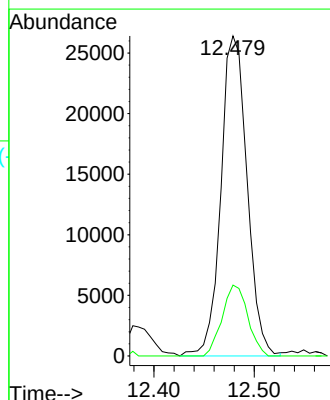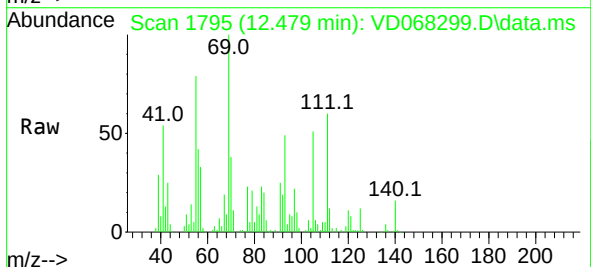



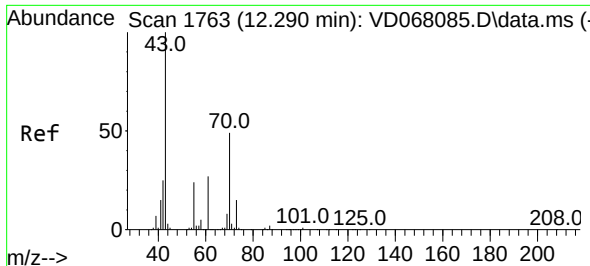


#74
N-amy1 acetate
Concen: 72.95 ug/l
RT: 12.267 min Scan# 1759
Delta R.T. -0.023 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Instrument :
MSVOA_D
ClientSampled :
R-A



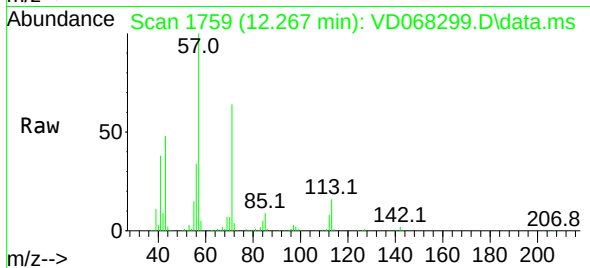



Tgt Ion:	43	Resp:	169470
Ion Ratio	100	Lower	Upper
43	100		
70	22.2	41.8	62.8#
55	0.0	24.2	36.4#
61	0.0	21.7	32.5#

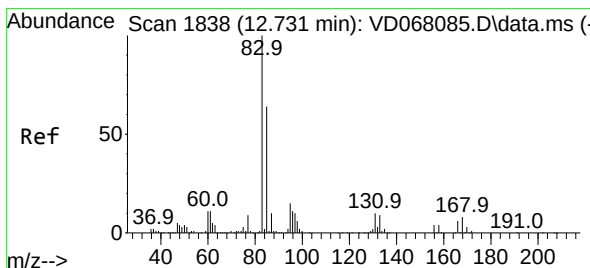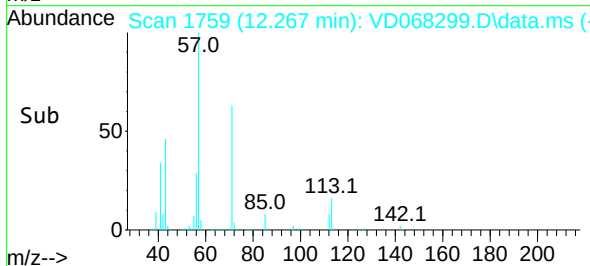

#75
1,1,2,2-Tetrachloroethane
Concen: 15.68 ug/l
RT: 12.708 min Scan# 1834
Delta R.T. -0.023 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion:	83	Resp:	27869
Ion Ratio	100	Lower	Upper
83	100		
131	0.0	5.8	17.4#
85	49.1	32.4	97.2


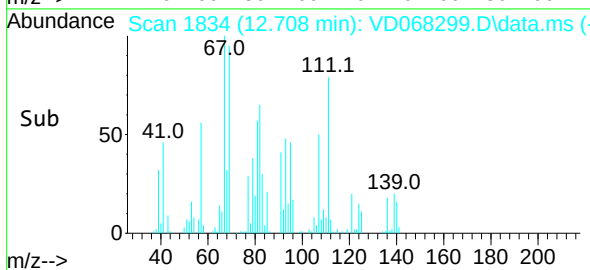

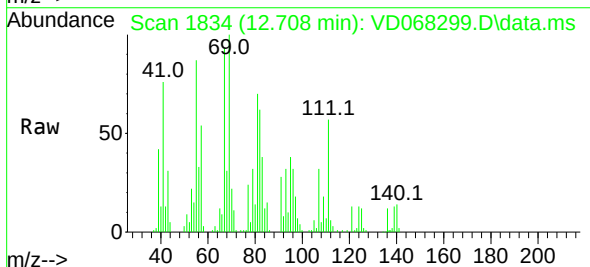




#76
1,2,3-Trichloropropane
Concen: 81.82 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.153 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion: 75 Resp: 106253
Ion Ratio Lower Upper
75 100
77 4.1 0.0 0.0#

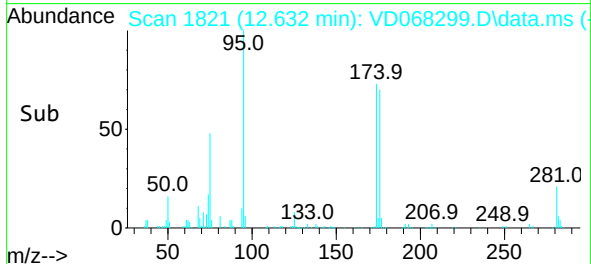

#78
n-propylbenzene
Concen: 7.45 ug/l
RT: 12.820 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 91 Resp: 98473
Ion Ratio Lower Upper
91 100
120 22.1 12.0 36.0




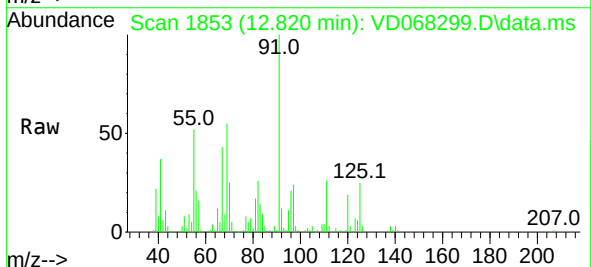


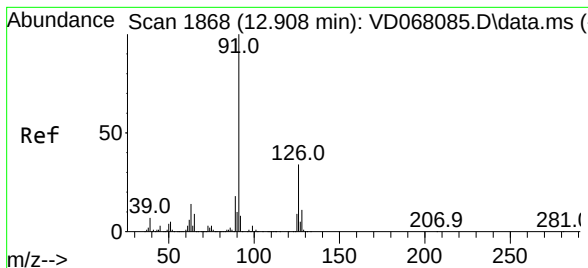

#79
2-Chlorotoluene
Concen: 1.88 ug/l
RT: 12.914 min Scan# 1869
Delta R.T. 0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion: 91 Resp: 13947
Ion Ratio Lower Upper
91 100
126 10.8 17.8 53.5#

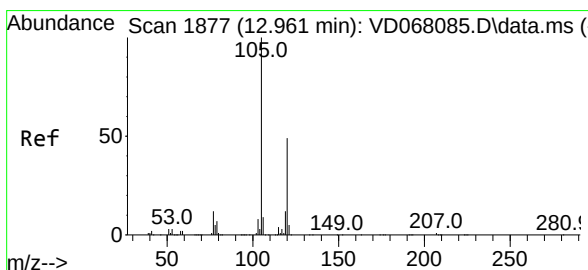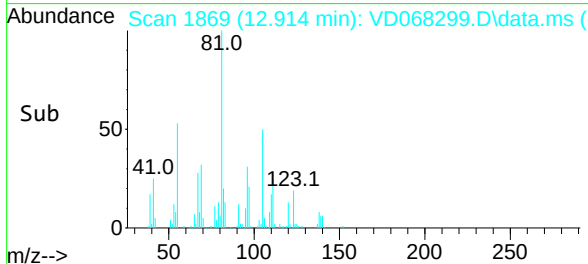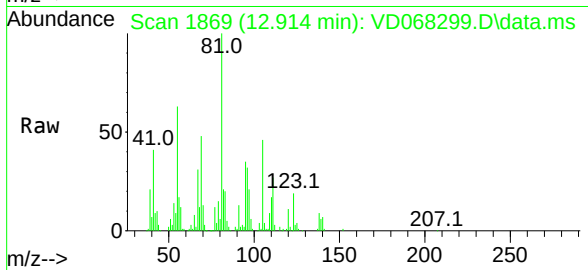

#80
1,3,5-Trimethylbenzene
Concen: 6.64 ug/l
RT: 12.961 min Scan# 1877
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 105 Resp: 61796
Ion Ratio Lower Upper
105 100
120 51.6 24.2 72.6


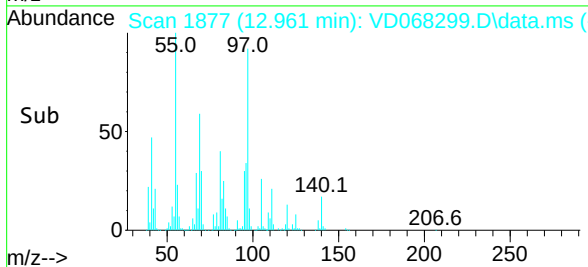

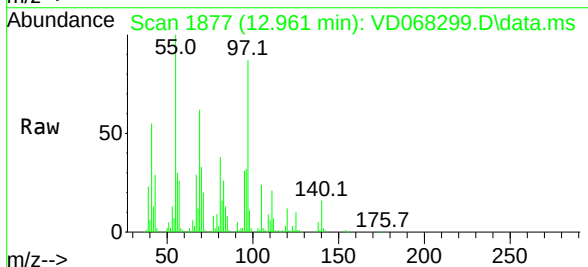


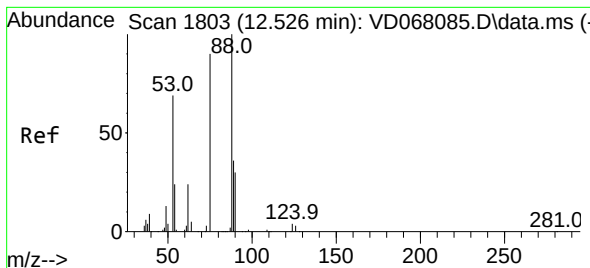

#81
 trans-1,4-Dichloro-2-butene
 Concen: 165.56 ug/l
 RT: 12.632 min Scan# 1821
 Delta R.T. 0.106 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03




Instrument :
 MSVOA_D
 ClientSampleId :
 R-A


Tgt Ion: 75 Resp: 106253
 Ion Ratio Lower Upper
 75 100
 53 5.5 70.2 105.2#
 89 4.3 40.3 60.5#

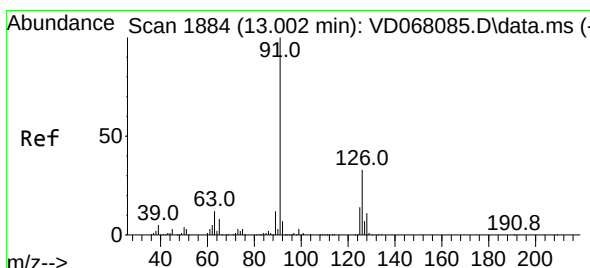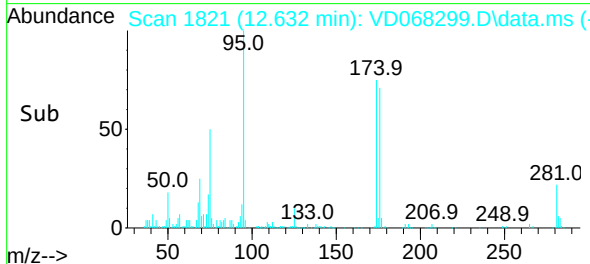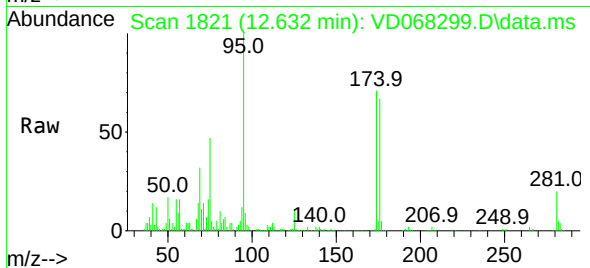

#82
 4-Chlorotoluene
 Concen: 1.12 ug/l
 RT: 12.955 min Scan# 1876
 Delta R.T. -0.047 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03

Tgt Ion: 91 Resp: 8630
 Ion Ratio Lower Upper
 91 100
 126 63.8 17.7 53.1#


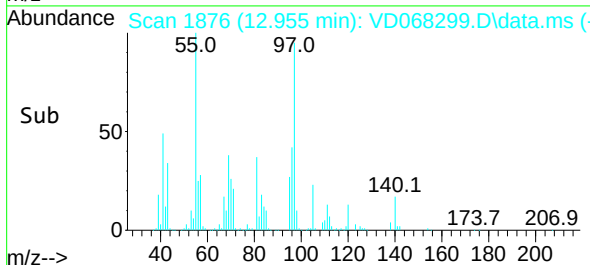

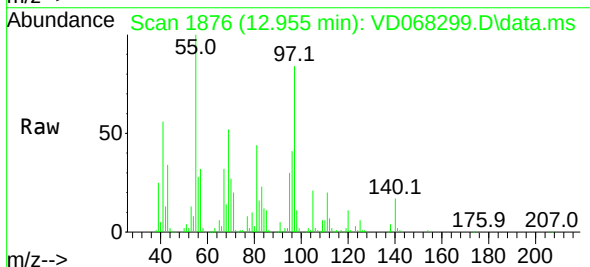




#83
tert-Butylbenzene
Concen: 1.75 ug/l
RT: 13.220 min Scan# 1921
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion:119 Resp: 13790
Ion Ratio Lower Upper
119 100
91 47.8 31.1 93.5
134 24.9 13.3 39.8

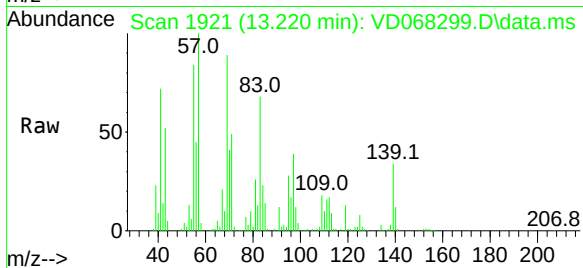

#84
1,2,4-Trimethylbenzene
Concen: 23.71 ug/l
RT: 13.267 min Scan# 1929
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion:105 Resp: 219028
Ion Ratio Lower Upper
105 100
120 46.2 22.4 67.0


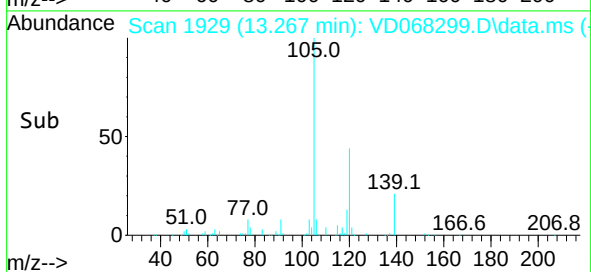

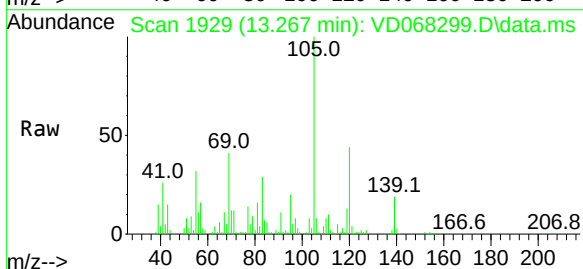




#85
 sec-Butylbenzene
 Concen: 8.93 ug/l
 RT: 13.402 min Scan# 1952
 Delta R.T. 0.000 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03




Instrument :
 MSVOA_D
 ClientSampled :
 R-A


Tgt Ion:105 Resp: 98497
 Ion Ratio Lower Upper
 105 100
 134 32.7 10.3 30.9#

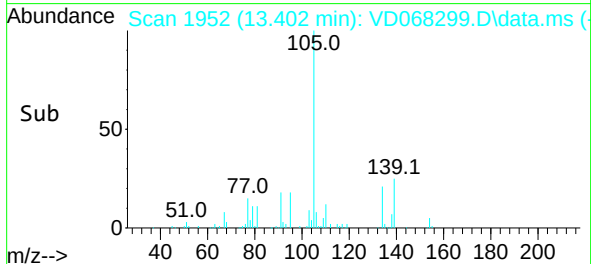

#86
 p-Isopropyltoluene
 Concen: 5.28 ug/l
 RT: 13.514 min Scan# 1971
 Delta R.T. 0.000 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03

Tgt Ion:119 Resp: 52940
 Ion Ratio Lower Upper
 119 100
 134 24.7 12.9 38.7
 91 27.5 11.7 35.0


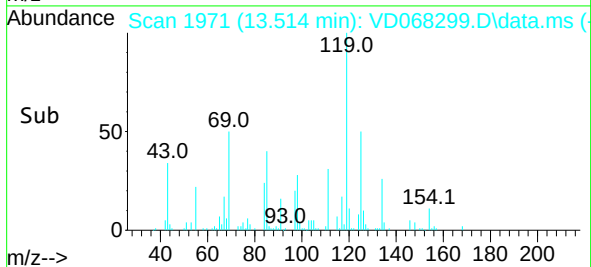

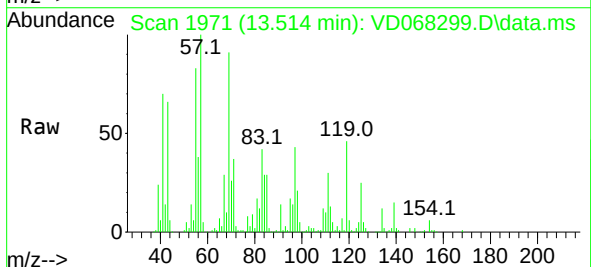


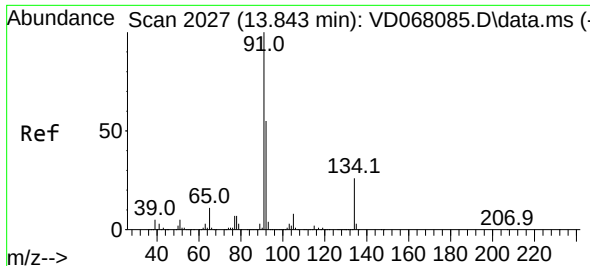

#89
n-Butylbenzene
Concen: 9.40 ug/l
RT: 13.843 min Scan# 2027
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampleId :
R-A


Tgt Ion: 91 Resp: 90532
Ion Ratio Lower Upper
91 100
92 44.2 27.2 81.6
134 0.0 13.9 41.7#

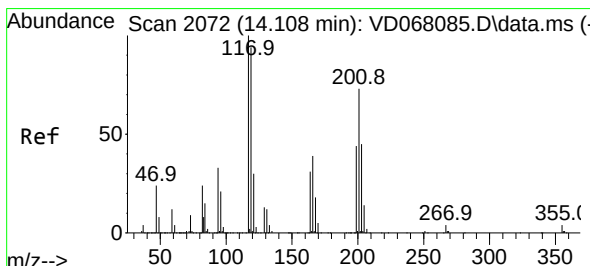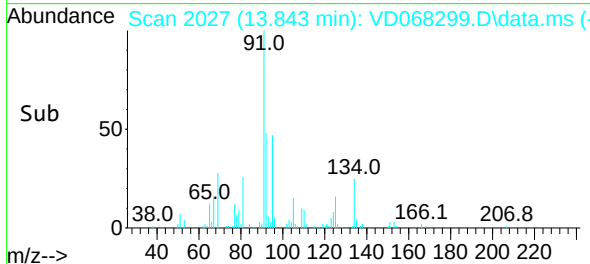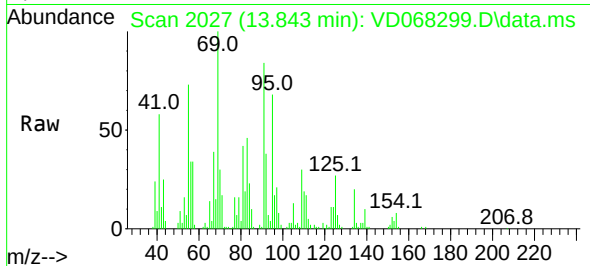

#90
Hexachloroethane
Concen: 7.87 ug/l
RT: 14.114 min Scan# 2073
Delta R.T. 0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 117 Resp: 14257
Ion Ratio Lower Upper
117 100
201 3.0 39.5 118.5#


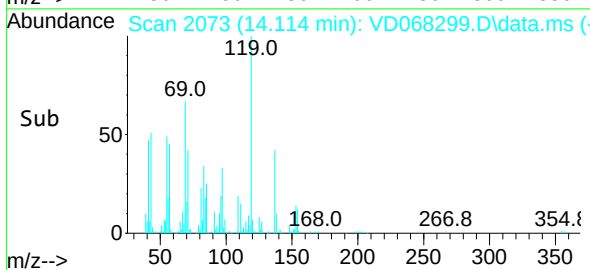

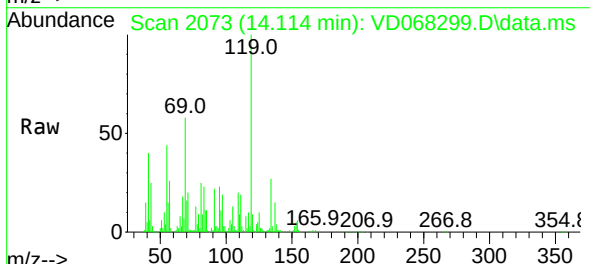


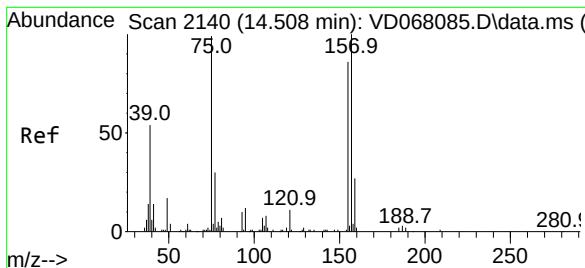

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.97 ug/l
RT: 14.526 min Scan# 2143
Delta R.T. 0.018 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion: 75 Resp: 863
Ion Ratio Lower Upper
75 100
155 36.7 48.0 144.2#
157 0.0 65.0 194.8#

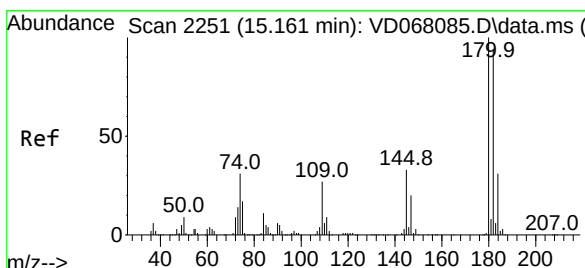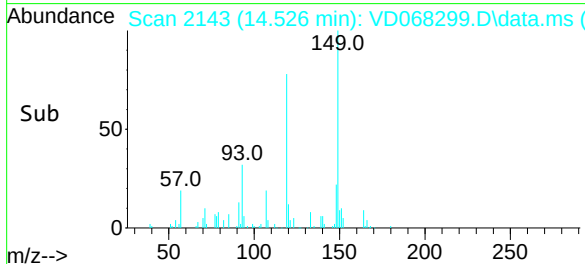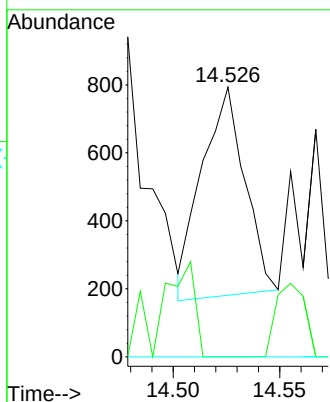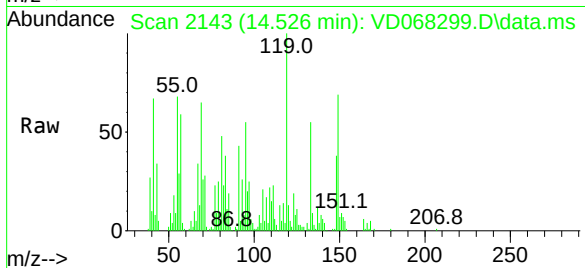

#93
1,2,4-Trichlorobenzene
Concen: 1.45 ug/l
RT: 15.167 min Scan# 2252
Delta R.T. 0.006 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion: 180 Resp: 3926
Ion Ratio Lower Upper
180 100
182 97.7 46.8 140.4
145 692.0 15.2 45.5#


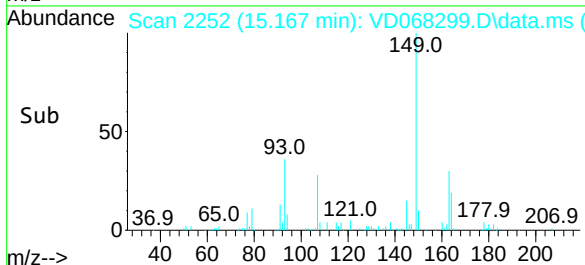
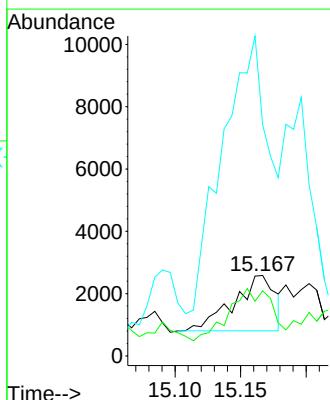
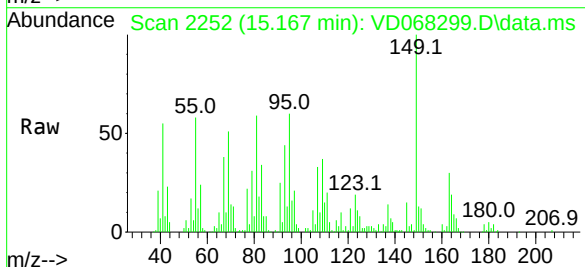




#94
Hexachlorobutadiene
Concen: 1.12 ug/l
RT: 15.267 min Scan# 2269
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03




Instrument :
MSVOA_D
ClientSampled :
R-A


Tgt Ion:	225	Resp:	1682
Ion Ratio	Lower	Upper	
225	100		
223	57.1	31.9	95.5
227	31.1	32.1	96.5#

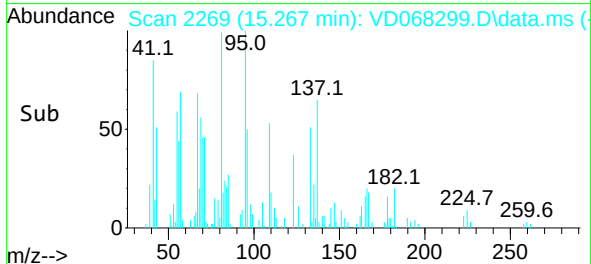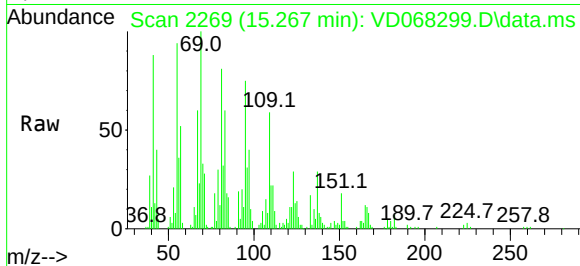

#95
Naphthalene
Concen: 20.36 ug/l
RT: 15.402 min Scan# 2292
Delta R.T. 0.000 min
Lab File: VD068299.D
Acq: 05 Feb 2021 14:03

Tgt Ion:	128	Resp:	103264
Ion Ratio	Lower	Upper	
128	100		
127	17.1	10.2	15.2#
129	11.8	8.8	13.2

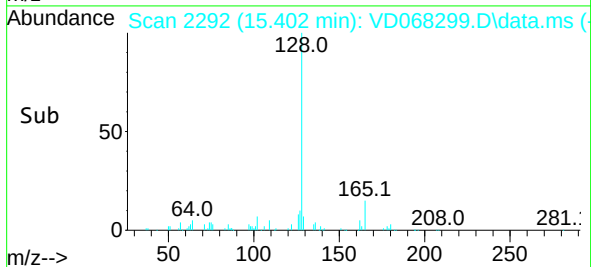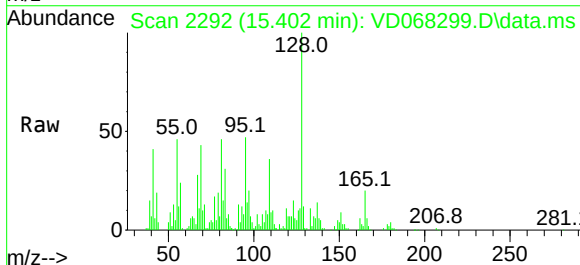

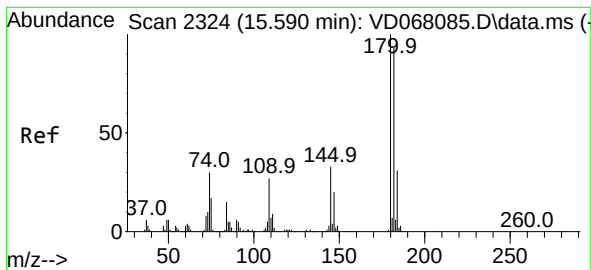

#96
 1,2,3-Trichlorobenzene
 Concen: 2.05 ug/l
 RT: 15.608 min Scan# 2327
 Delta R.T. 0.018 min
 Lab File: VD068299.D
 Acq: 05 Feb 2021 14:03

Instrument :
 MSVOA_D
 ClientSampleId :
 R-A

Tgt Ion:180 Resp: 4677
 Ion Ratio Lower Upper
 180 100
 182 45.7 48.3 144.8#
 145 0.0 16.7 50.1#

