


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD020720\
 Data File : VD065101.D
 Acq On : 07 Feb 2020 09:38
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D020520S.M
 Title : SW846 8260
 Last Update : Wed Feb 05 15:53:00 2020

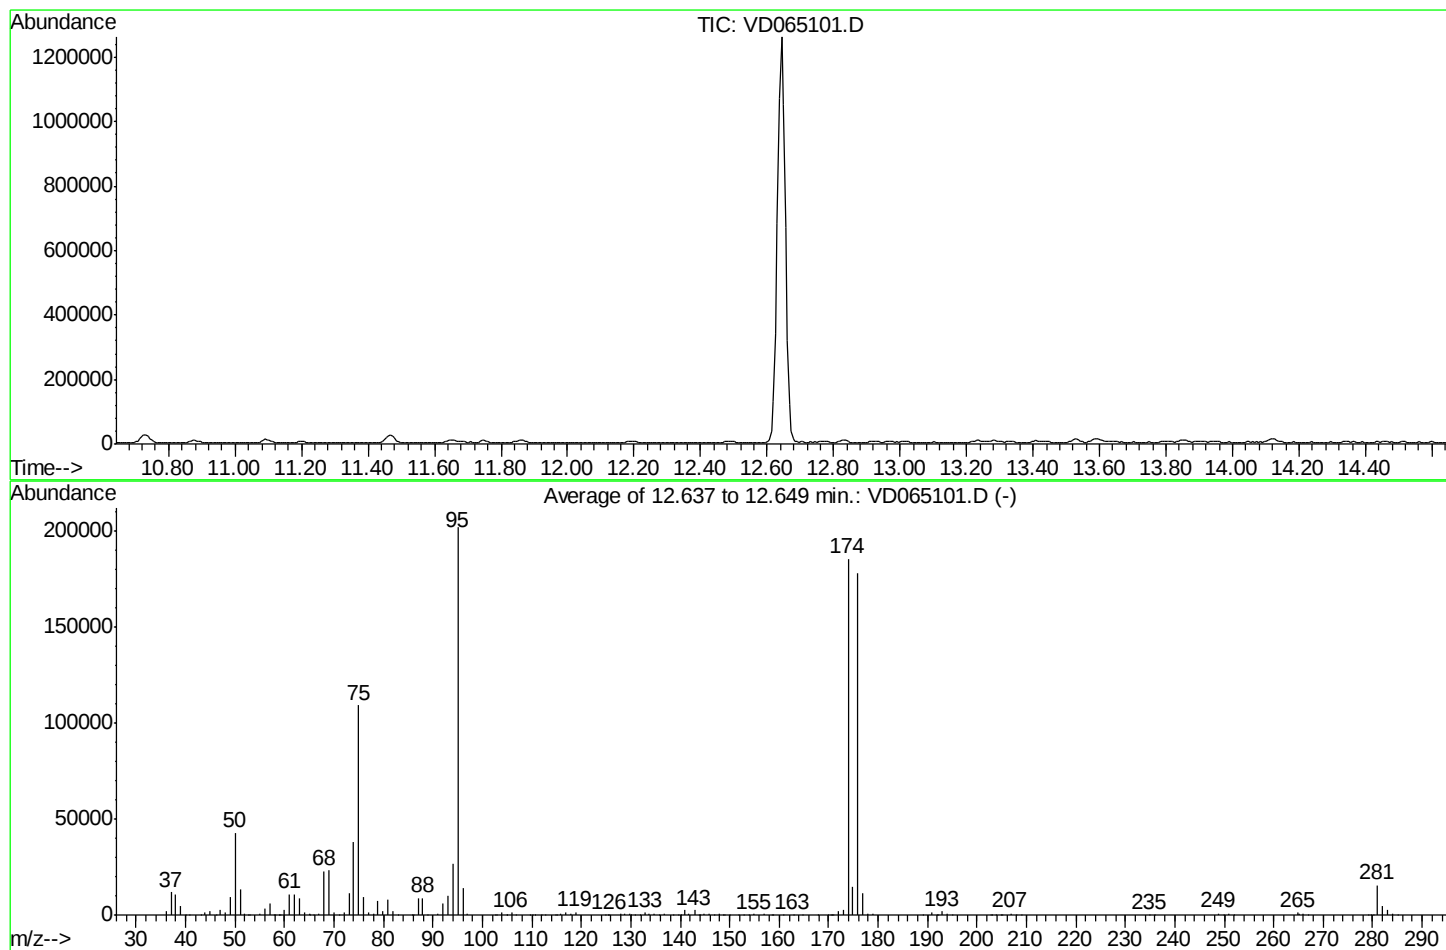

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	42962	PASS
75	95	30	60	54.1	109408	PASS
95	95	100	100	100.0	202112	PASS
96	95	5	9	7.0	14210	PASS
173	174	0.00	2	1.5	2699	PASS
174	95	50	100	92.0	185877	PASS
175	174	5	9	7.9	14762	PASS
176	174	95	101	96.0	178389	PASS
177	176	5	9	6.2	11113	PASS