
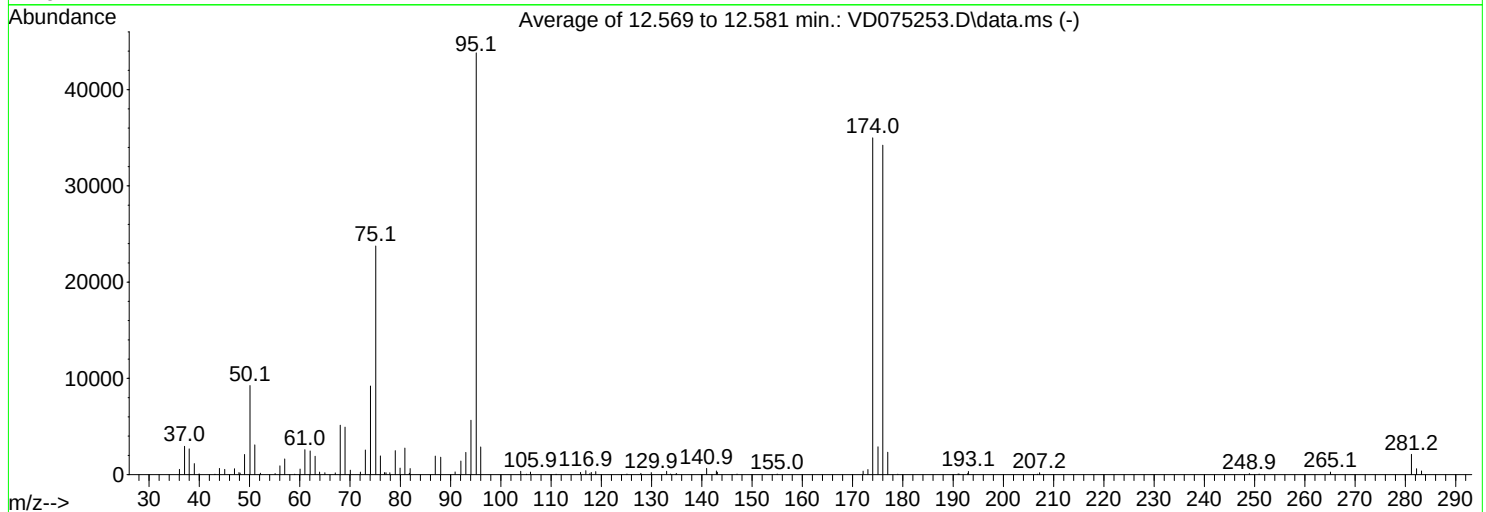


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD0723\
Data File : VD075253.D
Acq On : 07 Feb 2023 08:55
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020723S.M
Title : SW846 8260
Last Update : Wed Feb 08 04:26:58 2023

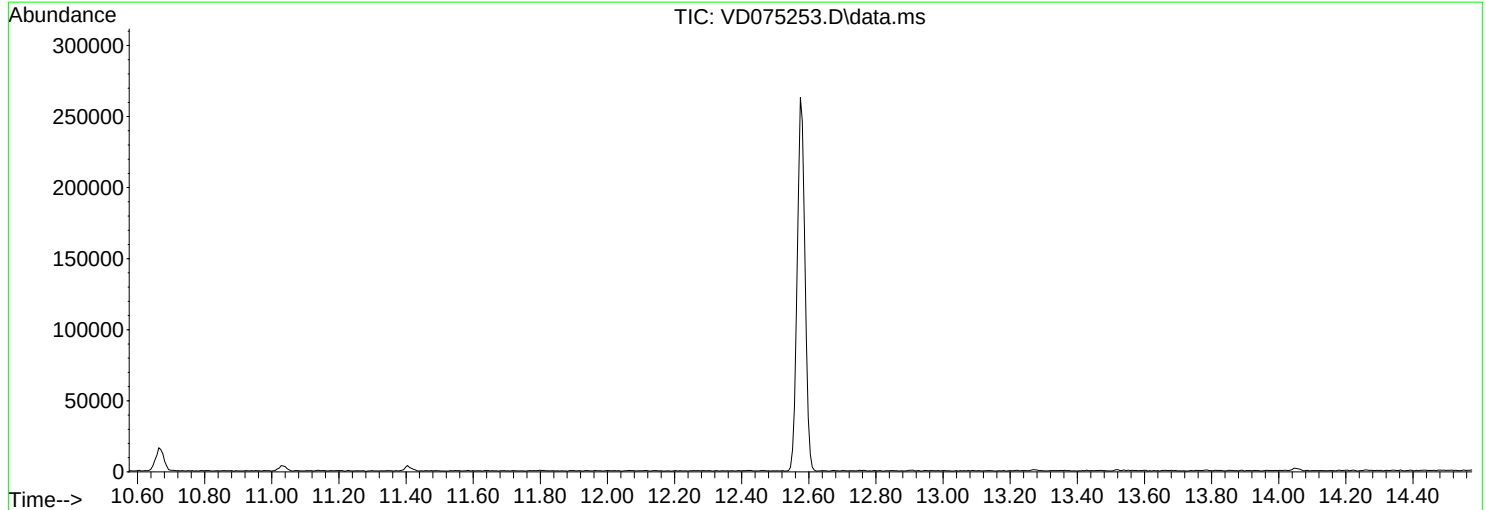

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.1	9260	PASS
75	95	30	60	54.2	23749	PASS
95	95	100	100	100.0	43821	PASS
96	95	5	9	6.6	2883	PASS
173	174	0.00	2	1.5	537	PASS
174	95	50	100	79.9	34995	PASS
175	174	5	9	8.3	2899	PASS
176	174	95	101	97.8	34224	PASS
177	176	5	9	6.8	2331	PASS