

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020921\
 Data File : VD068333.D
 Acq On : 09 Feb 2021 17:13
 Operator : VA/SY
 Sample : M1345-01
 Misc : 6.02G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 NB-07-020921

Quant Time: Feb 10 00:18:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 13:19:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.985	168	461455	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	848844	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	749128	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	299323	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.338	65	271031	61.40	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.80%
35) Dibromofluoromethane	7.920	113	259388	55.27	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.54%
50) Toluene-d8	10.344	98	1047627	55.81	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	111.62%
62) 4-Bromofluorobenzene	12.632	95	326225	48.26	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.52%
Target Compounds						
95) Naphthalene	15.396	128	20306	1.80	ug/l	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020921\
Data File : VD068333.D
Acq On : 09 Feb 2021 17:13
Operator : VA/SY
Sample : M1345-01
Misc : 6.02G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
NB-07-020921

Quant Time: Feb 10 00:18:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 19 13:19:08 2021
Response via : Initial Calibration




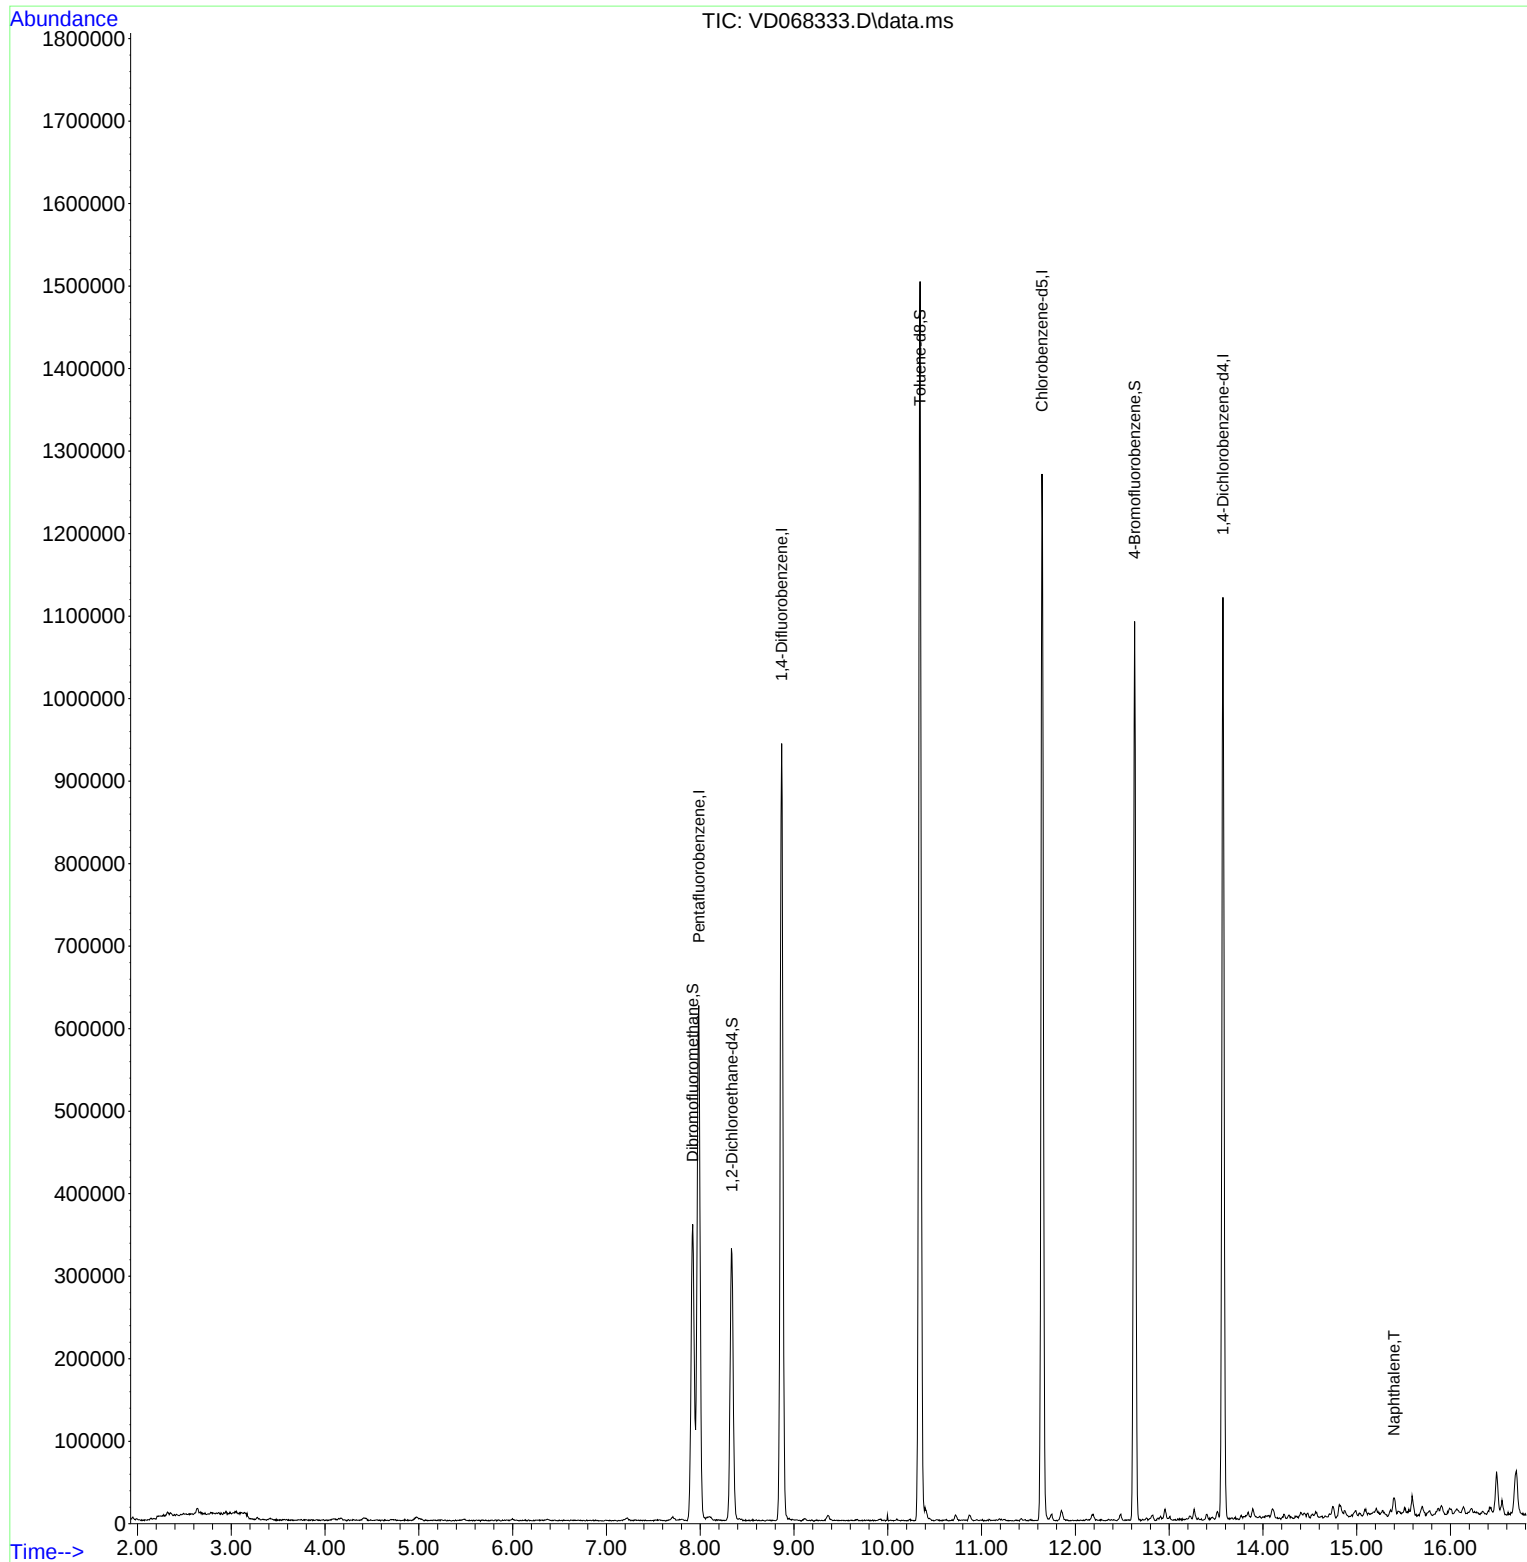




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. -0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13




Instrument :
MSVOA_D
ClientSampleId :
NB-07-020921

Tgt Ion:168 Resp: 461455
Ion Ratio Lower Upper
168 100
99 60.7 43.5 65.3

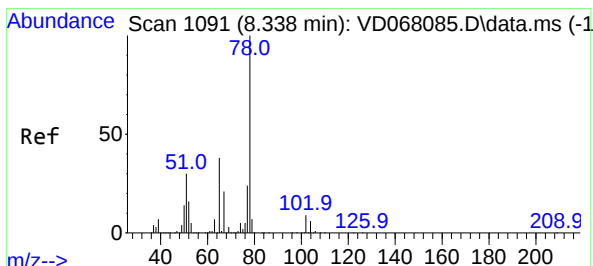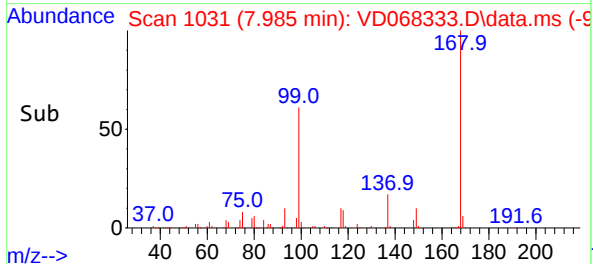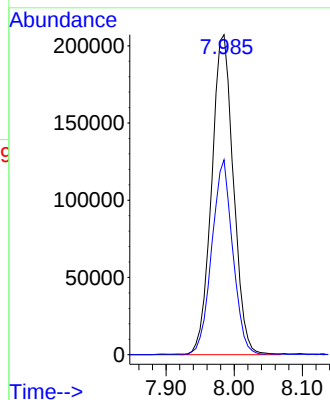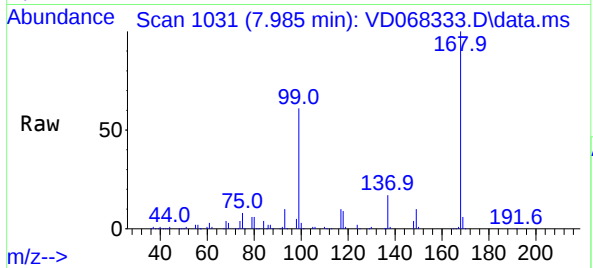

#33
1,2-Dichloroethane-d4
Concen: 61.40 ug/l
RT: 8.338 min Scan# 1091
Delta R.T. 0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13

Tgt Ion: 65 Resp: 271031
Ion Ratio Lower Upper
65 100
67 52.5 0.0 105.0

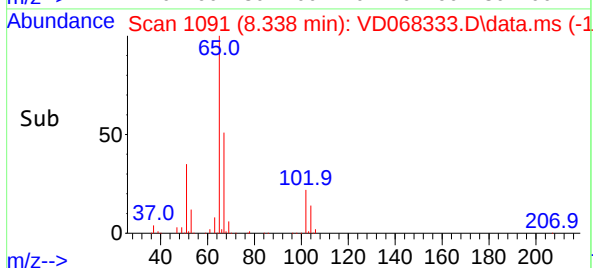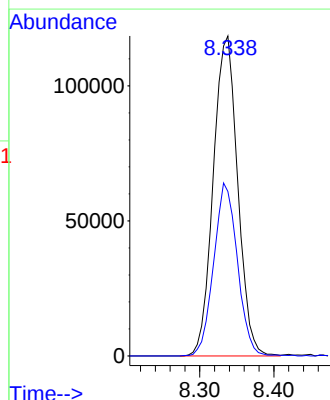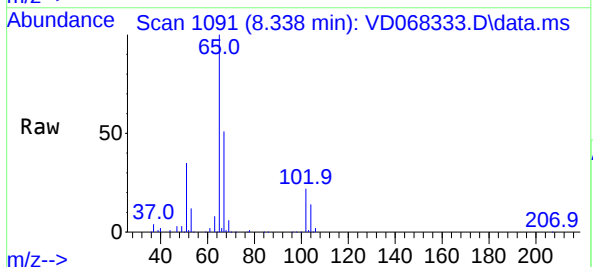







#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13

Instrument :
MSVOA_D
ClientSampleId :
NB-07-020921

Tgt Ion:114 Resp: 848844




Ion	Ratio	Lower	Upper
114	100		
63	19.3	0.0	34.8
88	15.7	0.0	31.6

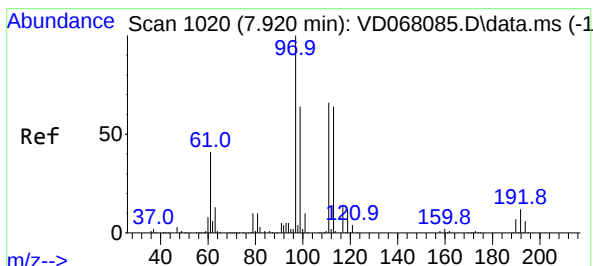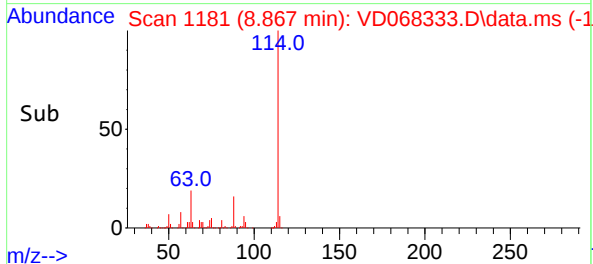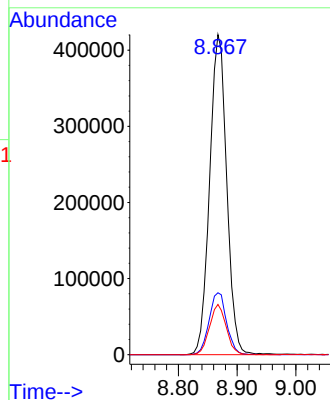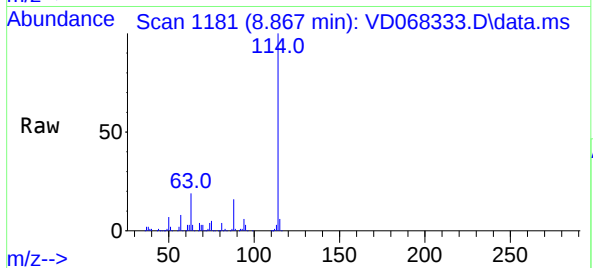


#35
Dibromofluoromethane
Concen: 55.27 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13

Tgt Ion:113 Resp: 259388

Ion	Ratio	Lower	Upper
113	100		
111	103.2	81.4	122.0
192	18.7	16.1	24.1


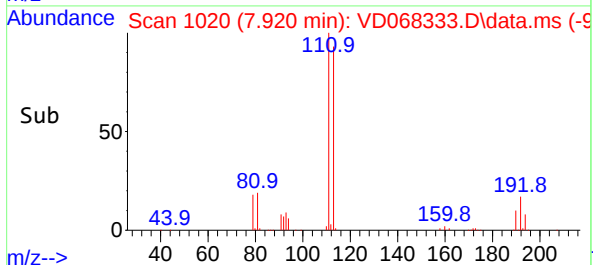
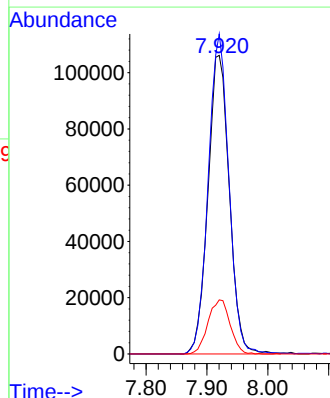
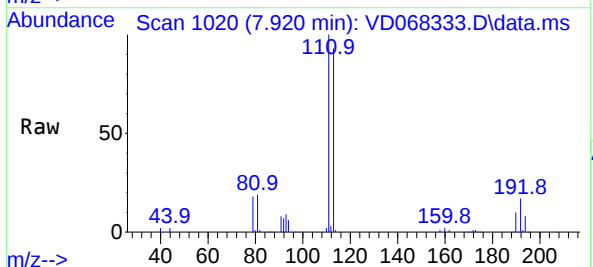


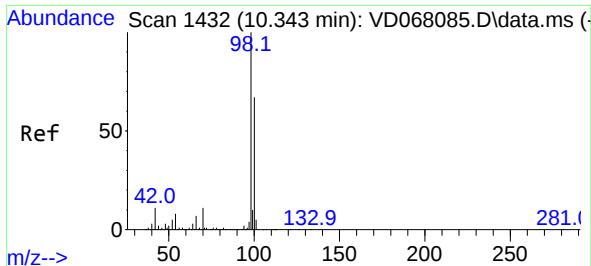

#50
Toluene-d8
Concen: 55.81 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. 0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13




Instrument :
MSVOA_D
ClientSampleId :
NB-07-020921

Tgt Ion: 98 Resp: 1047627
Ion Ratio Lower Upper
98 100
100 65.4 53.0 79.4

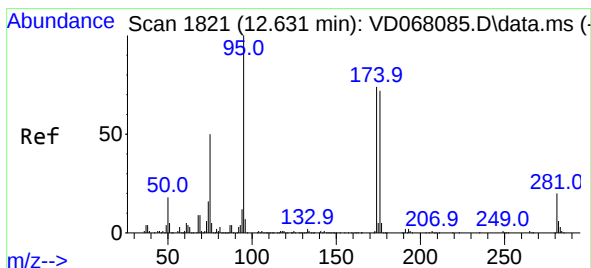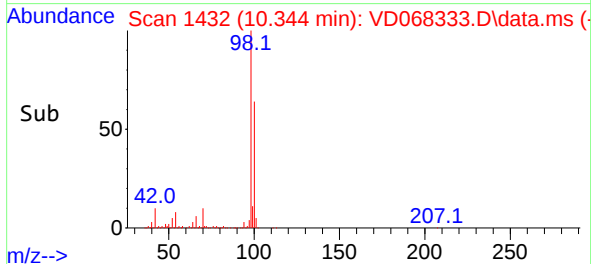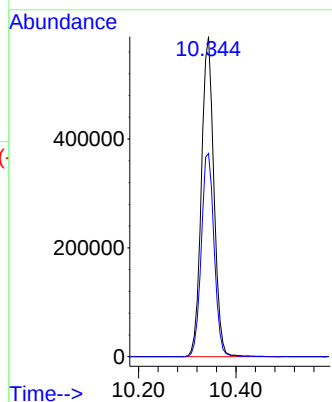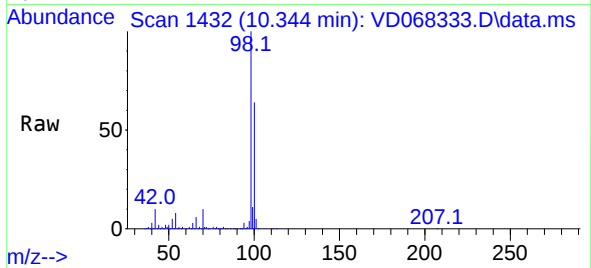

#62
4-Bromofluorobenzene
Concen: 48.26 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13


Tgt Ion: 95 Resp: 326225
Ion Ratio Lower Upper
95 100
174 77.8 0.0 172.4
176 75.9 0.0 168.4

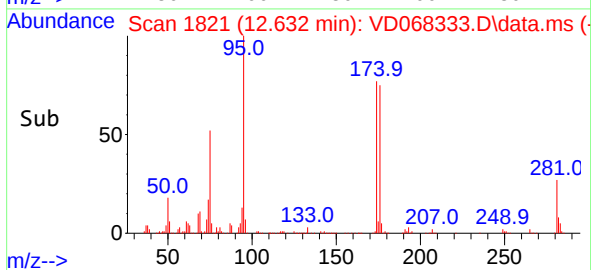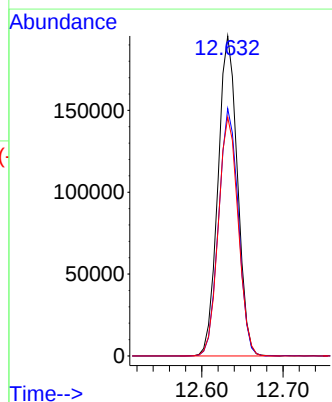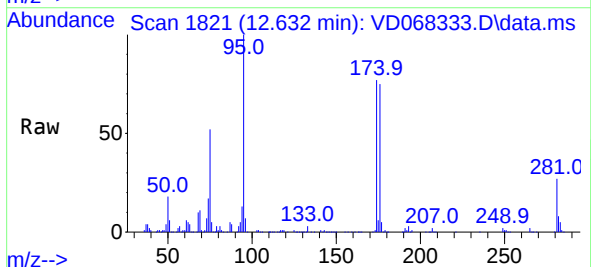






#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. -0.005 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13

Instrument :
MSVOA_D
ClientSampleId :
NB-07-020921

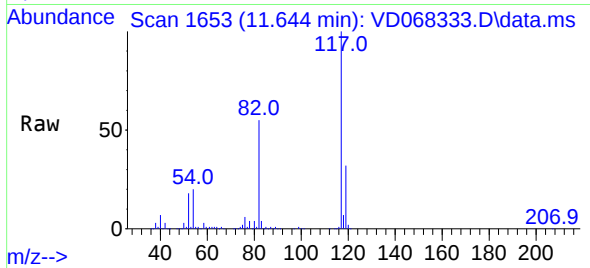


Tgt Ion:117 Resp: 749128

Ion	Ratio	Lower	Upper
117	100		
82	54.9	41.4	62.0
119	32.4	26.1	39.1

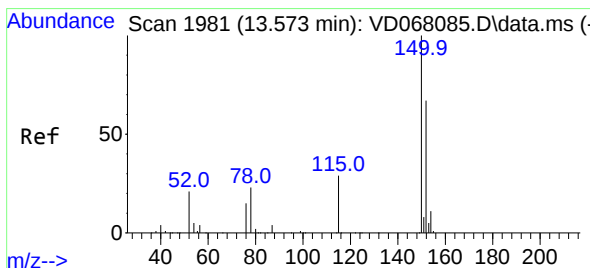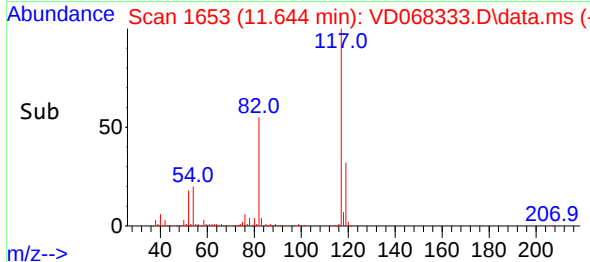
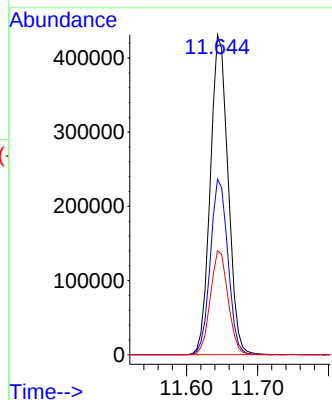



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.000 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13

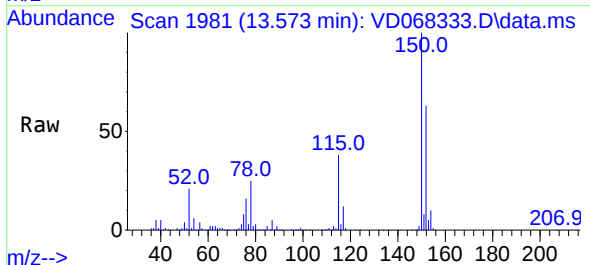

Tgt Ion:152 Resp: 299323

Ion	Ratio	Lower	Upper
152	100		
115	59.0	28.9	86.8
150	157.6	0.0	344.4

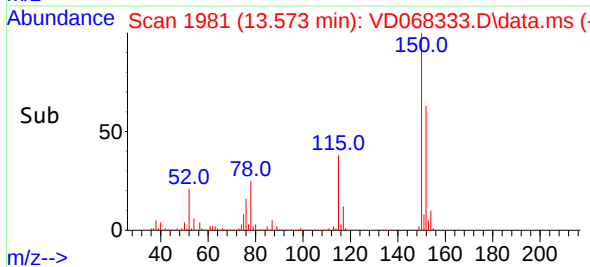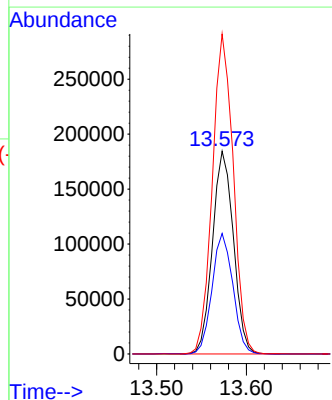

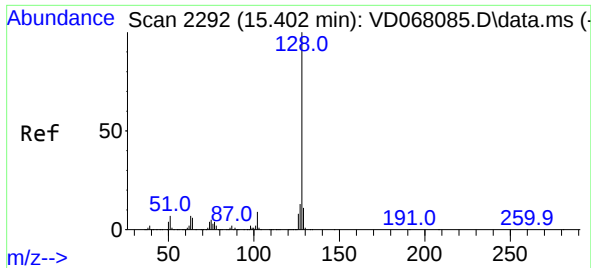

#95
Naphthalene
Concen: 1.80 ug/l
RT: 15.396 min Scan# 2291
Delta R.T. -0.006 min
Lab File: VD068333.D
Acq: 09 Feb 2021 17:13

Instrument :
MSVOA_D
ClientSampleId :
NB-07-020921

Tgt Ion:	128	Resp:	20306
Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.2	15.2
129	12.2	8.8	13.2

