
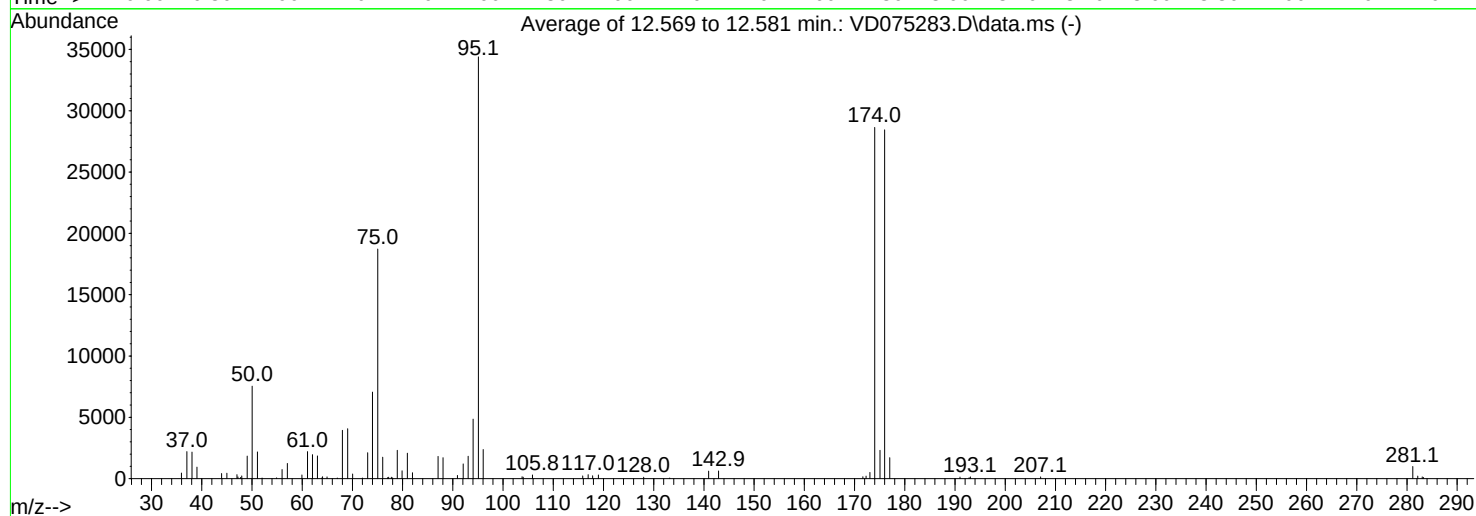


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020923\
Data File : VD075283.D
Acq On : 09 Feb 2023 09:12
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020723S.M
Title : SW846 8260
Last Update : Wed Feb 08 04:26:58 2023

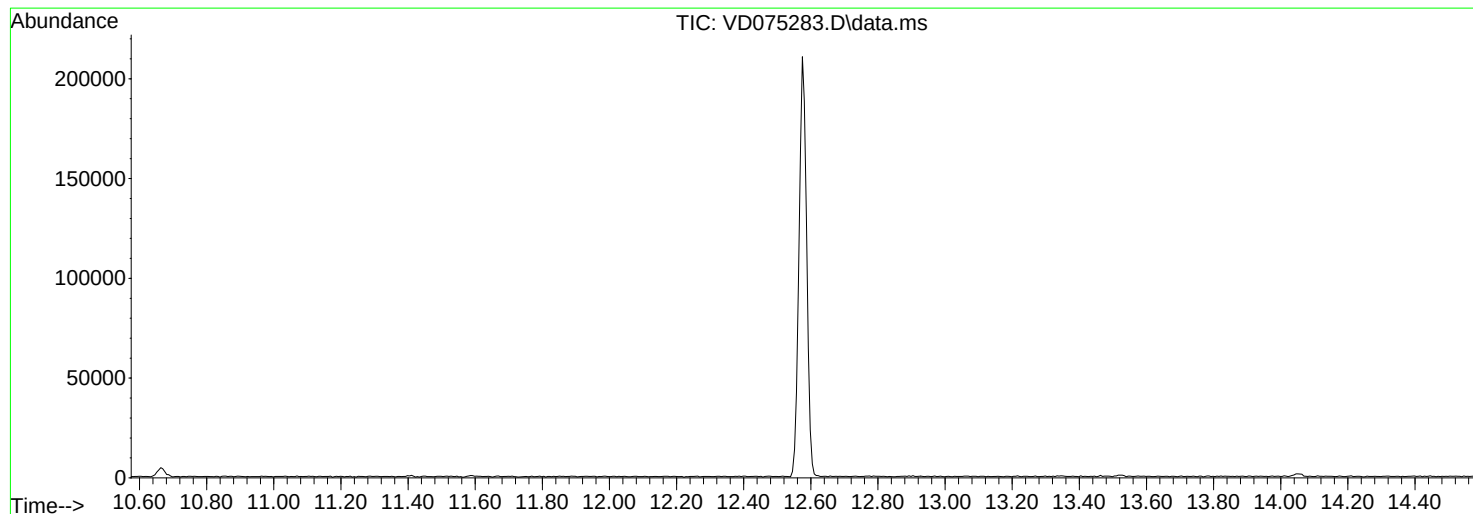

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	7541	PASS
75	95	30	60	54.4	18722	PASS
95	95	100	100	100.0	34392	PASS
96	95	5	9	6.9	2372	PASS
173	174	0.00	2	1.8	507	PASS
174	95	50	100	83.3	28640	PASS
175	174	5	9	8.1	2312	PASS
176	174	95	101	99.3	28445	PASS
177	176	5	9	6.0	1707	PASS