

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD021120\
 Data File : VD065142.D
 Acq On : 11 Feb 2020 11:10
 Operator : VA/SY
 Sample : VD0211SBL01
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0211SBL01

Quant Time: Feb 12 07:10:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D020520S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 05 15:53:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	489583	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	797570	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	833003	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	419947	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	229124	55.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.12%	
35) Dibromofluoromethane	7.92	113	248129	55.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.52%	
50) Toluene-d8	10.34	98	973953	54.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.98%	
62) 4-Bromofluorobenzene	12.64	95	372332	66.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	132.68%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD021120\
Data File : VD065142.D
Acq On : 11 Feb 2020 11:10
Operator : VA/SY
Sample : VD0211SBL01
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0211SBL01

Quant Time: Feb 12 07:10:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D020520S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 05 15:53:00 2020
Response via : Initial Calibration




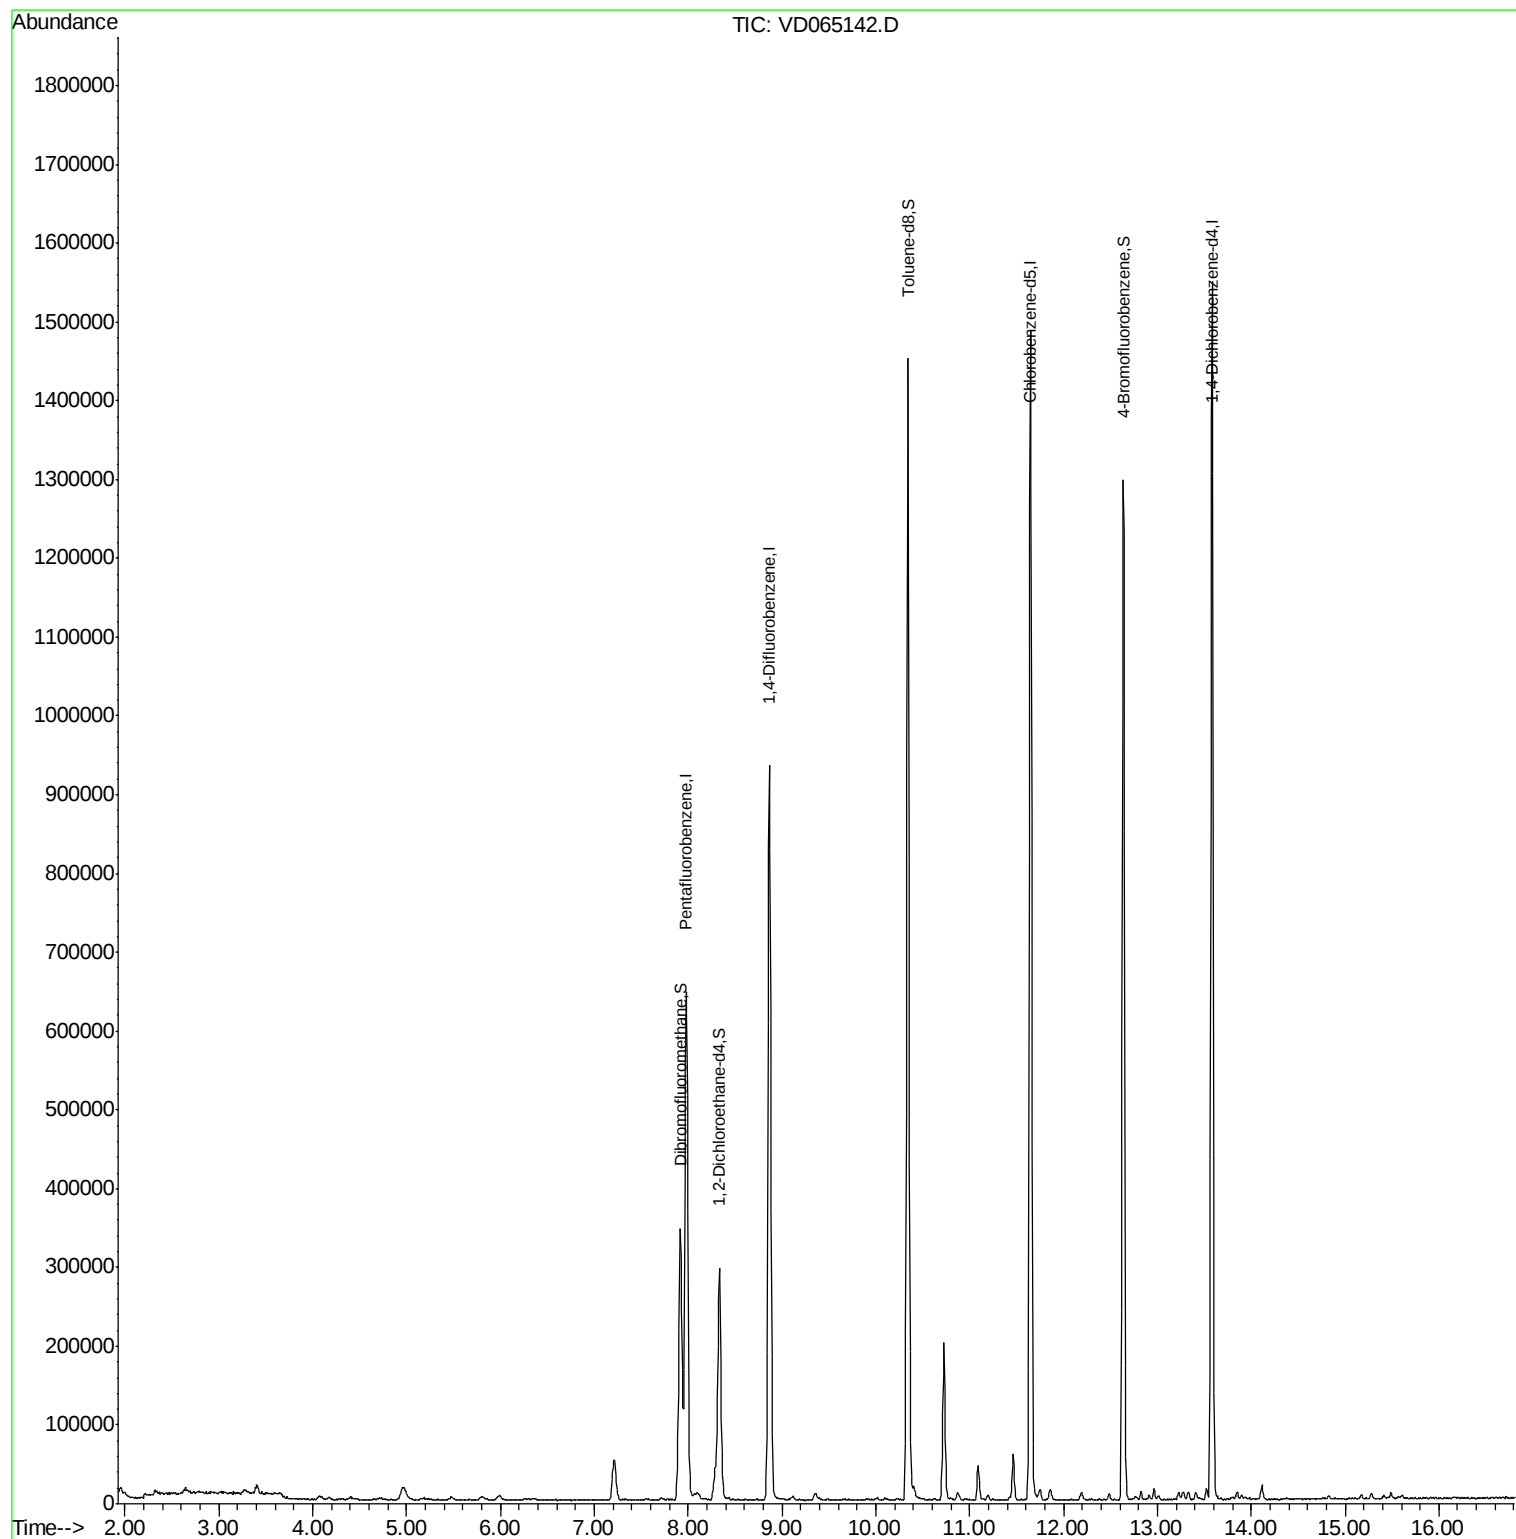




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.98 min Scan# 1030
Delta R.T. -0.01 min
Lab File: VD065142.D
Acq: 11 Feb 2020 11:10




Instrument :
MSVOA_D
ClientSampleId :
VD0211SBL01


Tot Ion:168 Resp: 489583
Ion Ratio Lower Upper
168 100
99 54.1 41.0 61.6

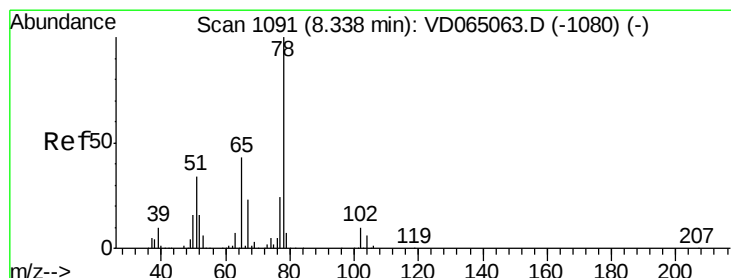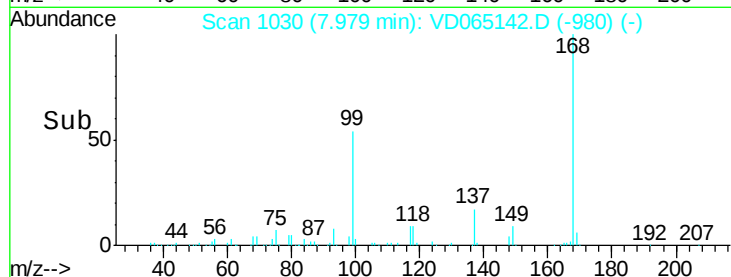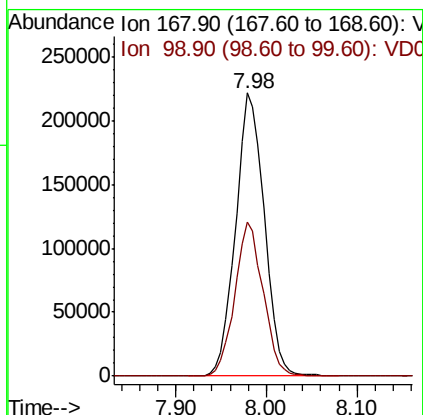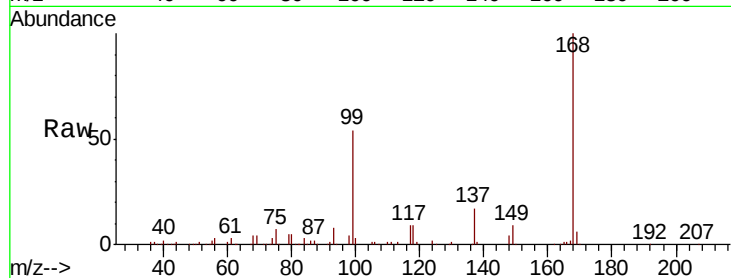

#33
1,2-Dichloroethane-d4
Concen: 55.064 ug/l
RT: 8.33 min Scan# 1090
Delta R.T. -0.01 min
Lab File: VD065142.D
Acq: 11 Feb 2020 11:10

Tgt Ion: 65 Resp: 229124
Ion Ratio Lower Upper
65 100
67 53.4 0.0 105.8

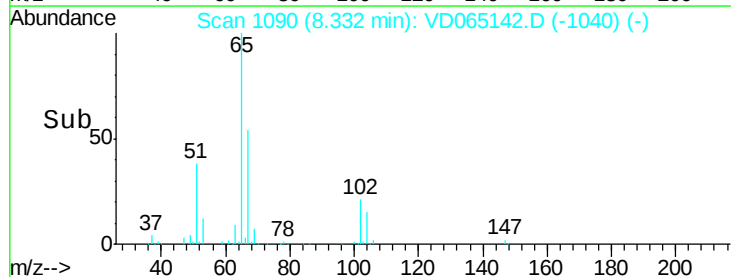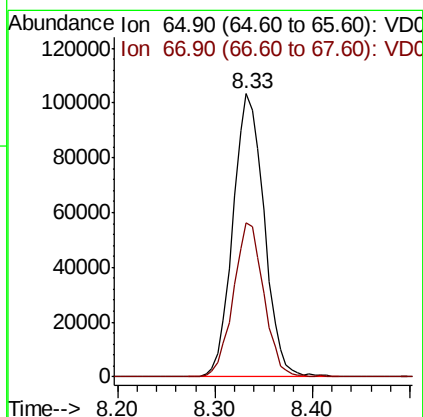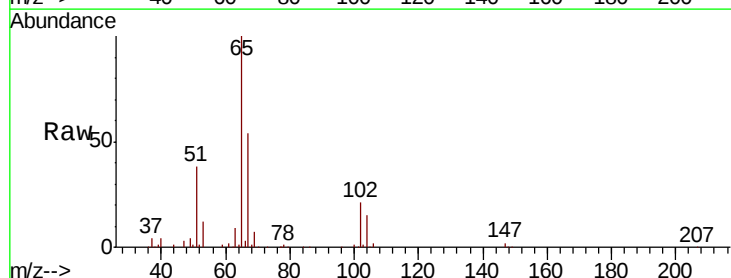


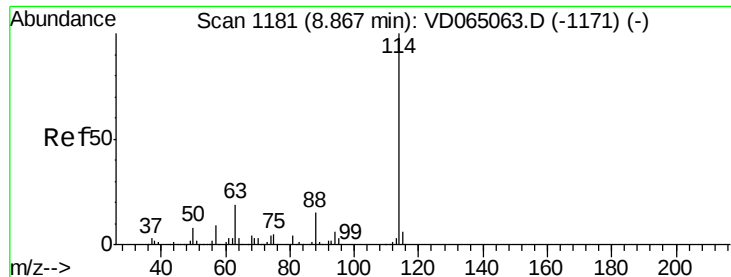




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. -0.00 min
 Lab File: VD065142.D
 Acq: 11 Feb 2020 11:10

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0211SBL01

Tot Ion	Ratio	Lower	Upper
114	100		
63	20.4	0.0	38.8
88	15.4	0.0	29.6

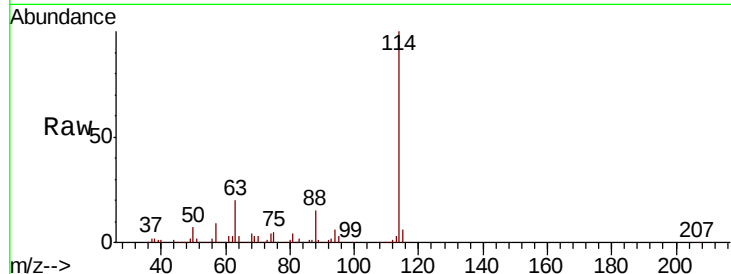


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VDC
 Ion 87.90 (87.60 to 88.60): VDC

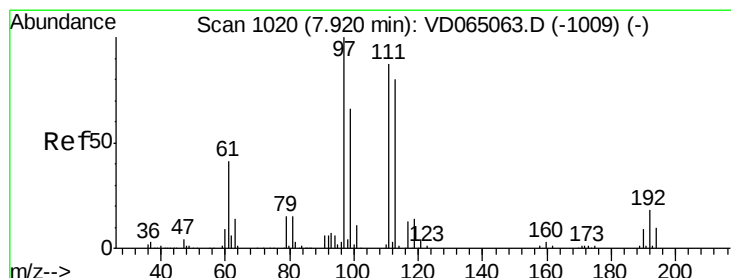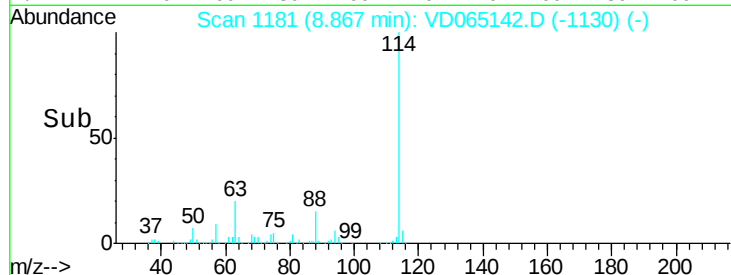
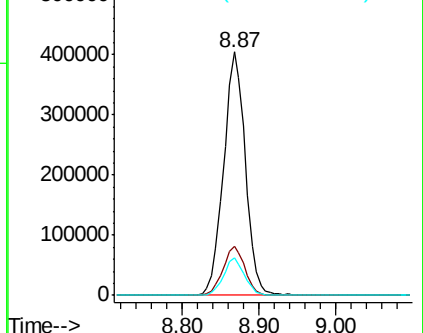



#35
 Dibromofluoromethane
 Concen: 55.760 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. -0.00 min
 Lab File: VD065142.D
 Acq: 11 Feb 2020 11:10

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.1	83.1	124.7
192	22.0	18.1	27.1

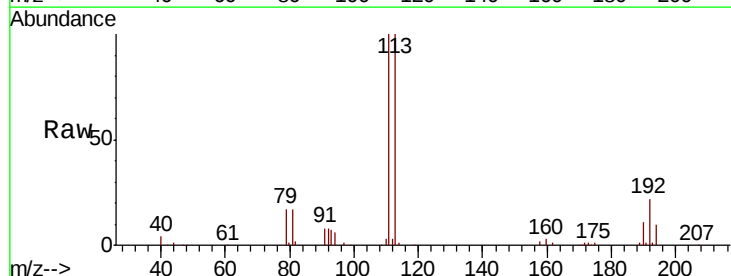

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

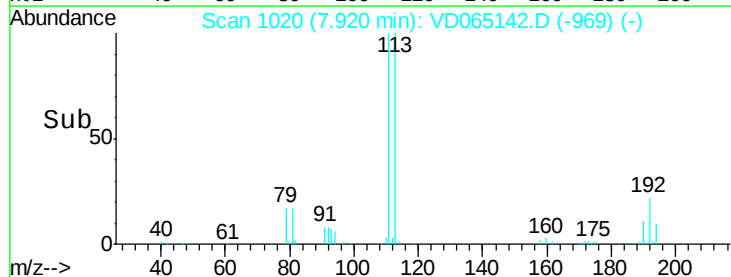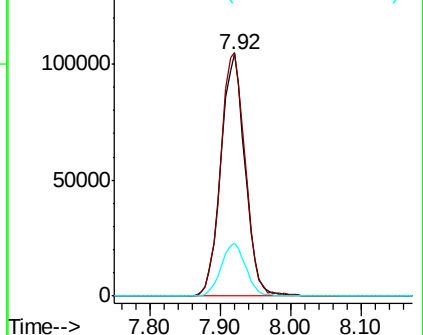

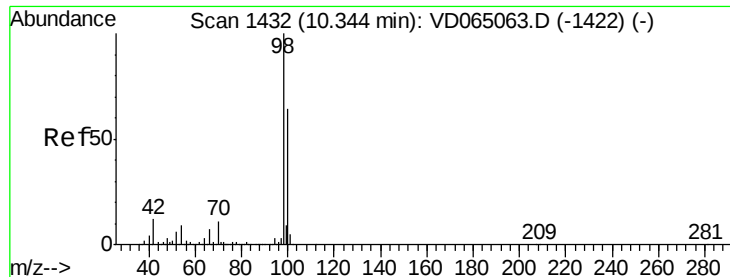

#50

Toluene-d8

Concen: 54.988 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. -0.00 min

Lab File: VD065142.D

Acq: 11 Feb 2020 11:10

Instrument :

MSVOA_D

ClientSampleId :


VD0211SBL01

Tot Ion: 98 Resp: 973953

Ion Ratio Lower Upper

98 100

100 65.5 52.1 78.1

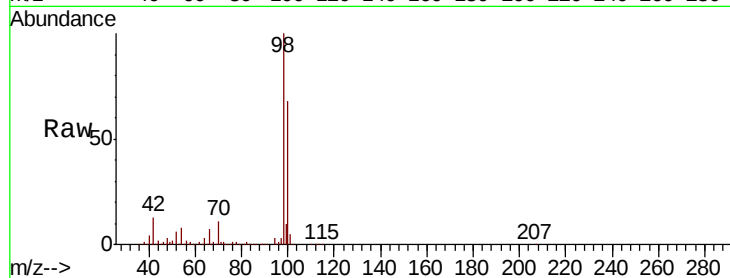

Abundance Ion 98.00 (97.70 to 98.70): VDC

Ion 100.00 (99.70 to 100.70): VDC

10.34

600000

500000

400000



300000

200000

100000

0

Time--> 10.20 10.30 10.40 10.50

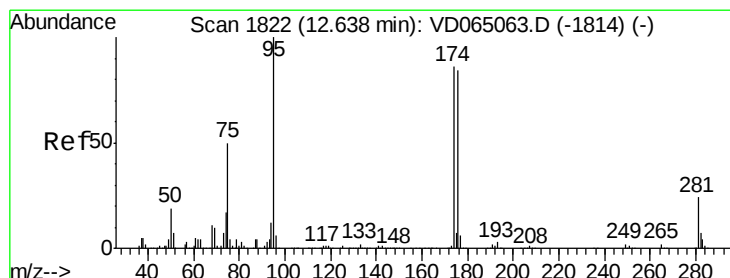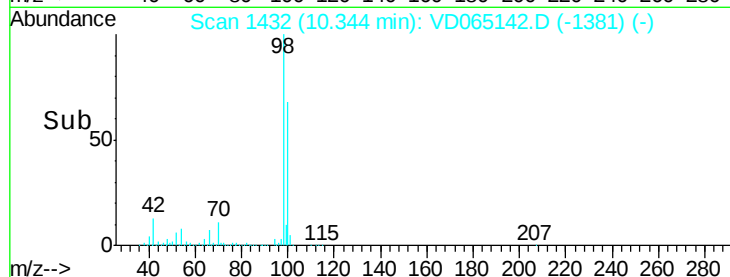

#62

4-Bromofluorobenzene

Concen: 66.342 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. -0.00 min

Lab File: VD065142.D

Acq: 11 Feb 2020 11:10


Tgt Ion: 95 Resp: 372332

Ion Ratio Lower Upper

95 100

174 90.4 0.0 180.0

176 86.3 0.0 173.2

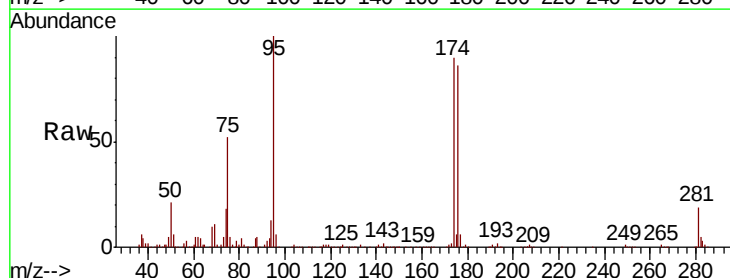

Abundance Ion 94.90 (94.60 to 95.60): VDC

Ion 173.80 (173.50 to 174.50): VDC

Ion 175.80 (175.50 to 176.50): VDC

12.64

300000

250000

200000


150000


100000

50000

0

Time--> 12.60 12.70




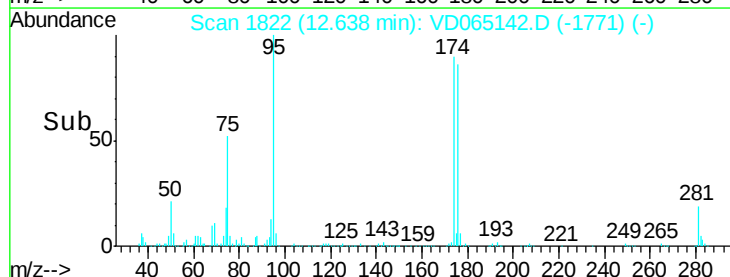


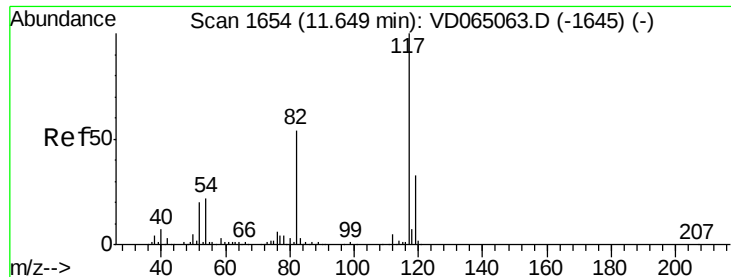

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD065142.D
Acq: 11 Feb 2020 11:10

Instrument :
MSVOA_D
ClientSampleId :
VD0211SBL01

Tot Ion:117 Resp: 833003
Ion Ratio Lower Upper
117 100
82 54.8 43.1 64.7
119 32.1 26.0 39.0

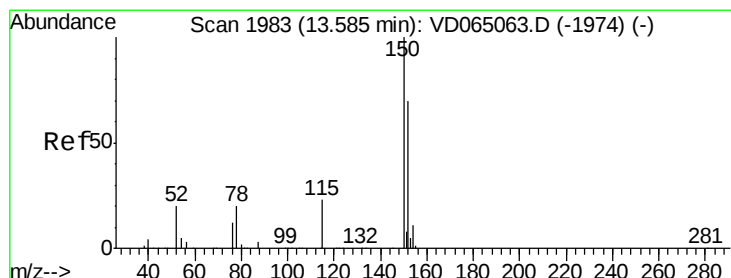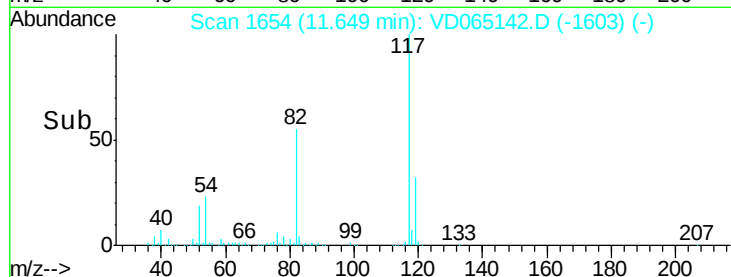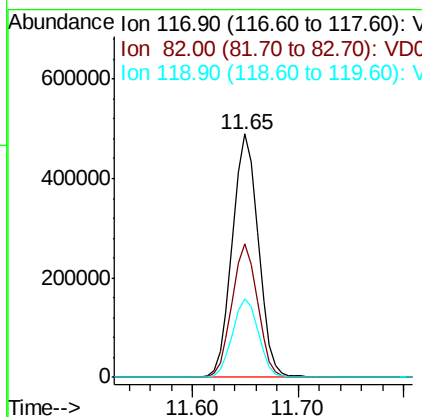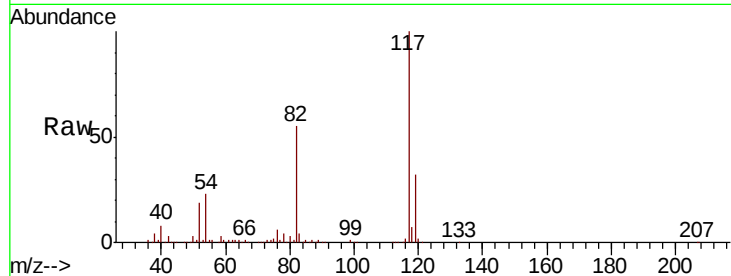

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. -0.00 min
Lab File: VD065142.D
Acq: 11 Feb 2020 11:10

Tgt Ion:152 Resp: 419947
Ion Ratio Lower Upper
152 100
115 55.2 27.5 82.4
150 155.1 0.0 343.2

