


Methylene Chloride

Response Ratio

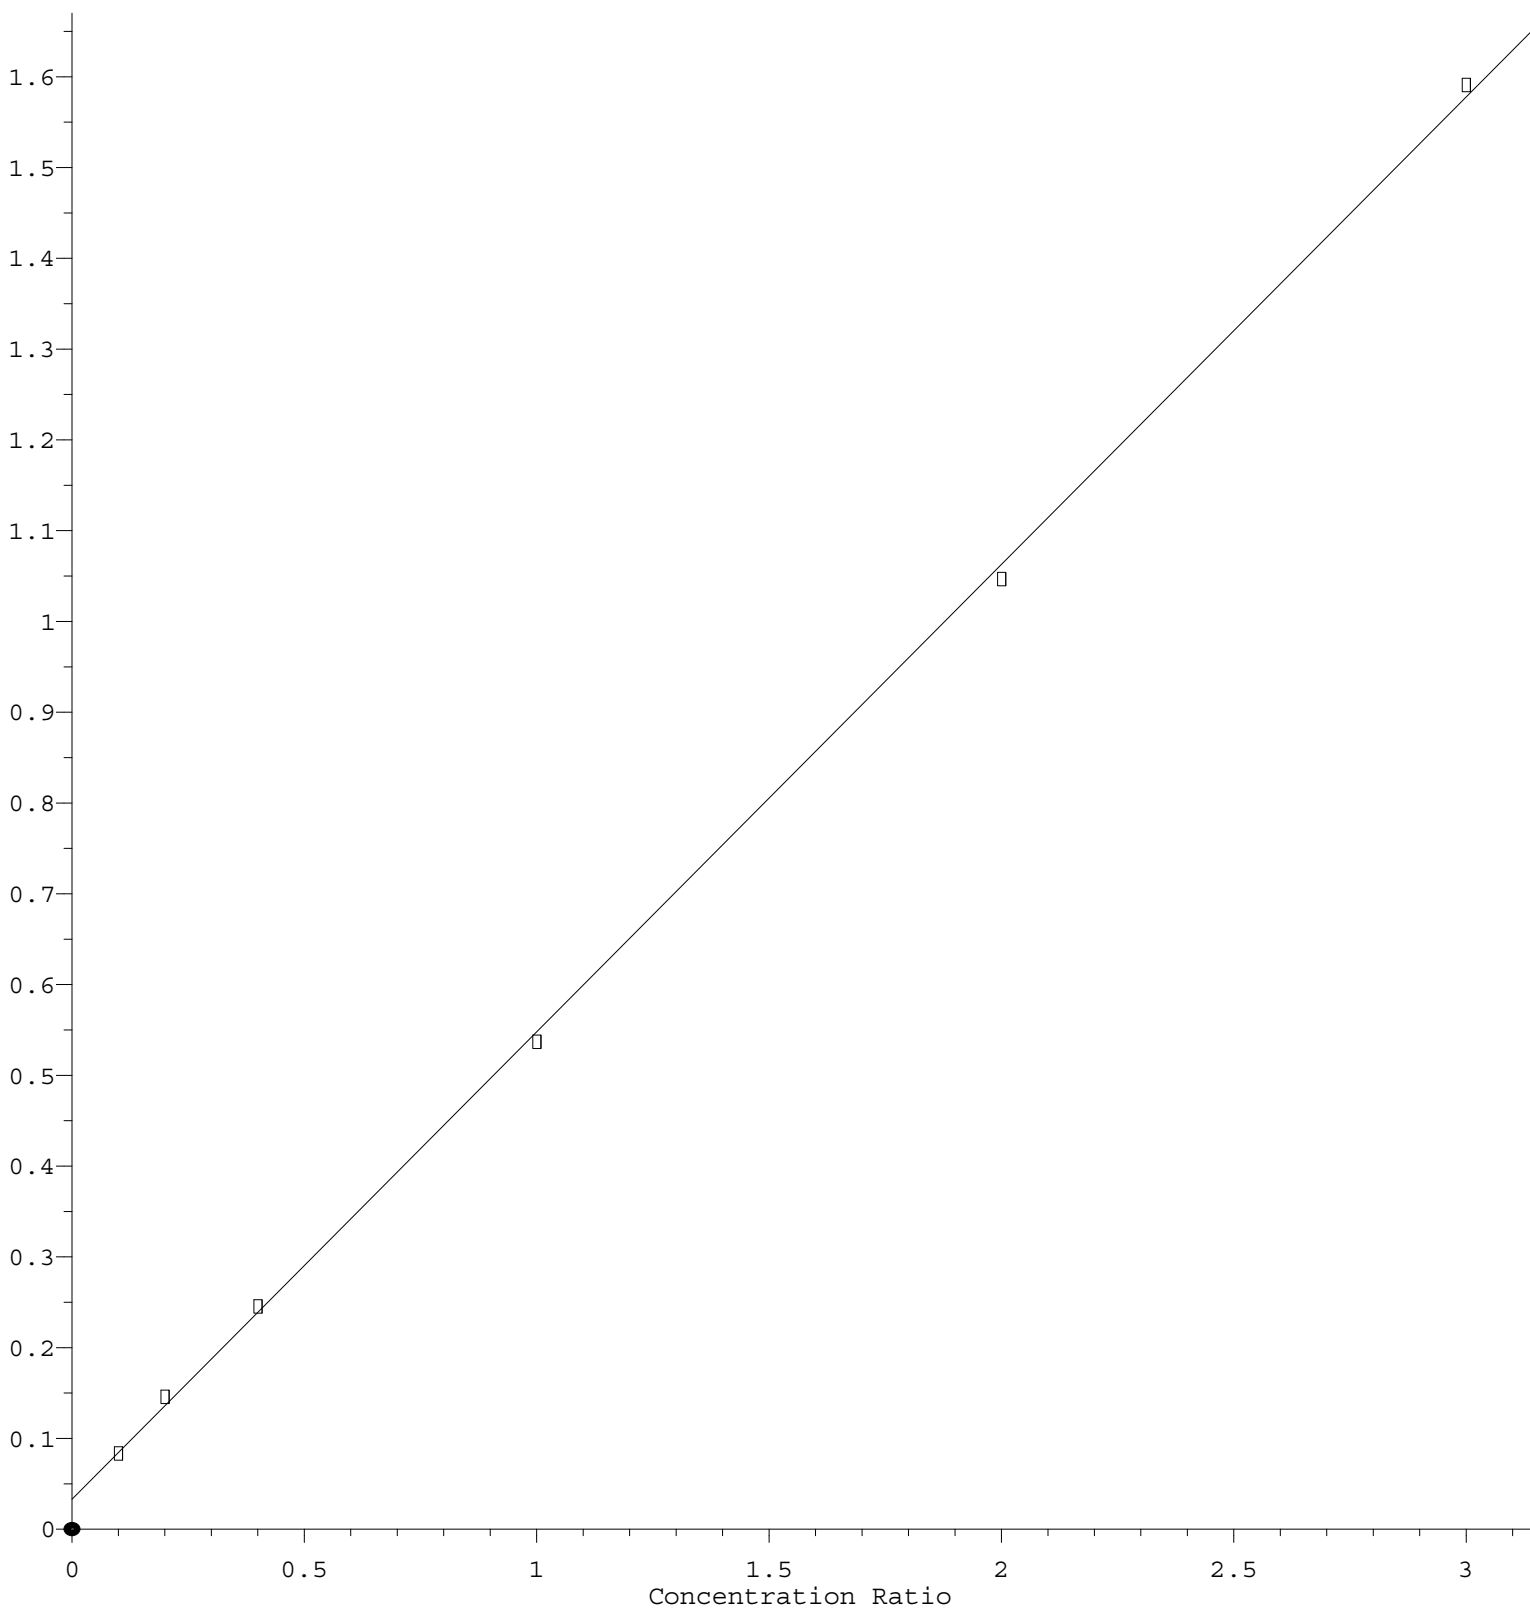

$$\text{Response} = 5.148\text{e-}001 * \text{Amt} + 3.324\text{e-}002$$


Coef of Det (r^2) = 0.999607 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D021221S.M

Calibration Table Last Updated: Fri Feb 12 13:30:51 2021

Cyclohexane

Response Ratio

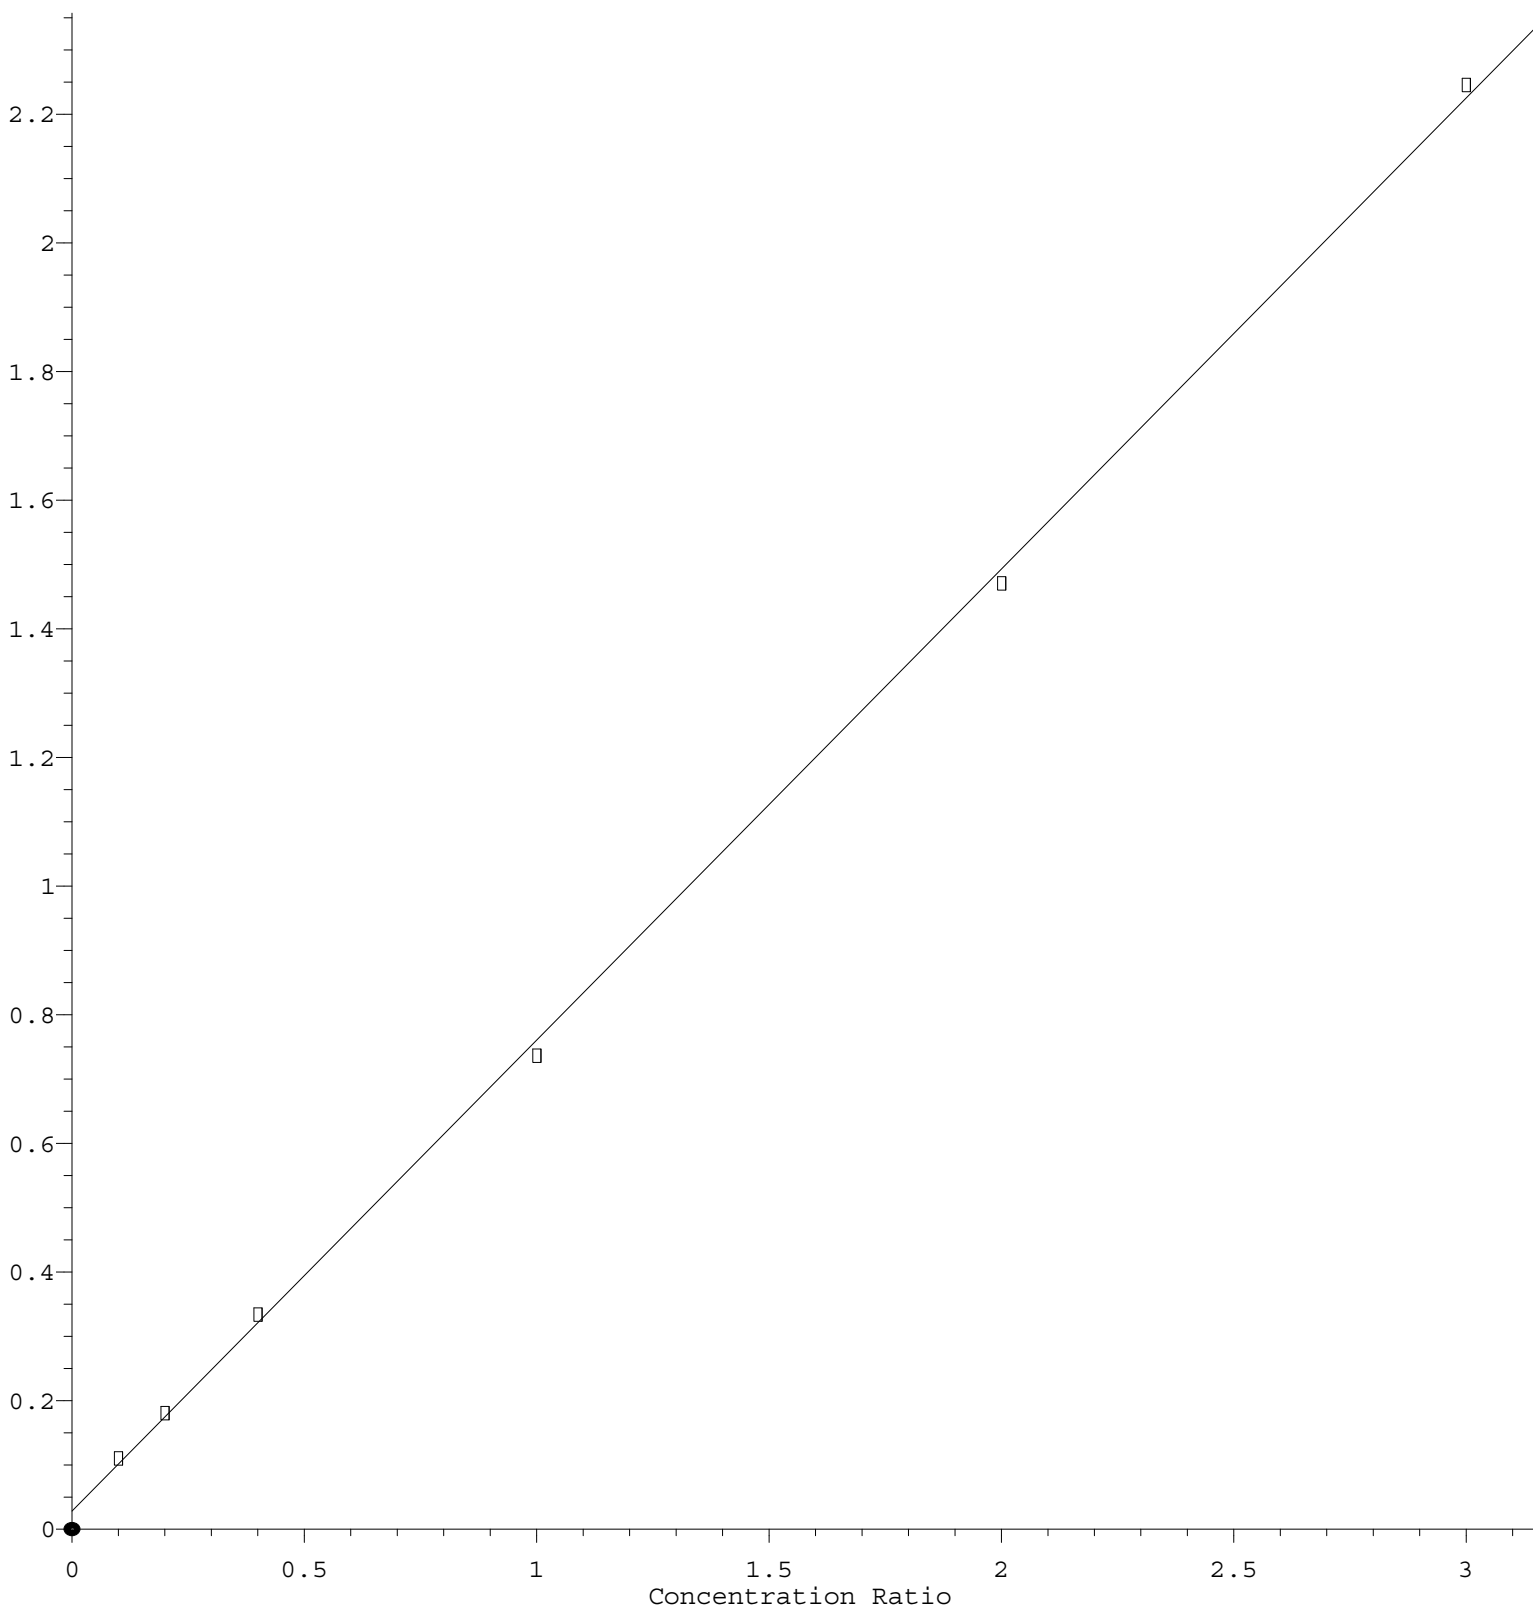

$$\text{Response} = 7.321\text{e-}001 * \text{Amt} + 2.848\text{e-}002$$

Coef of Det (r^2) = 0.999511 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D021221S.M

Calibration Table Last Updated: Fri Feb 12 13:30:51 2021