


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD021420\
Data File : VD065183.D
Acq On : 14 Feb 2020 09:30
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D020520S.M
Title : SW846 8260
Last Update : Wed Feb 05 15:53:00 2020

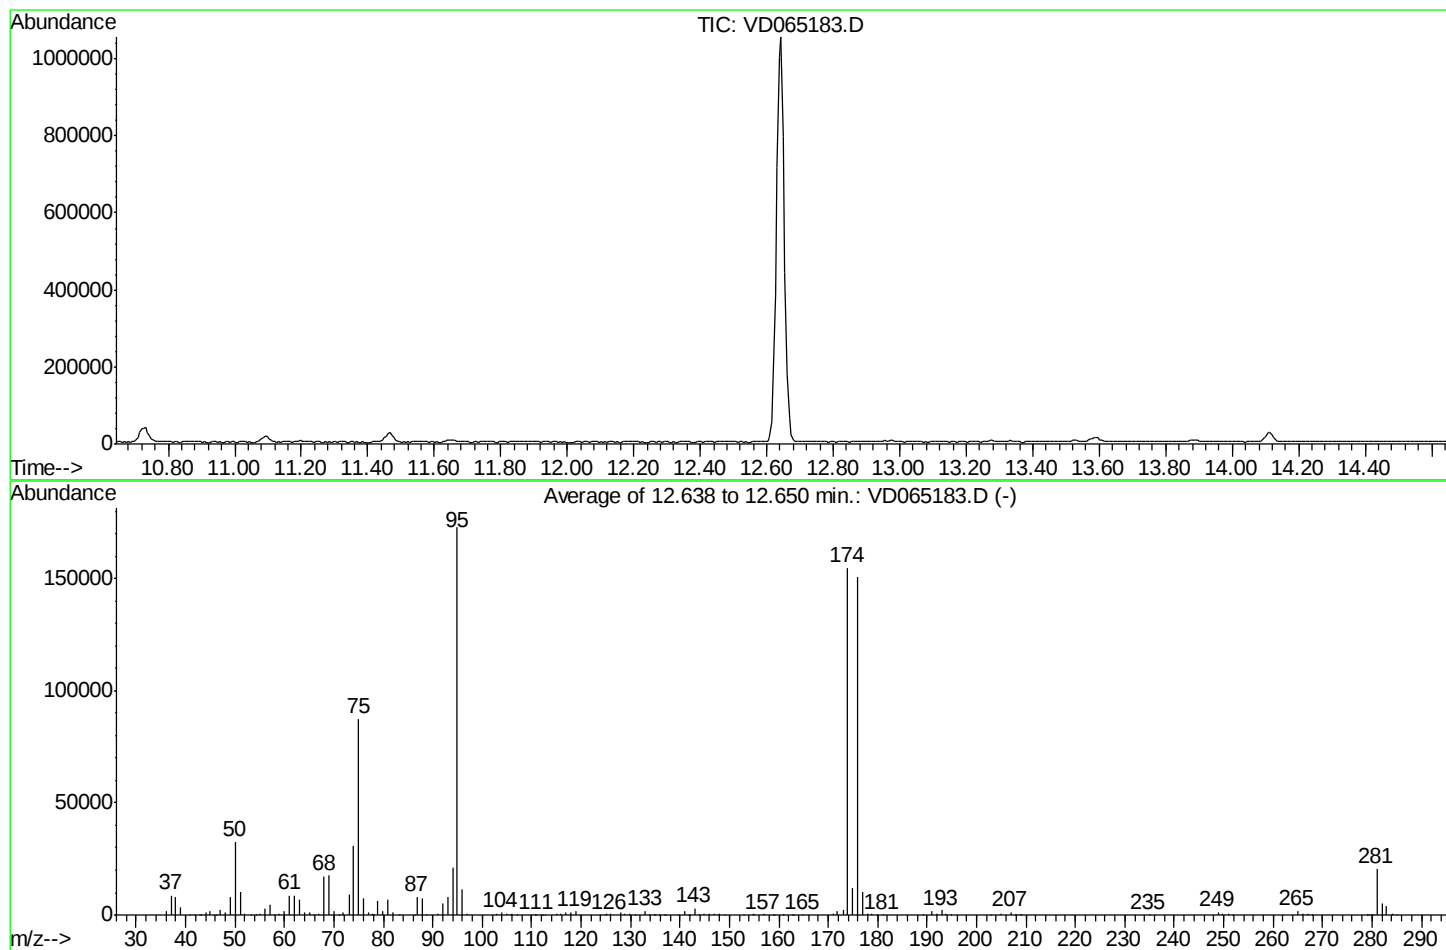

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	32824	PASS
75	95	30	60	50.7	87538	PASS
95	95	100	100	100.0	172800	PASS
96	95	5	9	6.5	11201	PASS
173	174	0.00	2	1.4	2201	PASS
174	95	50	100	89.6	154773	PASS
175	174	5	9	7.6	11781	PASS
176	174	95	101	97.2	150421	PASS
177	176	5	9	7.0	10470	PASS