
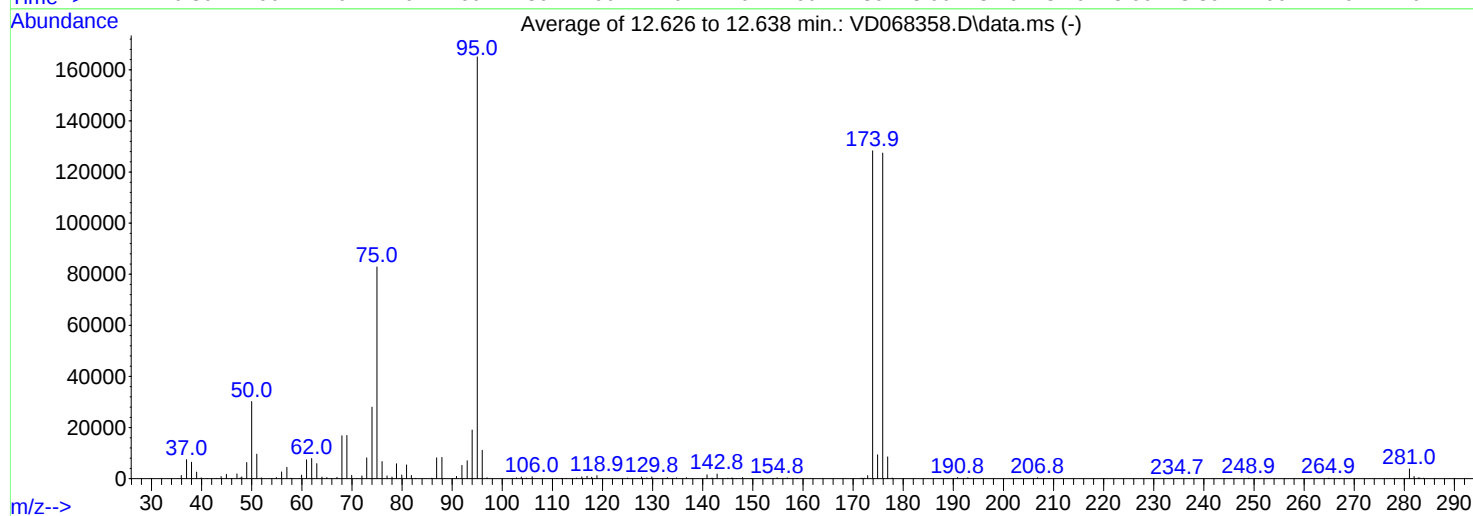


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021521\
 Data File : VD068358.D
 Acq On : 15 Feb 2021 12:51
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D0212215.M
 Title : SW846 8260
 Last Update : Fri Feb 12 13:30:51 2021

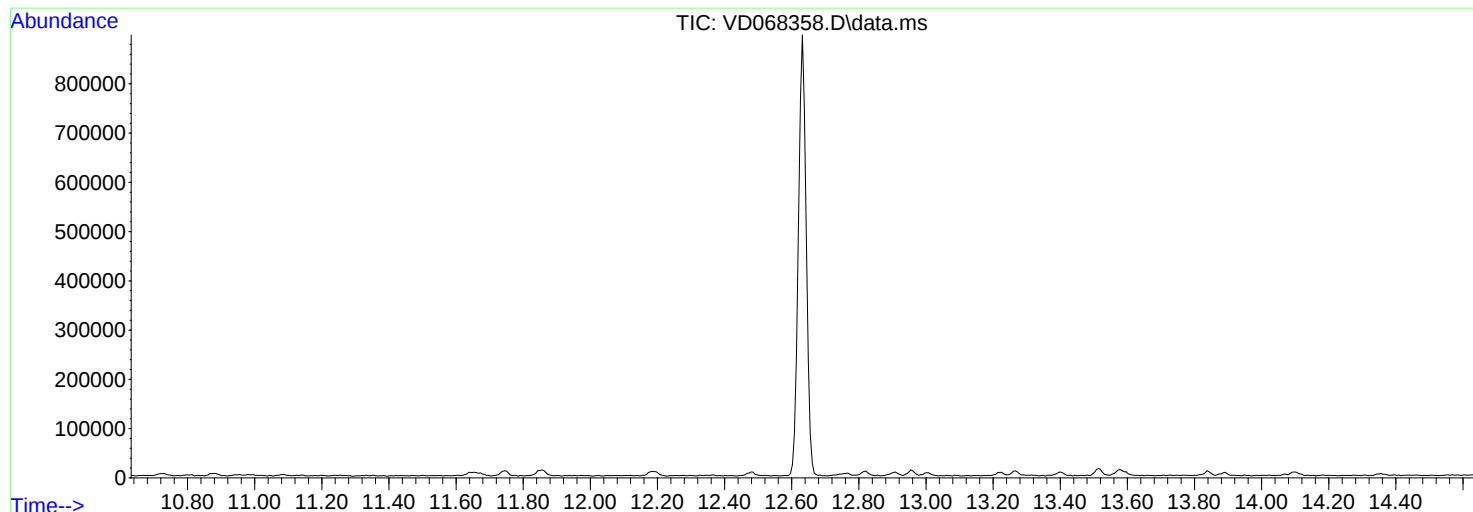

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	30205	PASS
75	95	30	60	50.2	82845	PASS
95	95	100	100	100.0	165077	PASS
96	95	5	9	6.7	11074	PASS
173	174	0.00	2	0.9	1169	PASS
174	95	50	100	77.7	128307	PASS
175	174	5	9	7.3	9305	PASS
176	174	95	101	99.3	127451	PASS
177	176	5	9	6.7	8495	PASS