

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021524\
 Data File : VD078437.D
 Acq On : 15 Feb 2024 15:50
 Operator : RP/MD
 Sample : P1473-01RE
 Misc : 5.06G/5ml/MSVOA_D/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SU-03-021424RE

Quant Time: Feb 16 02:36:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021324S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 14 01:16:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	39494	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	78990	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	97194	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	50985	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	24742	57.940	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.880%
35) Dibromofluoromethane	7.805	113	27640	55.086	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.180%
50) Toluene-d8	10.269	98	101349	50.494	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.980%
62) 4-Bromofluorobenzene	12.575	95	41537	71.113	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	142.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021524\
Data File : VD078437.D
Acq On : 15 Feb 2024 15:50
Operator : RP/MD
Sample : P1473-01RE
Misc : 5.06G/5ml/MSVOA_D/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SU-03-021424RE

Quant Time: Feb 16 02:36:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021324S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 14 01:16:20 2024
Response via : Initial Calibration




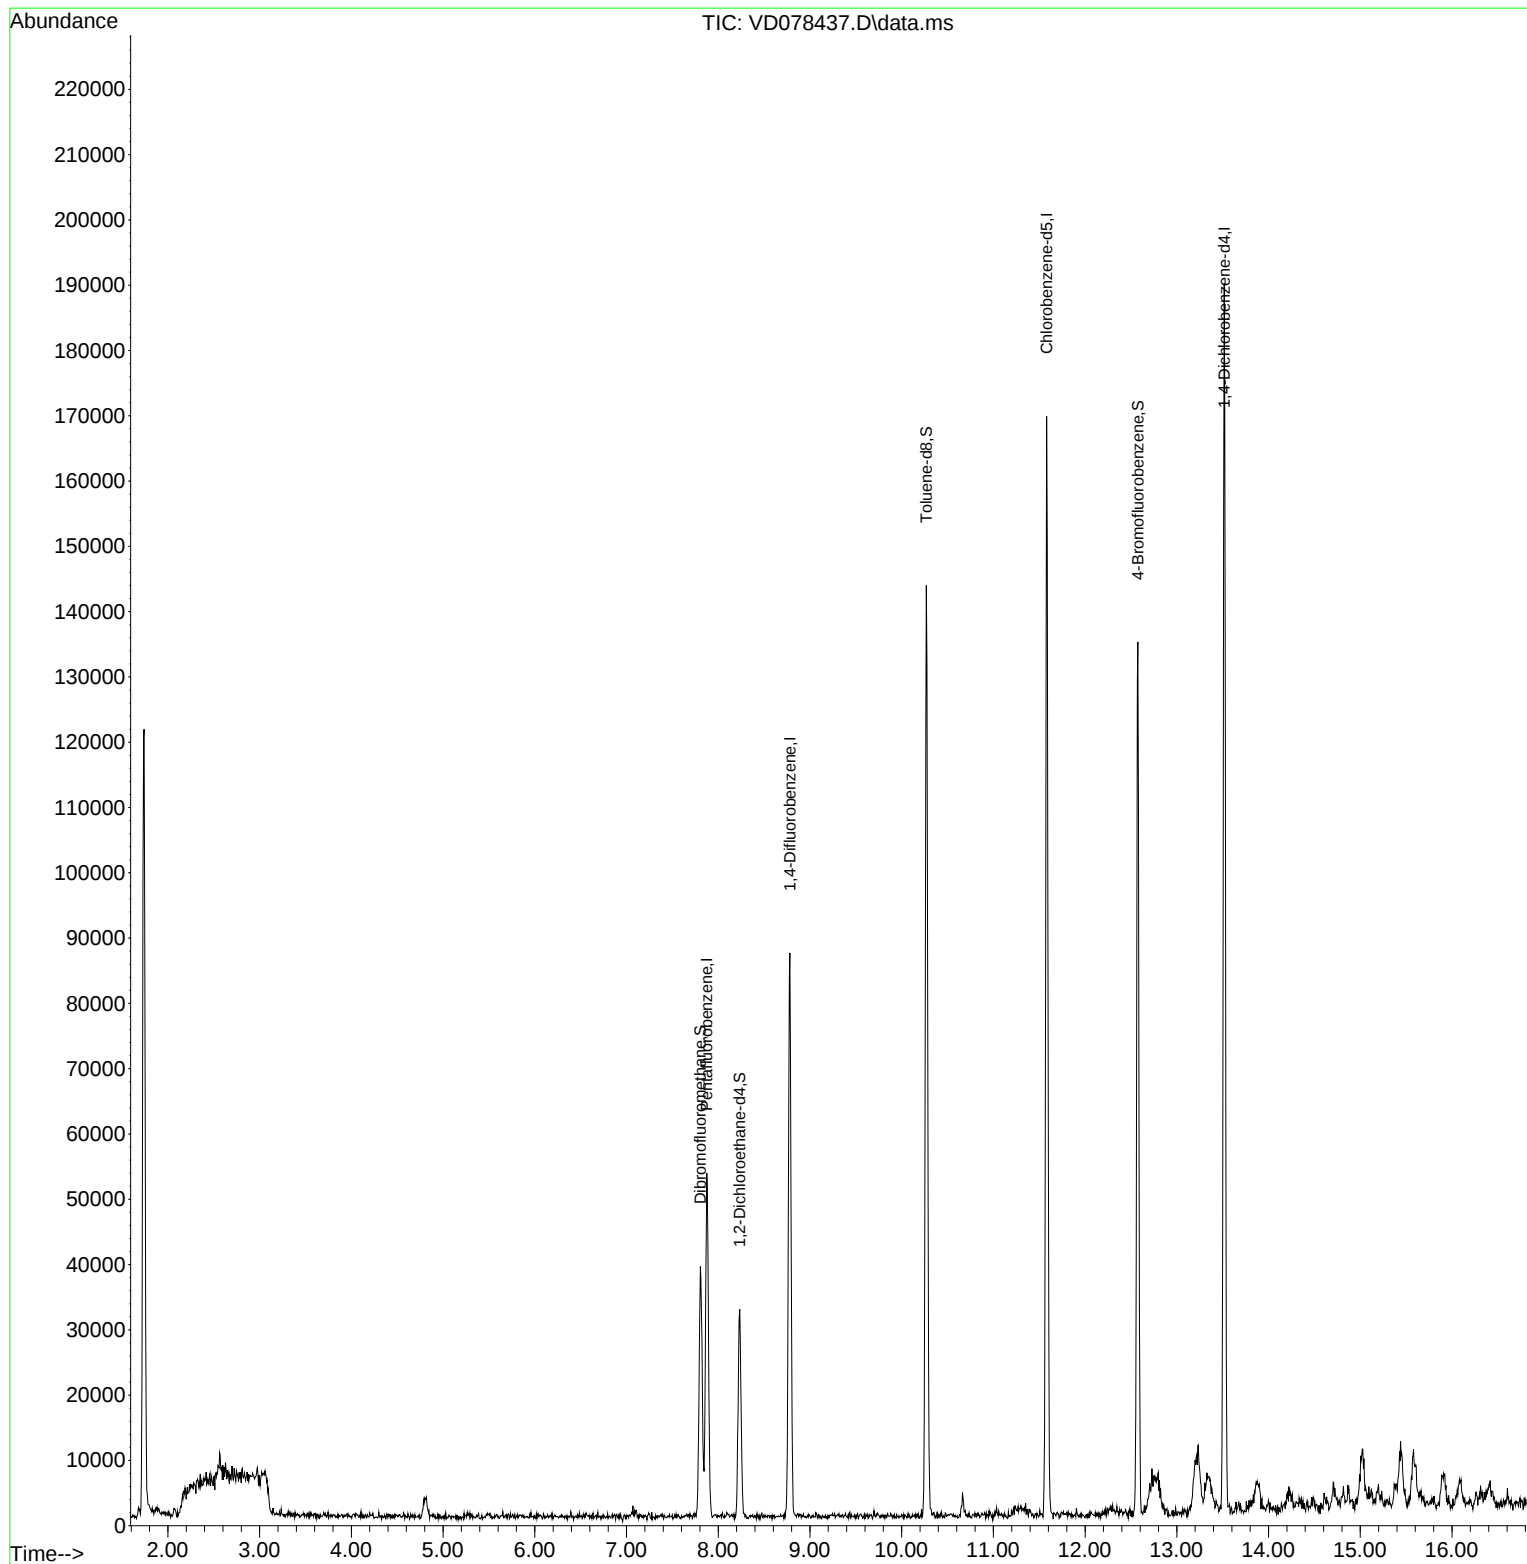


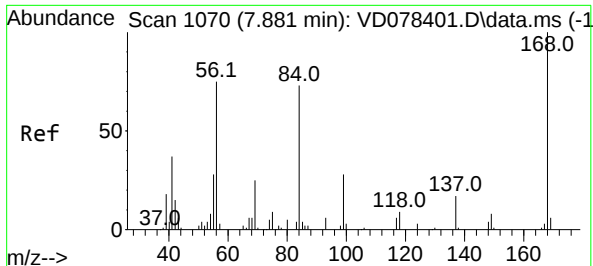

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. -0.006 min
Lab File: VD078437.D
Acq: 15 Feb 2024 15:50




Instrument :
MSVOA_D
ClientSampleId :
SU-03-021424RE


Tgt Ion:168 Resp: 39494
Ion Ratio Lower Upper
168 100
99 52.3 36.7 55.1

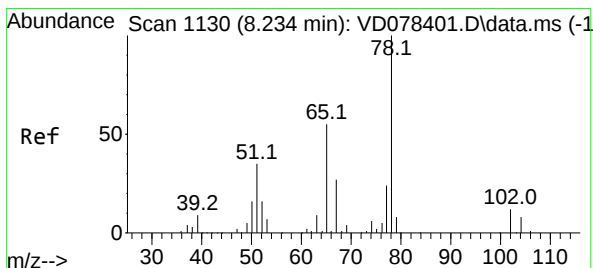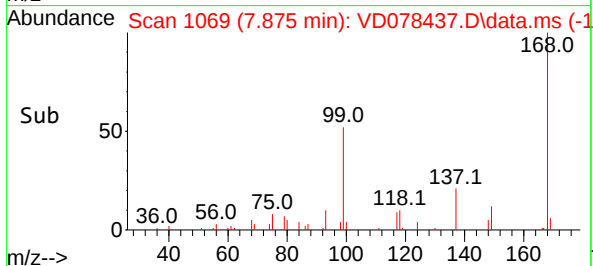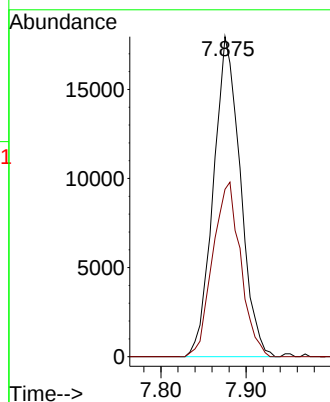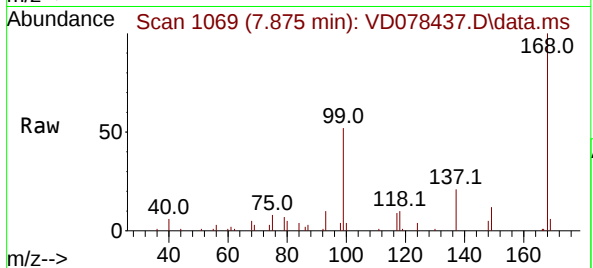

#33
1,2-Dichloroethane-d4
Concen: 57.940 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VD078437.D
Acq: 15 Feb 2024 15:50

Tgt Ion: 65 Resp: 24742
Ion Ratio Lower Upper
65 100
67 50.0 0.0 115.0

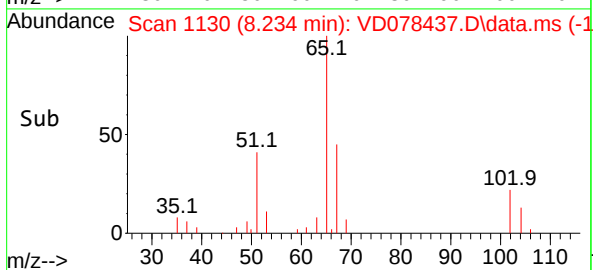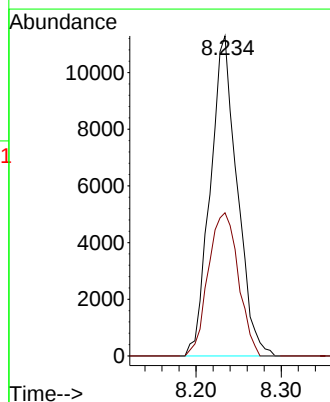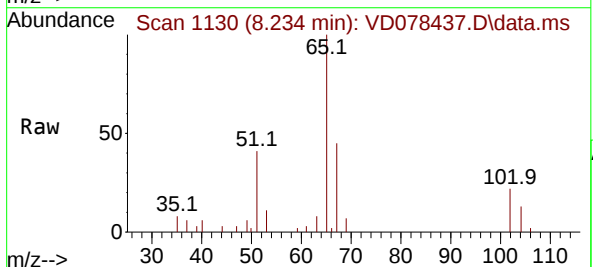

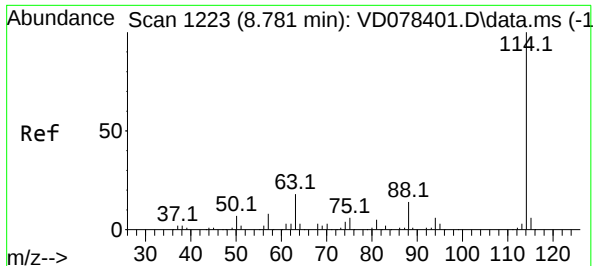

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD078437.D

Acq: 15 Feb 2024 15:50

Instrument :

MSVOA_D

ClientSampleId :

SU-03-021424RE





Tgt Ion:114 Resp: 78990

Ion Ratio Lower Upper

114 100

63 19.5 0.0 33.4

88 15.1 0.0 26.2

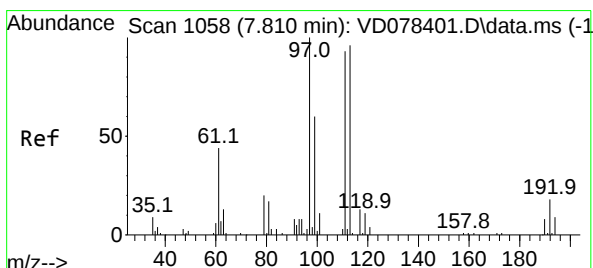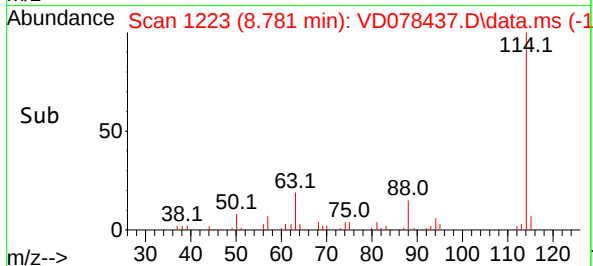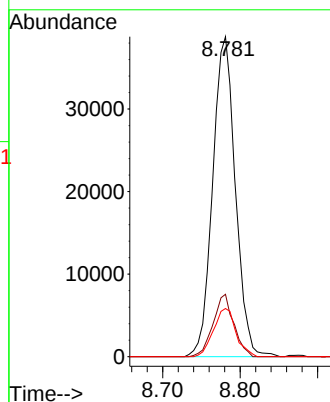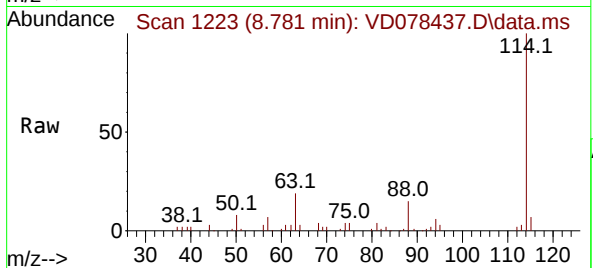

#35

Dibromofluoromethane

Concen: 55.086 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. -0.006 min

Lab File: VD078437.D

Acq: 15 Feb 2024 15:50




Tgt Ion:113 Resp: 27640


Ion Ratio Lower Upper

113 100

111 106.2 84.7 127.1

192 18.9 16.8 25.2


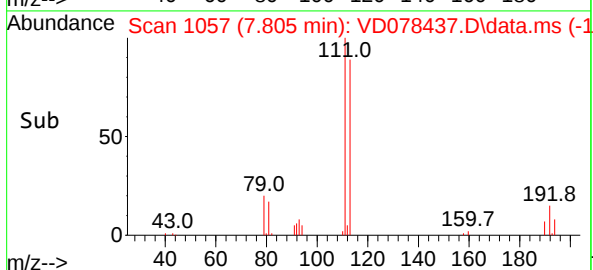
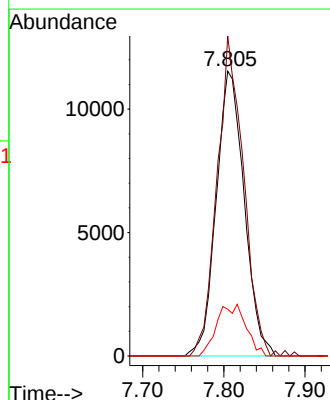
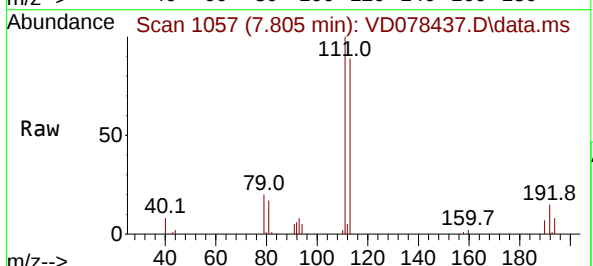


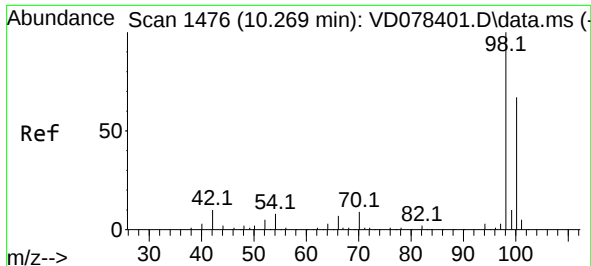

#50
Toluene-d8
Concen: 50.494 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078437.D
Acq: 15 Feb 2024 15:50




Instrument :
MSVOA_D
ClientSampleId :
SU-03-021424RE


Tgt Ion: 98 Resp: 101349
Ion Ratio Lower Upper
98 100
100 64.6 50.3 75.5

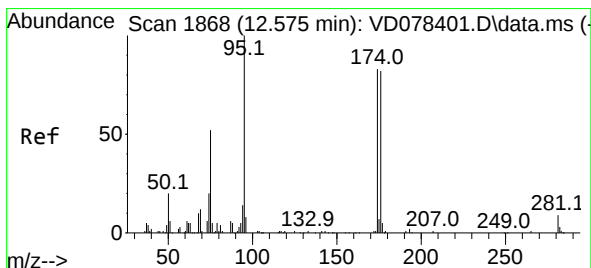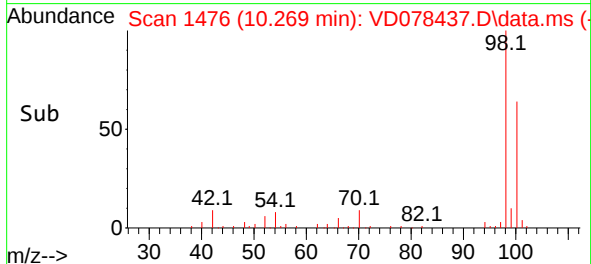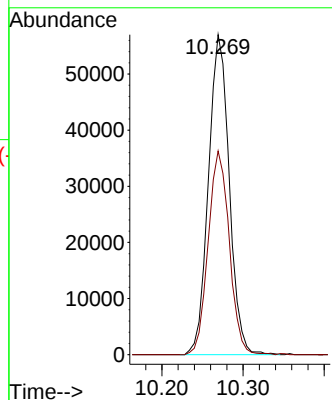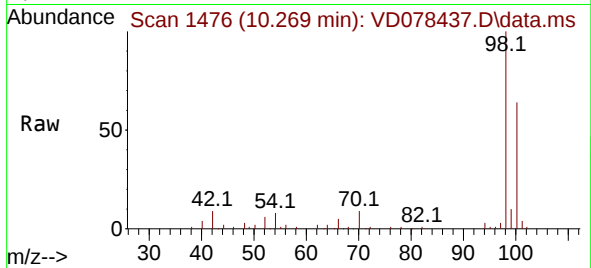

#62
4-Bromofluorobenzene
Concen: 71.113 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.000 min
Lab File: VD078437.D
Acq: 15 Feb 2024 15:50

Tgt Ion: 95 Resp: 41537
Ion Ratio Lower Upper
95 100
174 91.2 0.0 201.8
176 82.0 0.0 191.8


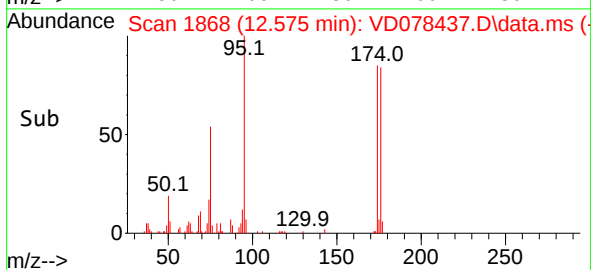
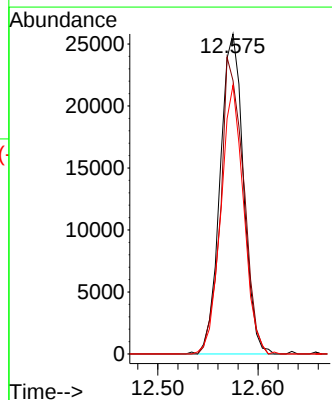
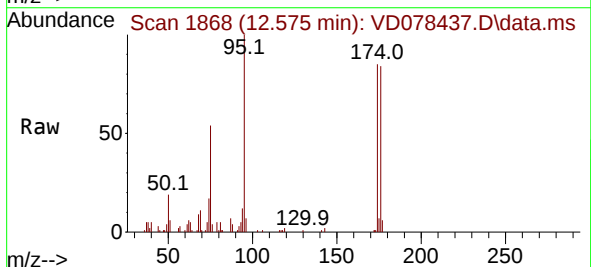


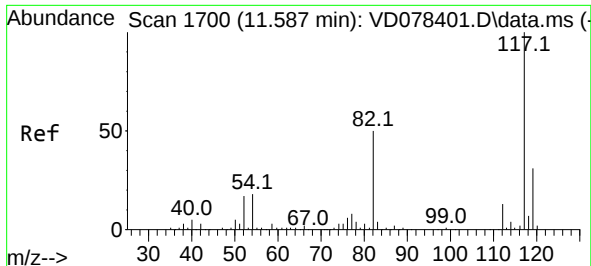

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.006 min
Lab File: VD078437.D
Acq: 15 Feb 2024 15:50

Instrument :
MSVOA_D
ClientSampleId :
SU-03-021424RE

Tgt Ion:117 Resp: 97194
Ion Ratio Lower Upper
117 100
82 50.4 38.3 57.5
119 34.0 25.0 37.4

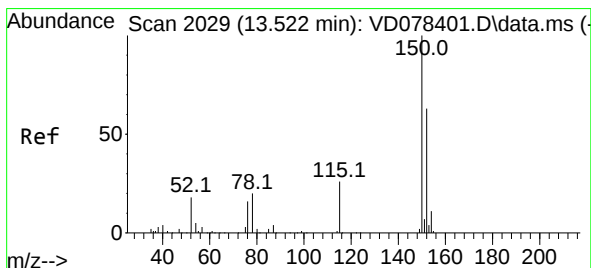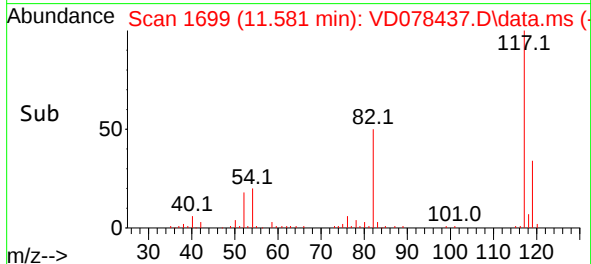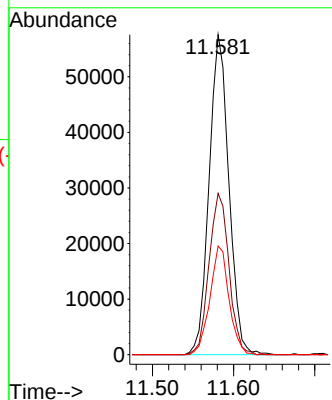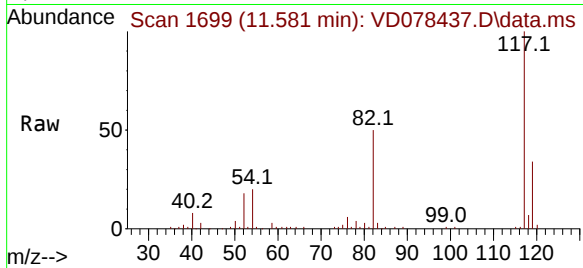

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD078437.D
Acq: 15 Feb 2024 15:50

Tgt Ion:152 Resp: 50985
Ion Ratio Lower Upper
152 100
115 56.3 27.1 81.3
150 158.9 0.0 353.6

