

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD021524\  
 Data File : VD078447.D  
 Acq On : 15 Feb 2024 20:29  
 Operator : RP/MD  
 Sample : P1483-03RE  
 Misc : 5.00G/5ml/MSVOA\_D/SOIL/B  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 VNJ-205RE

Quant Time: Feb 16 02:40:48 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D021324S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Feb 14 01:16:20 2024  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.881  | 168  | 130147   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.781  | 114  | 252448   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.581 | 117  | 292744   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.516 | 152  | 145127   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.234  | 65    | 60883    | 43.265   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 86.540%  |
| 35) Dibromofluoromethane    | 7.810  | 113   | 79200    | 49.389   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 98.780%  |
| 50) Toluene-d8              | 10.269 | 98    | 325663   | 50.768   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 58 - 134 | Recovery | =    | 101.540% |
| 62) 4-Bromofluorobenzene    | 12.575 | 95    | 121362   | 65.013   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 30 - 143 | Recovery | =    | 130.020% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD021524\  
Data File : VD078447.D  
Acq On : 15 Feb 2024 20:29  
Operator : RP/MD  
Sample : P1483-03RE  
Misc : 5.00G/5ml/MSVOA\_D/SOIL/B  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-205RE

Quant Time: Feb 16 02:40:48 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D021324S.M  
Quant Title : SW846 8260  
QLast Update : Wed Feb 14 01:16:20 2024  
Response via : Initial Calibration




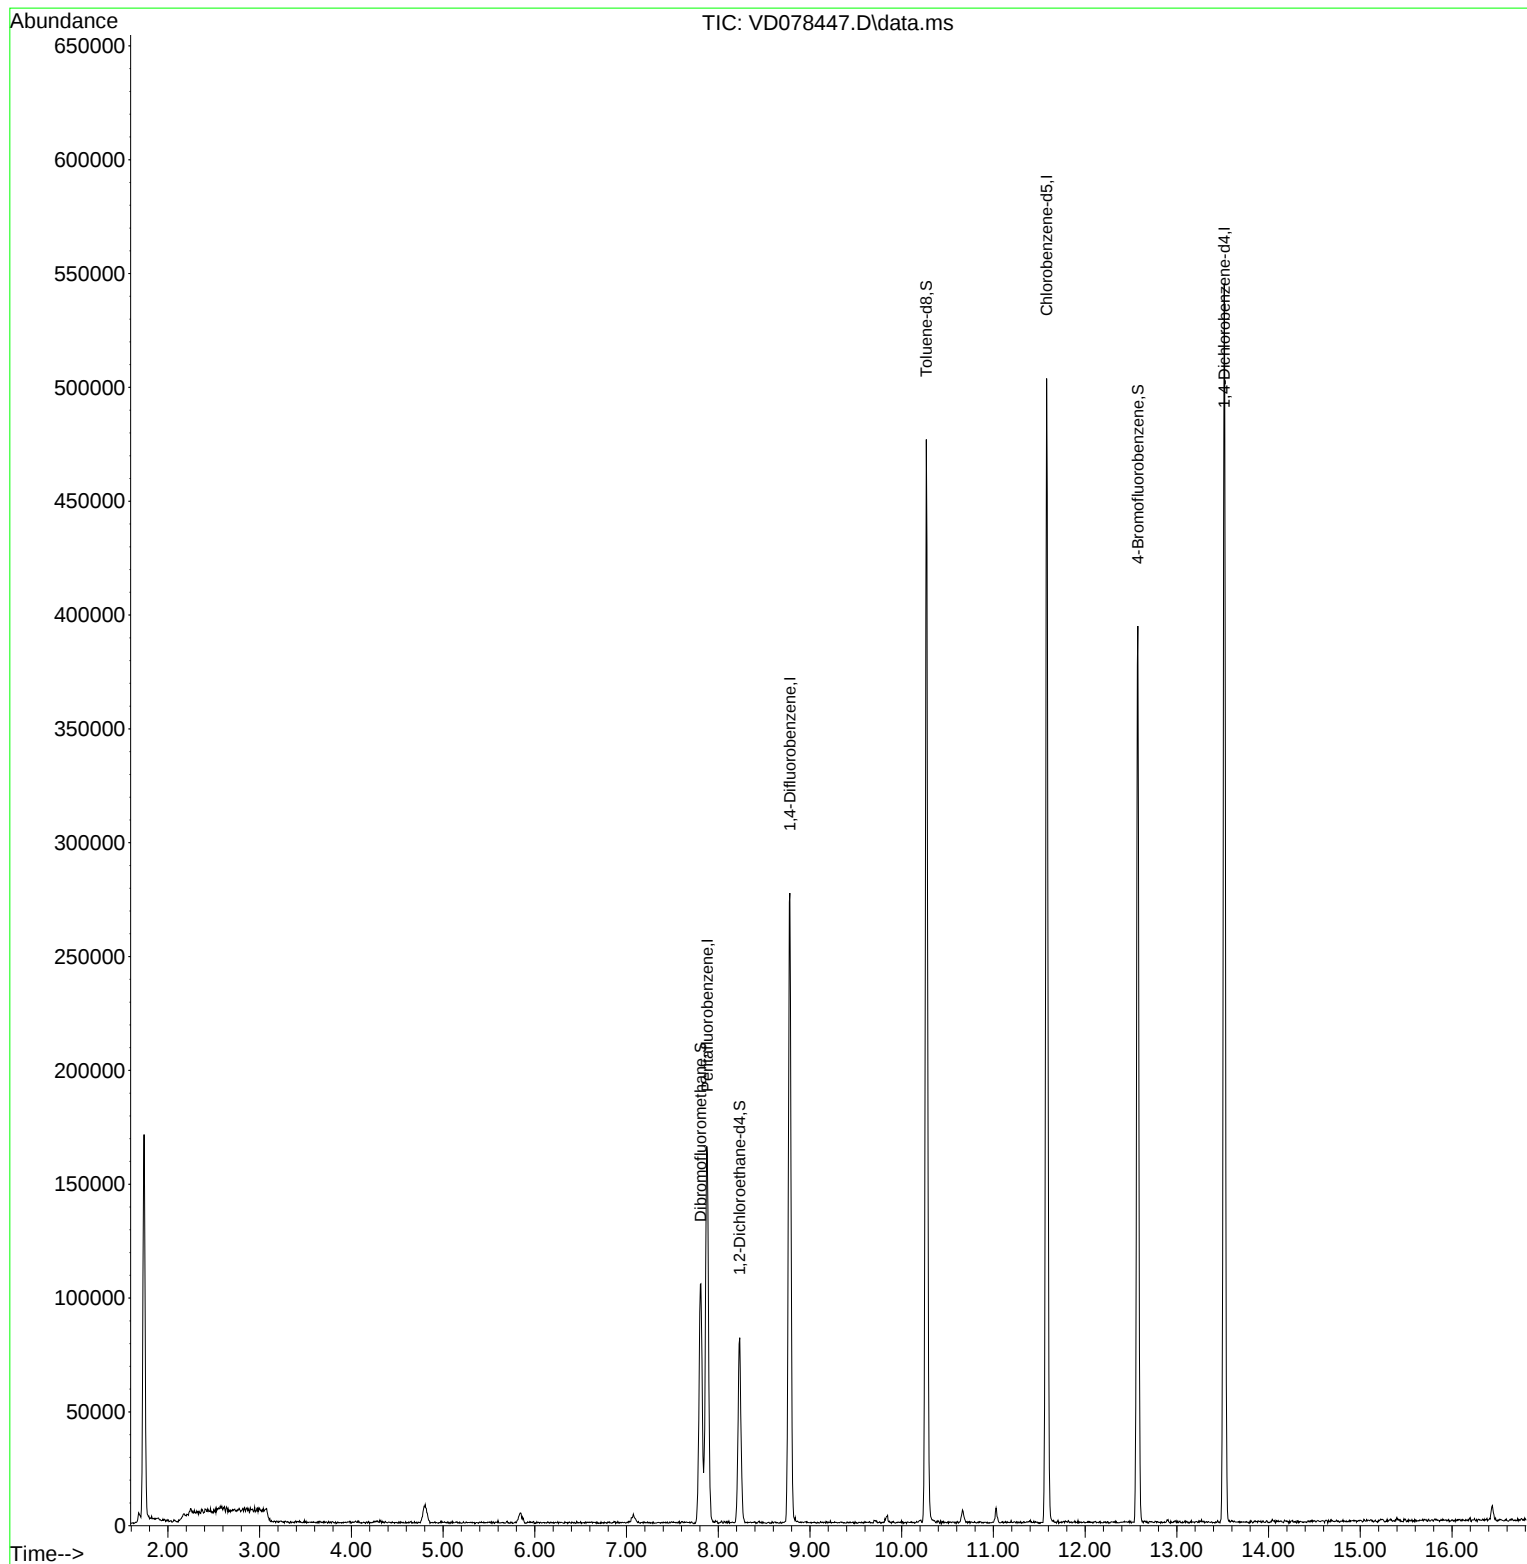


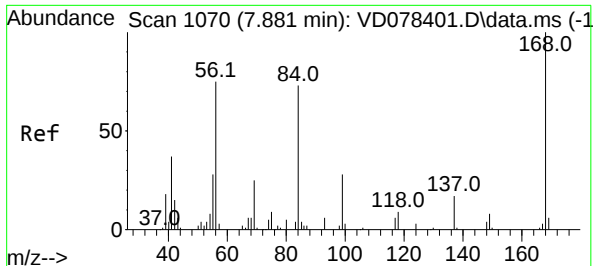

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.881 min Scan# 1070  
Delta R.T. 0.000 min  
Lab File: VD078447.D  
Acq: 15 Feb 2024 20:29




Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-205RE


Tgt Ion:168 Resp: 130147  
Ion Ratio Lower Upper  
168 100  
99 51.3 36.7 55.1

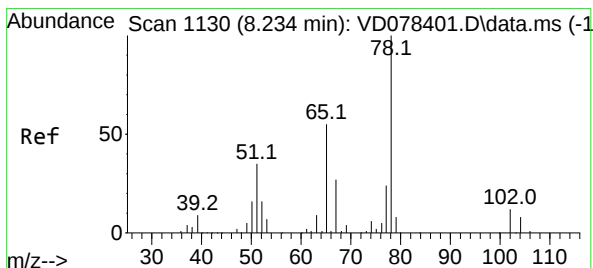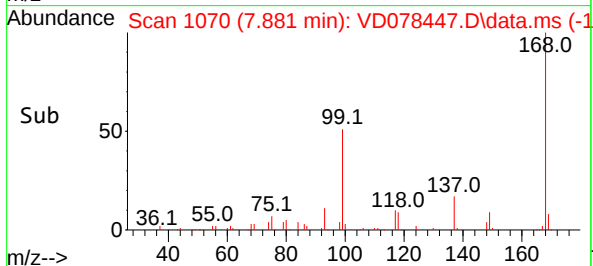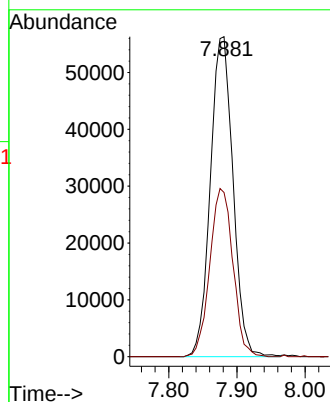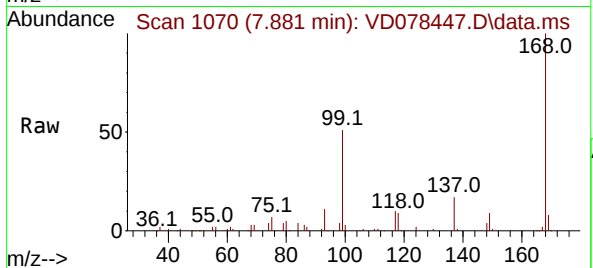

#33  
1,2-Dichloroethane-d4  
Concen: 43.265 ug/l  
RT: 8.234 min Scan# 1130  
Delta R.T. 0.000 min  
Lab File: VD078447.D  
Acq: 15 Feb 2024 20:29

Tgt Ion: 65 Resp: 60883  
Ion Ratio Lower Upper  
65 100  
67 56.0 0.0 115.0

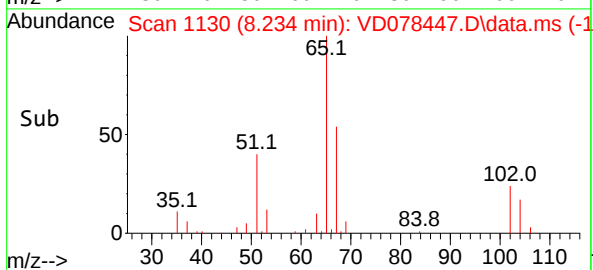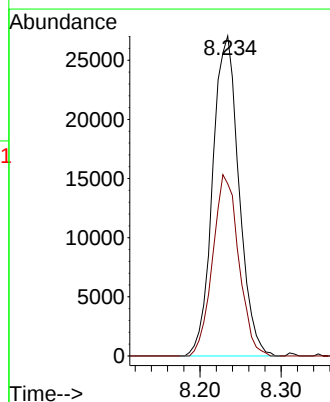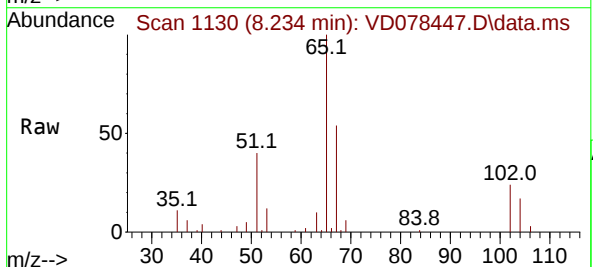

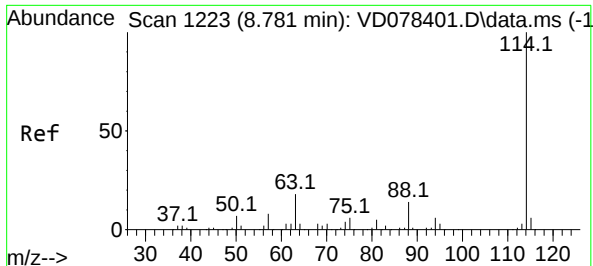

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD078447.D

Acq: 15 Feb 2024 20:29

Instrument :

MSVOA\_D

ClientSampleId :

VNJ-205RE





Tgt Ion:114 Resp: 252448

Ion Ratio Lower Upper

114 100

63 18.3 0.0 33.4

88 13.6 0.0 26.2

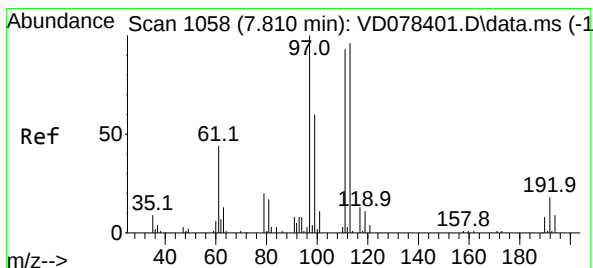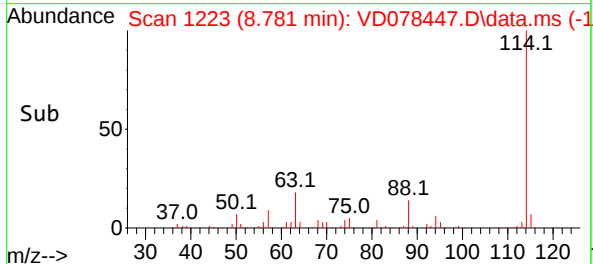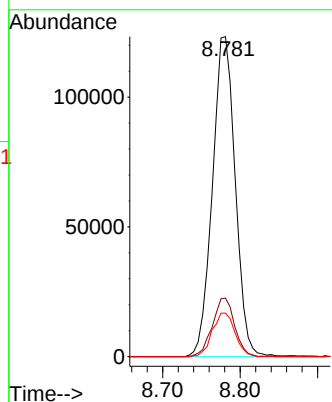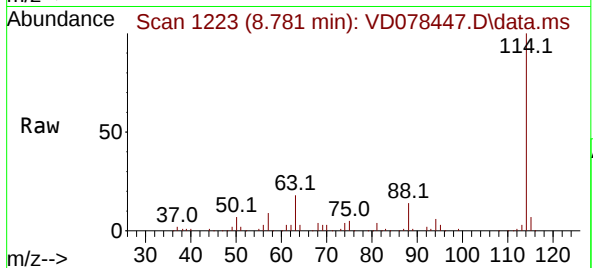

#35

Dibromofluoromethane

Concen: 49.389 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.000 min

Lab File: VD078447.D

Acq: 15 Feb 2024 20:29




Tgt Ion:113 Resp: 79200


Ion Ratio Lower Upper

113 100

111 101.0 84.7 127.1

192 18.7 16.8 25.2


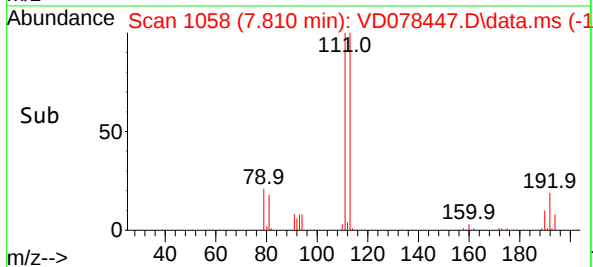
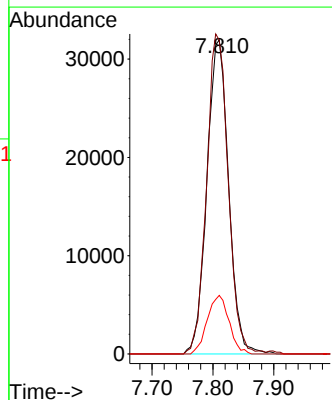
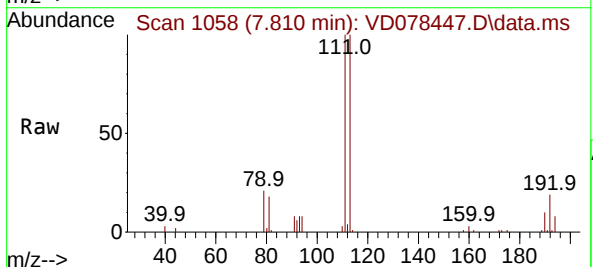


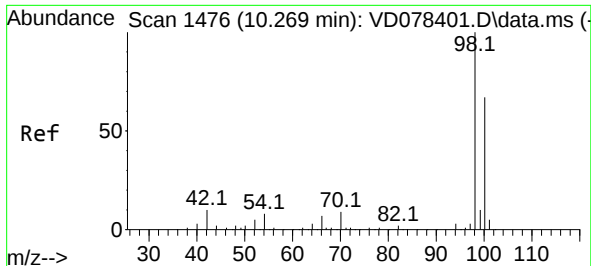

#50  
Toluene-d8  
Concen: 50.768 ug/l  
RT: 10.269 min Scan# 1476  
Delta R.T. 0.000 min  
Lab File: VD078447.D  
Acq: 15 Feb 2024 20:29




Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-205RE


Tgt Ion: 98 Resp: 325663  
Ion Ratio Lower Upper  
98 100  
100 63.6 50.3 75.5

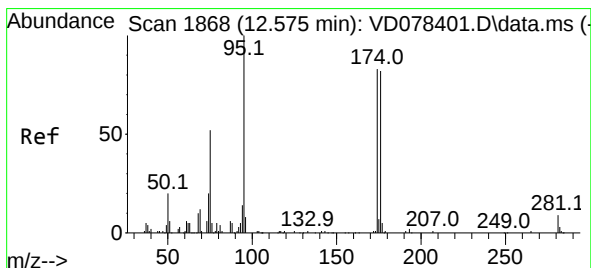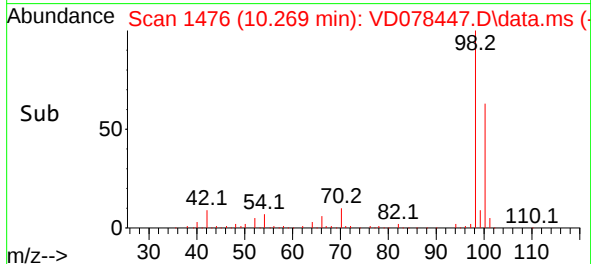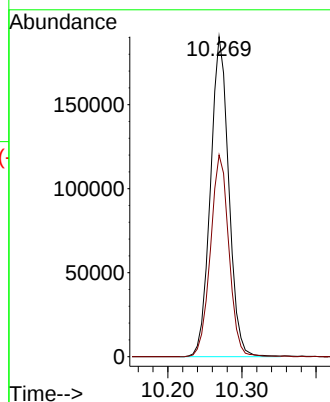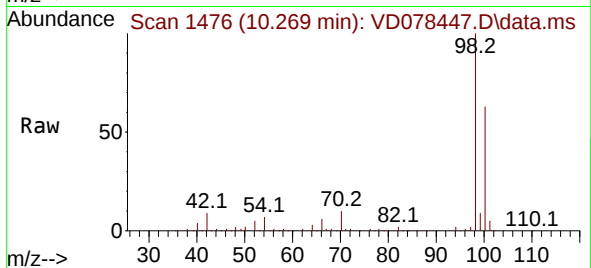

#62  
4-Bromofluorobenzene  
Concen: 65.013 ug/l  
RT: 12.575 min Scan# 1868  
Delta R.T. 0.000 min  
Lab File: VD078447.D  
Acq: 15 Feb 2024 20:29

Tgt Ion: 95 Resp: 121362  
Ion Ratio Lower Upper  
95 100  
174 86.7 0.0 201.8  
176 85.0 0.0 191.8


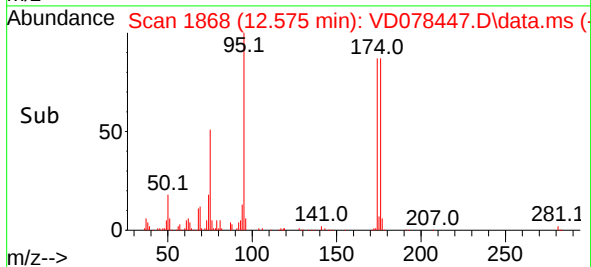
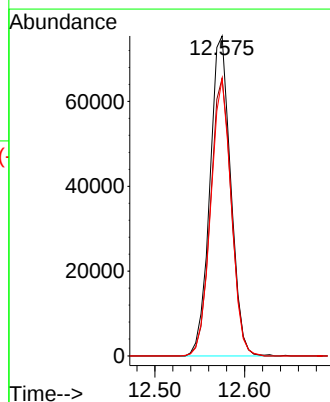
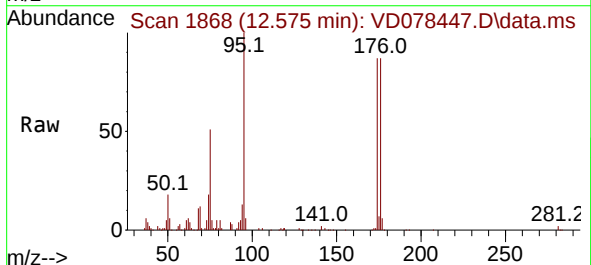


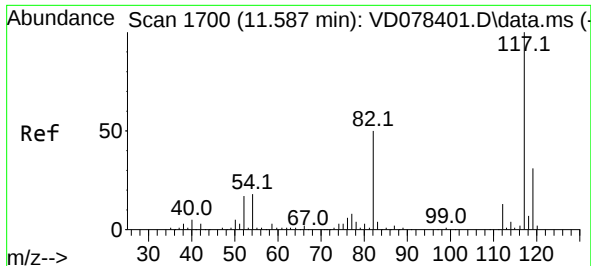

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.581 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: VD078447.D  
Acq: 15 Feb 2024 20:29

Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-205RE

Tgt Ion:117 Resp: 292744  
Ion Ratio Lower Upper  
117 100  
82 51.8 38.3 57.5  
119 33.0 25.0 37.4

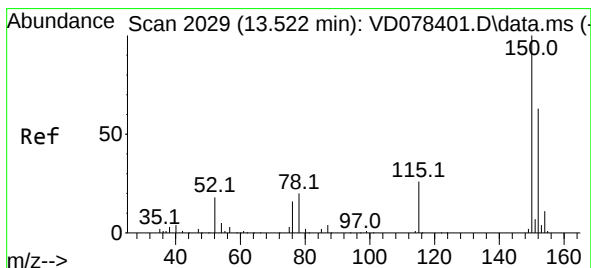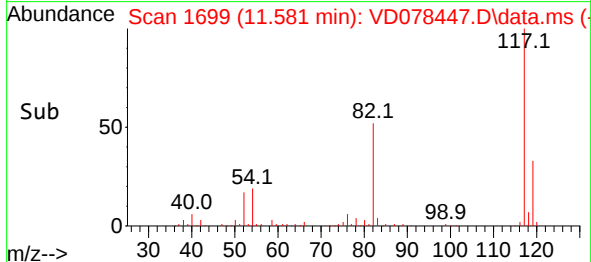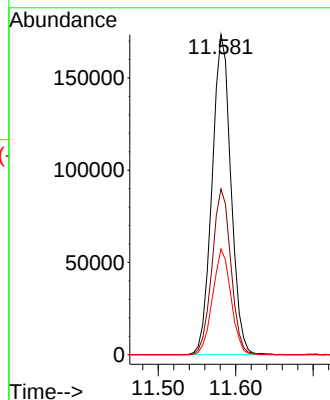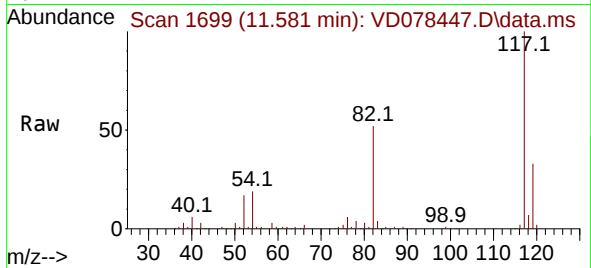

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.516 min Scan# 2028  
Delta R.T. -0.006 min  
Lab File: VD078447.D  
Acq: 15 Feb 2024 20:29

Tgt Ion:152 Resp: 145127  
Ion Ratio Lower Upper  
152 100  
115 58.3 27.1 81.3  
150 159.0 0.0 353.6

