


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021621\
Data File : VD068366.D
Acq On : 16 Feb 2021 09:19
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
Title : SW846 8260
Last Update : Fri Feb 12 13:30:51 2021

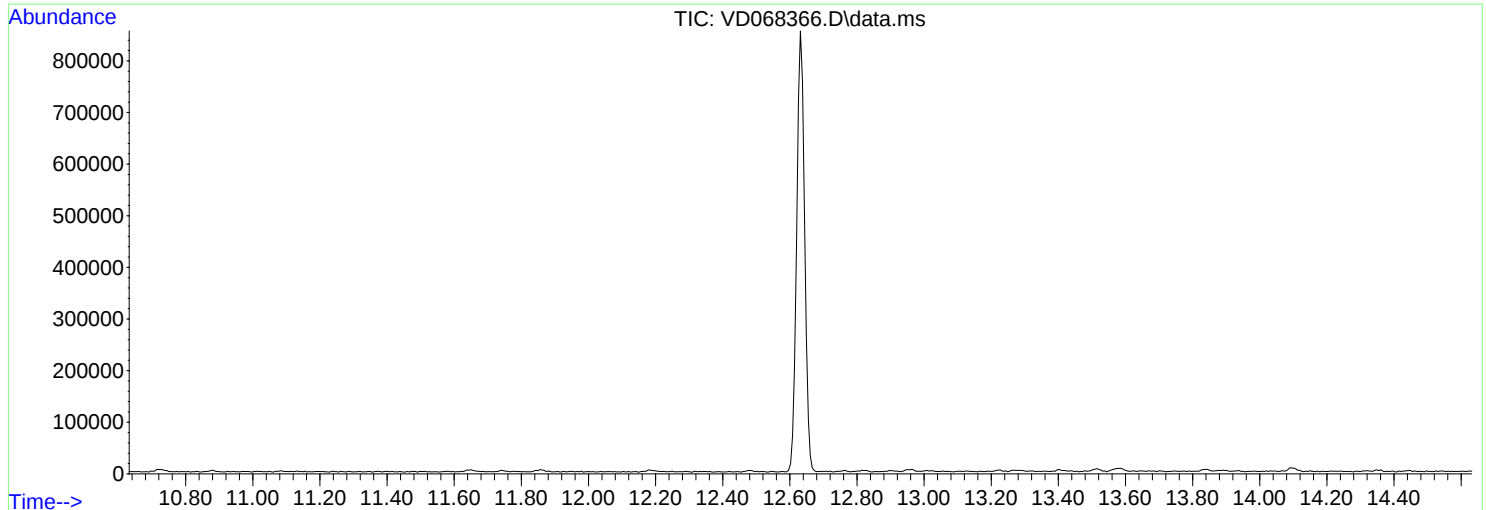

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	27955	PASS
75	95	30	60	50.7	81656	PASS
95	95	100	100	100.0	161003	PASS
96	95	5	9	6.3	10171	PASS
173	174	0.00	2	1.1	1388	PASS
174	95	50	100	77.2	124357	PASS
175	174	5	9	7.5	9337	PASS
176	174	95	101	96.7	120208	PASS
177	176	5	9	6.5	7783	PASS