

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021622\
 Data File : VD071984.D
 Acq On : 16 Feb 2022 10:55
 Operator : VA/SY
 Sample : VD0216SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0216SBL01

Quant Time: Feb 17 00:46:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 27 06:04:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	266856	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	491666	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	448323	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	203409	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	193603	57.399	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.800%
35) Dibromofluoromethane	7.914	113	168174	52.036	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	104.080%
50) Toluene-d8	10.338	98	569742	47.203	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	94.400%
62) 4-Bromofluorobenzene	12.626	95	189014	44.843	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	89.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021622\
Data File : VD071984.D
Acq On : 16 Feb 2022 10:55
Operator : VA/SY
Sample : VD0216SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0216SBL01

Quant Time: Feb 17 00:46:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 27 06:04:38 2022
Response via : Initial Calibration




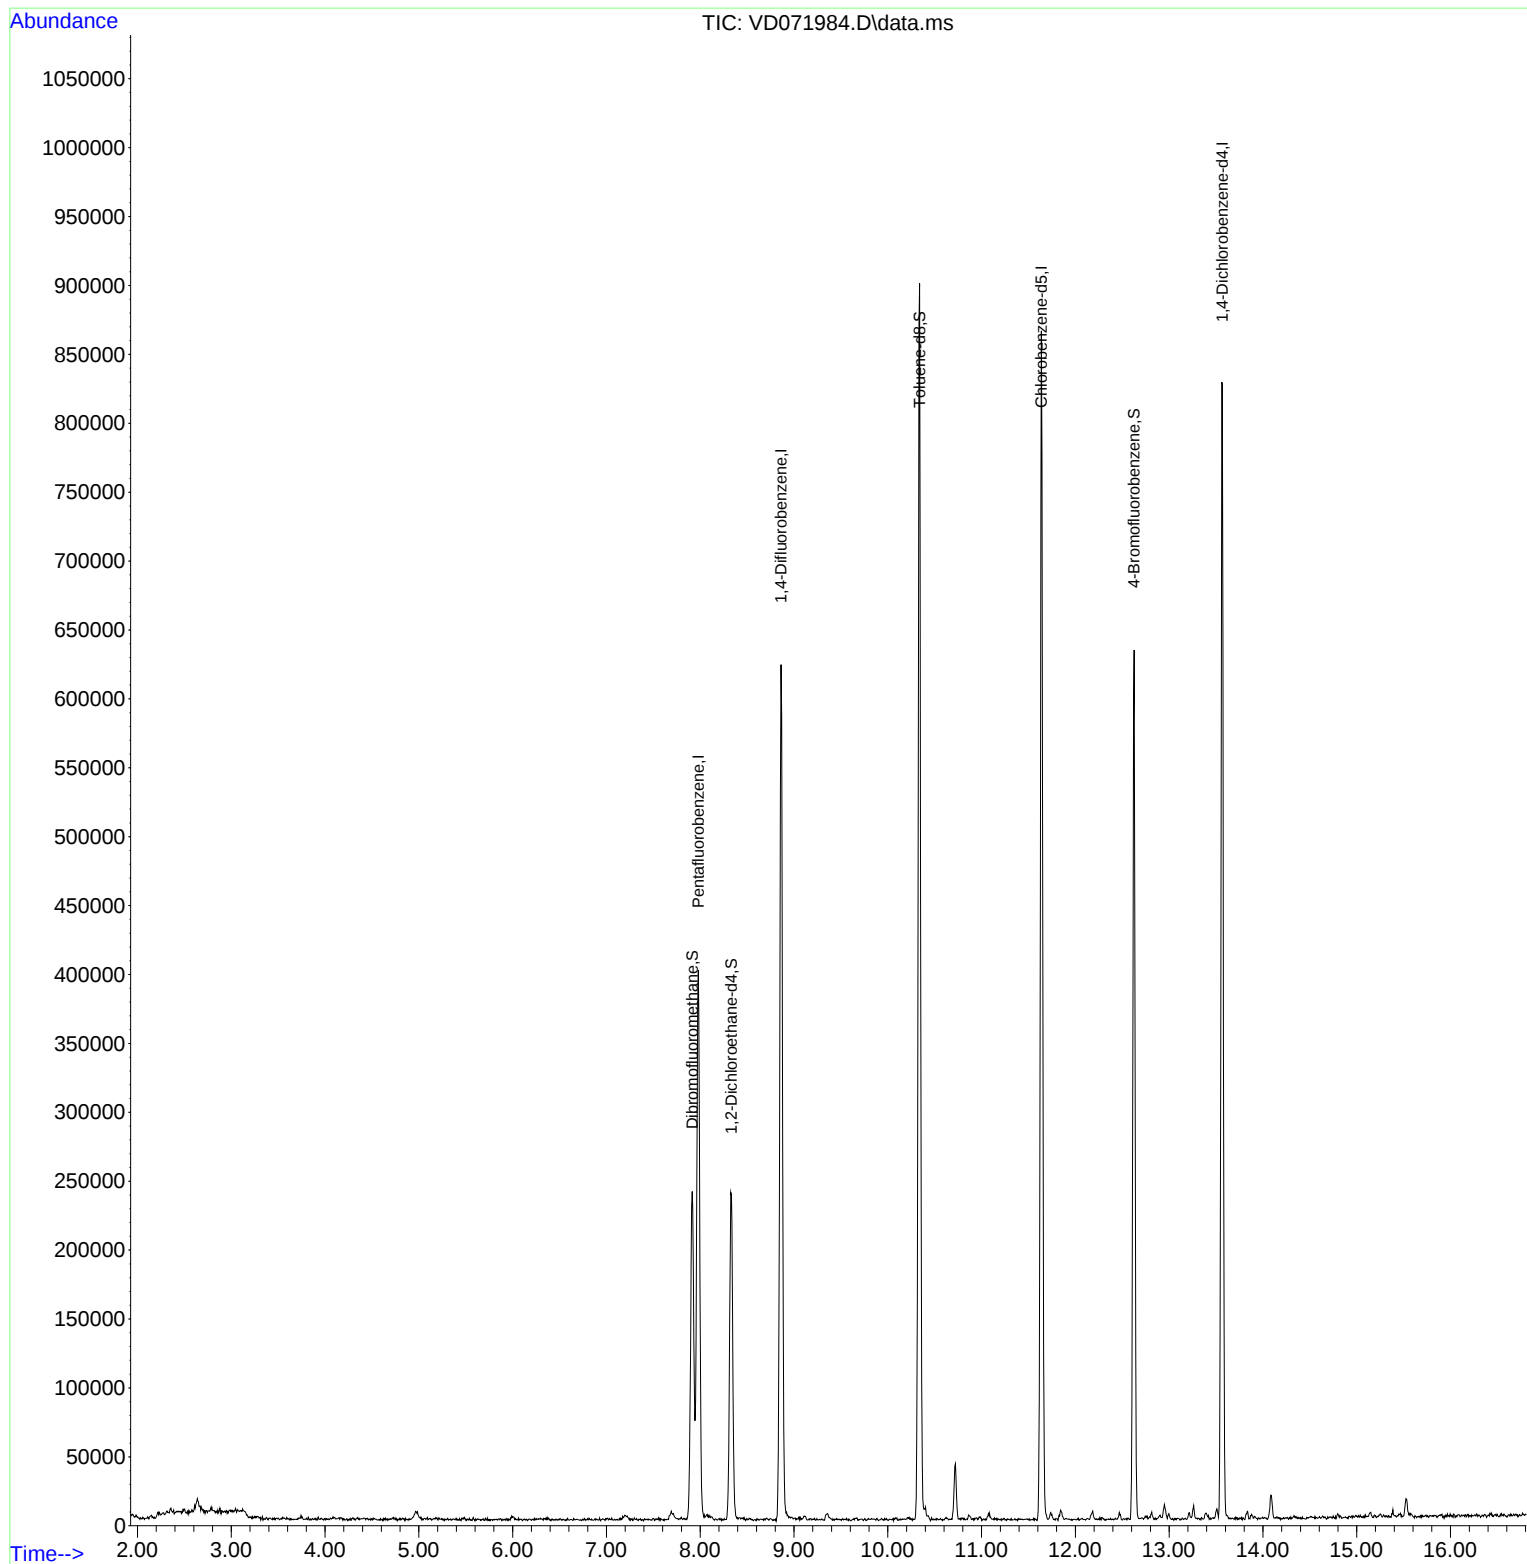


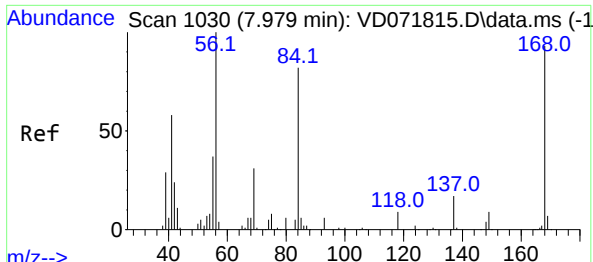

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD071984.D
Acq: 16 Feb 2022 10:55




Instrument :
MSVOA_D
ClientSampleId :
VD0216SBL01


Tgt Ion:168 Resp: 266856
Ion Ratio Lower Upper
168 100
99 64.3 49.8 74.6

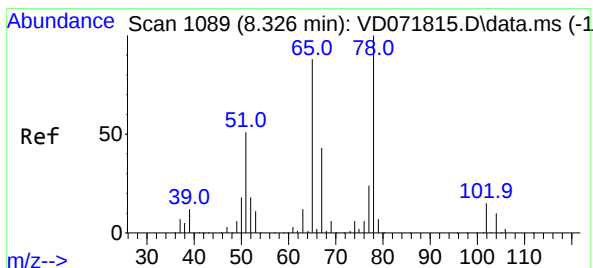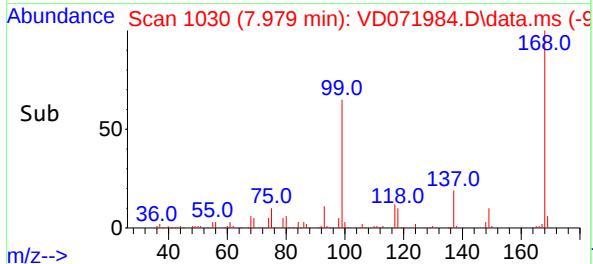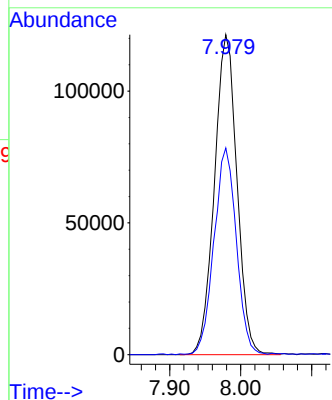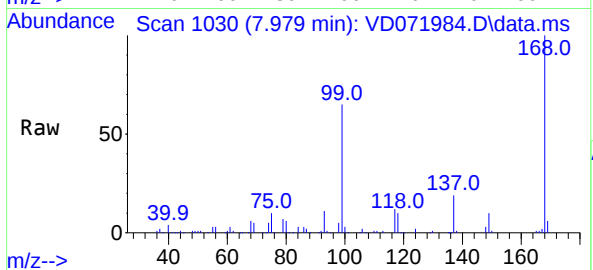

#33
1,2-Dichloroethane-d4
Concen: 57.399 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.006 min
Lab File: VD071984.D
Acq: 16 Feb 2022 10:55

Tgt Ion: 65 Resp: 193603
Ion Ratio Lower Upper
65 100
67 52.3 0.0 101.4

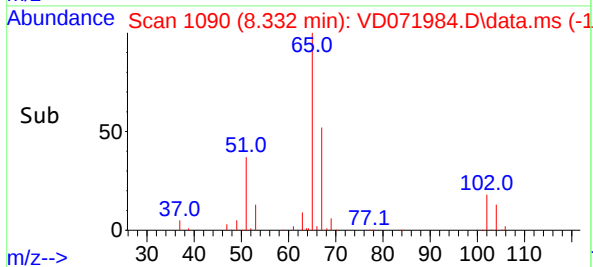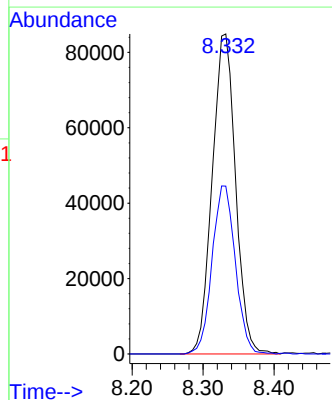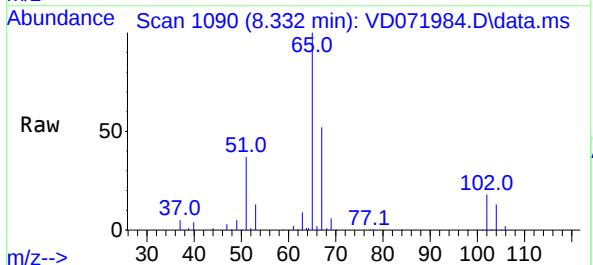

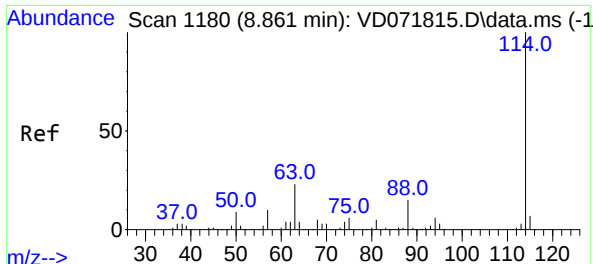

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD071984.D

Acq: 16 Feb 2022 10:55

Instrument :

MSVOA_D

ClientSampleId :

VD0216SBL01





Tgt Ion:114 Resp: 491666

Ion Ratio Lower Upper

114 100

63 22.5 0.0 46.6

88 15.1 0.0 33.2

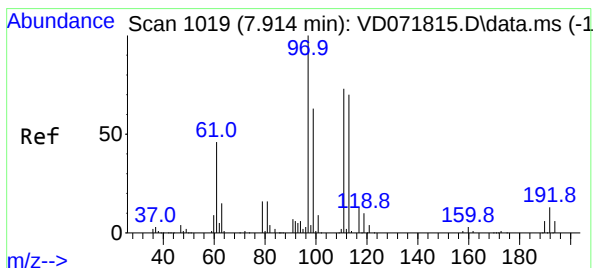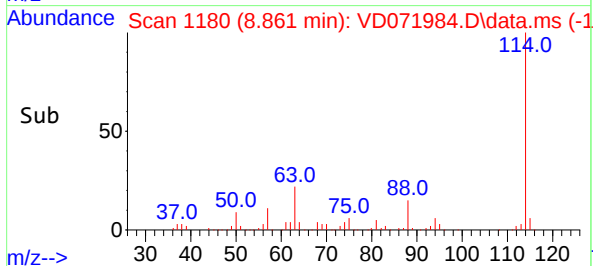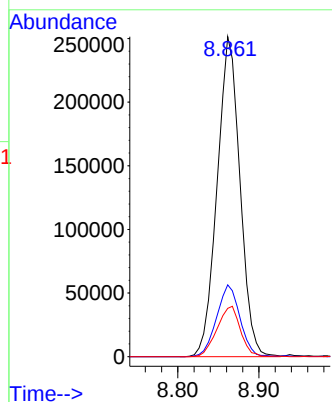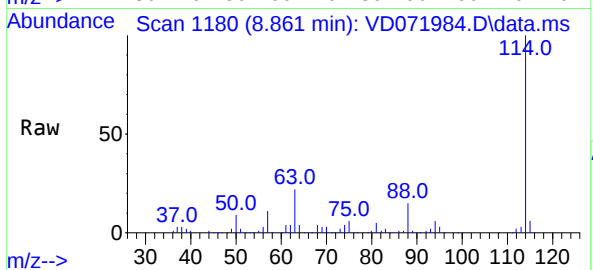

#35

Dibromofluoromethane

Concen: 52.036 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. 0.000 min

Lab File: VD071984.D

Acq: 16 Feb 2022 10:55




Tgt Ion:113 Resp: 168174


Ion Ratio Lower Upper

113 100

111 103.5 83.8 125.6

192 17.8 14.6 21.8


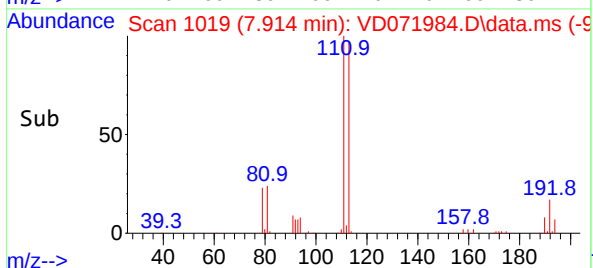
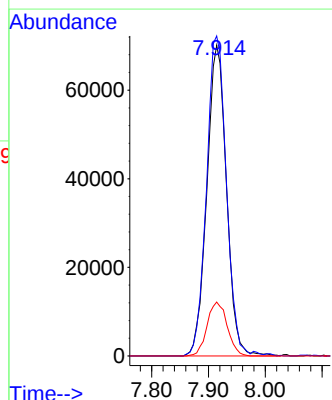
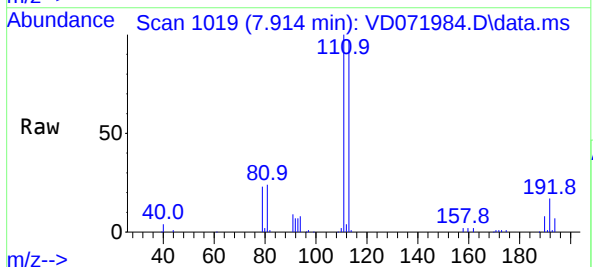


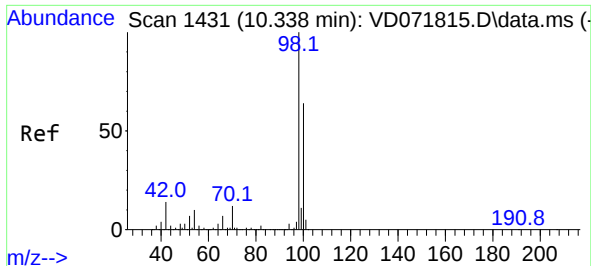

#50
Toluene-d8
Concen: 47.203 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.000 min
Lab File: VD071984.D
Acq: 16 Feb 2022 10:55




Instrument :
MSVOA_D
ClientSampleId :
VD0216SBL01


Tgt Ion: 98 Resp: 569742
Ion Ratio Lower Upper
98 100
100 63.9 52.4 78.6

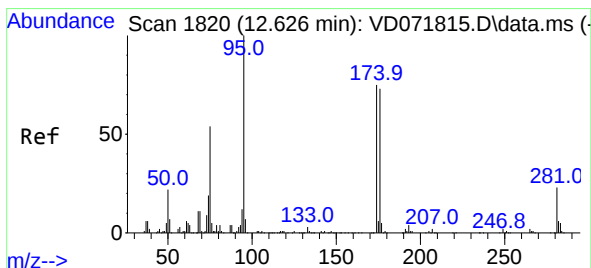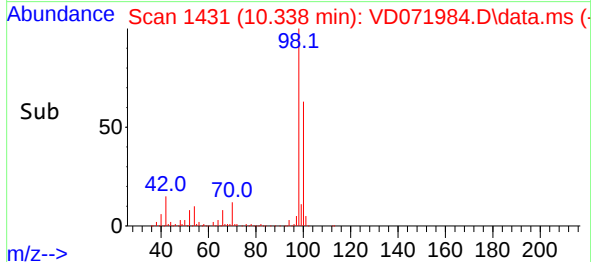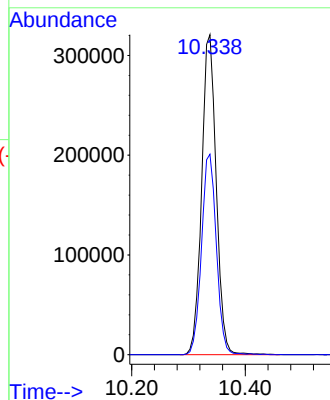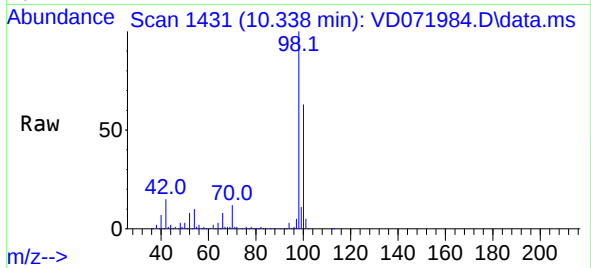

#62
4-Bromofluorobenzene
Concen: 44.843 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD071984.D
Acq: 16 Feb 2022 10:55

Tgt Ion: 95 Resp: 189014
Ion Ratio Lower Upper
95 100
174 75.6 0.0 152.8
176 71.9 0.0 145.4


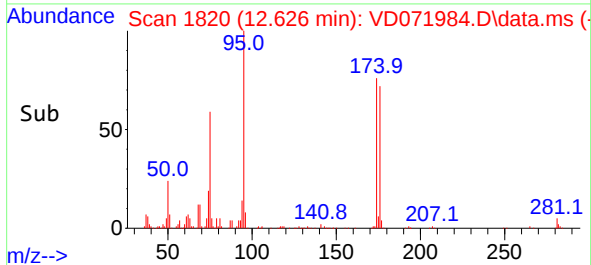
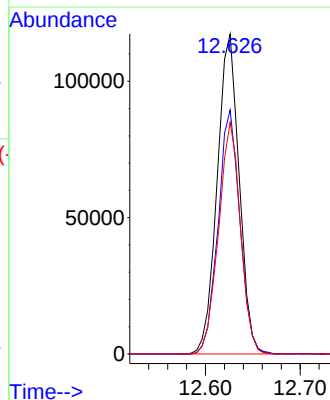
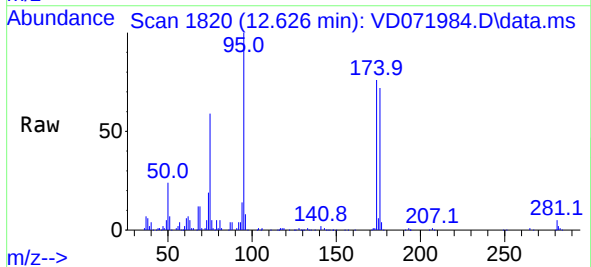


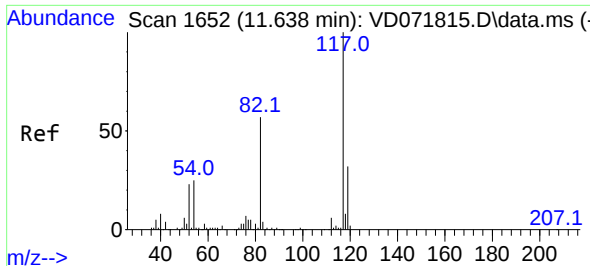

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD071984.D
Acq: 16 Feb 2022 10:55

Instrument :
MSVOA_D
ClientSampleId :
VD0216SBL01

Tgt Ion:117 Resp: 448323
Ion Ratio Lower Upper
117 100
82 59.3 45.3 67.9
119 32.8 26.6 40.0

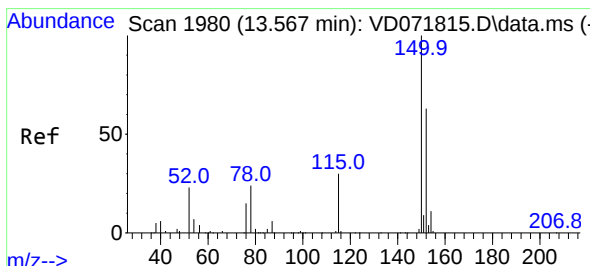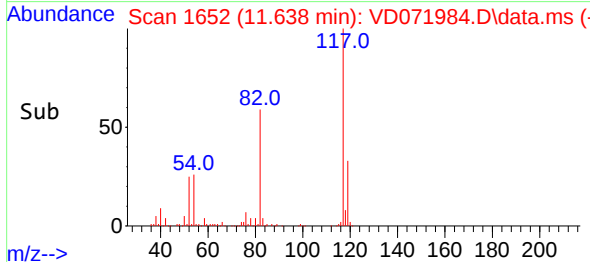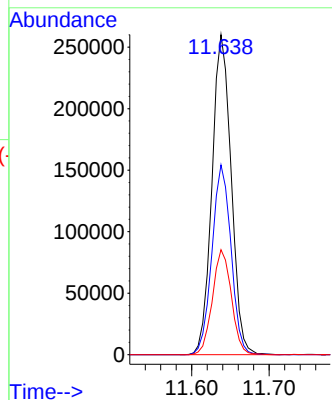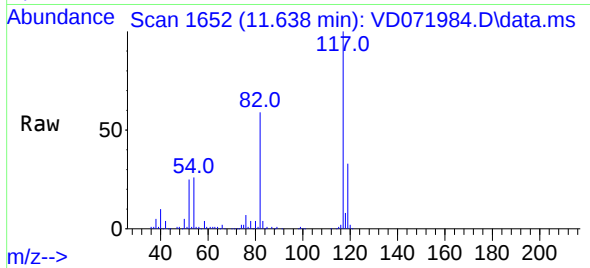

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.000 min
Lab File: VD071984.D
Acq: 16 Feb 2022 10:55

Tgt Ion:152 Resp: 203409
Ion Ratio Lower Upper
152 100
115 62.3 31.3 93.8
150 160.5 0.0 348.6

