

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021622\
 Data File : VD071989.D
 Acq On : 16 Feb 2022 13:44
 Operator : VA/SY
 Sample : N1554-01
 Misc : 5.73G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BU-03-021522

Quant Time: Feb 17 00:48:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 27 06:04:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	393938	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	726898	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	683691	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	288511	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	245691	49.344	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.680%
35) Dibromofluoromethane	7.914	113	229933	48.122	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.240%
50) Toluene-d8	10.338	98	932624	52.264	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.520%
62) 4-Bromofluorobenzene	12.626	95	305939	49.095	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	98.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021622\
Data File : VD071989.D
Acq On : 16 Feb 2022 13:44
Operator : VA/SY
Sample : N1554-01
Misc : 5.73G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BU-03-021522

Quant Time: Feb 17 00:48:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 27 06:04:38 2022
Response via : Initial Calibration




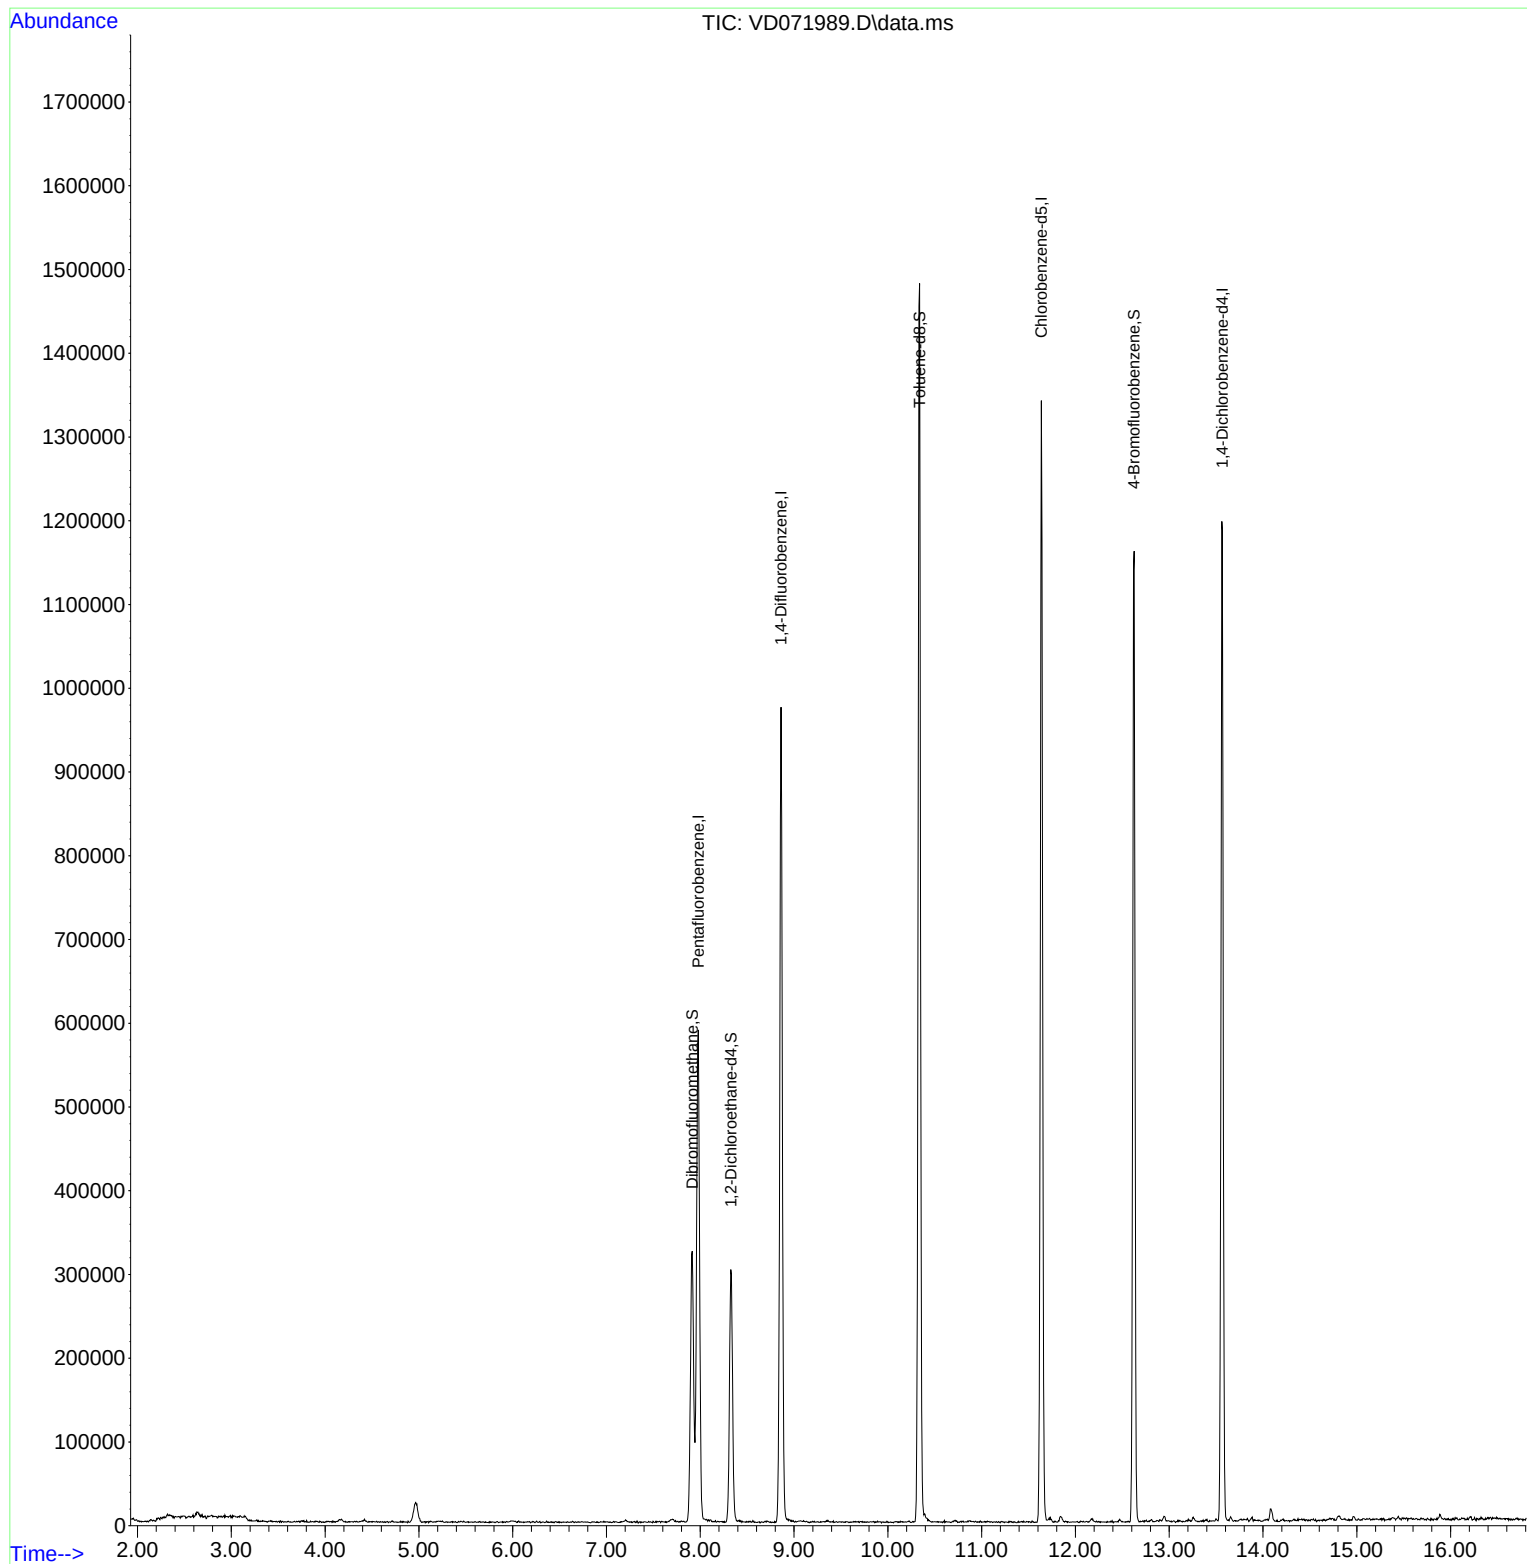


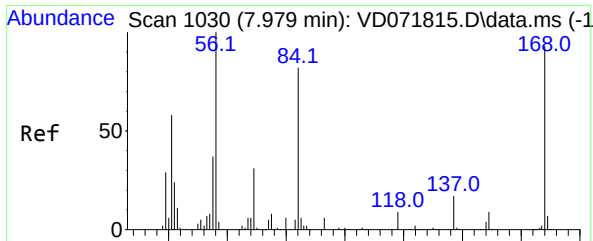

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44




Instrument :
MSVOA_D
ClientSampleId :
BU-03-021522


Tgt Ion:168 Resp: 393938
Ion Ratio Lower Upper
168 100
99 62.5 49.8 74.6

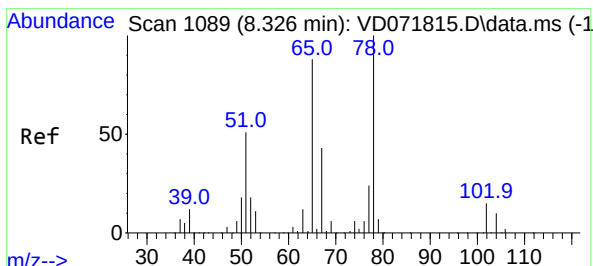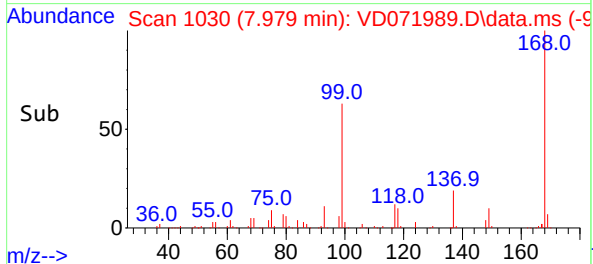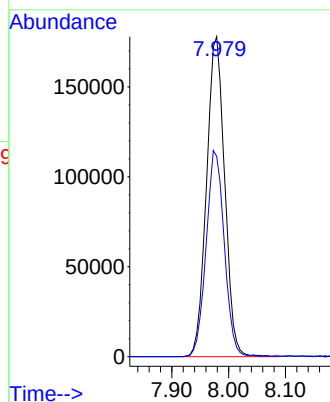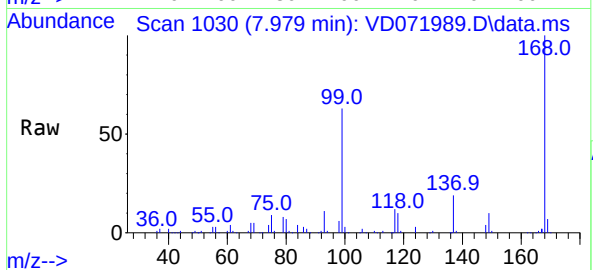

#33
1,2-Dichloroethane-d4
Concen: 49.344 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44

Tgt Ion: 65 Resp: 245691
Ion Ratio Lower Upper
65 100
67 50.6 0.0 101.4

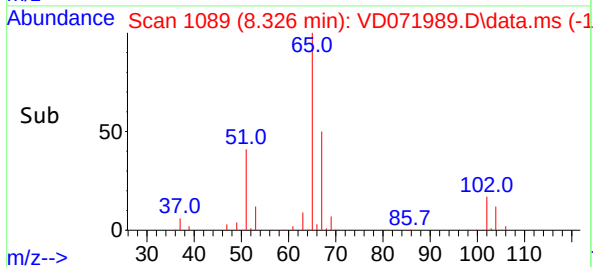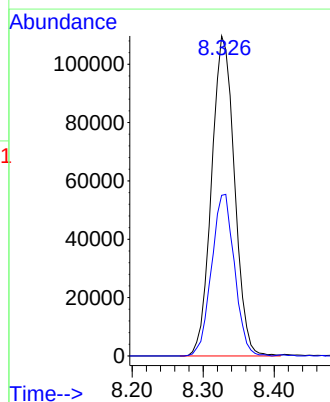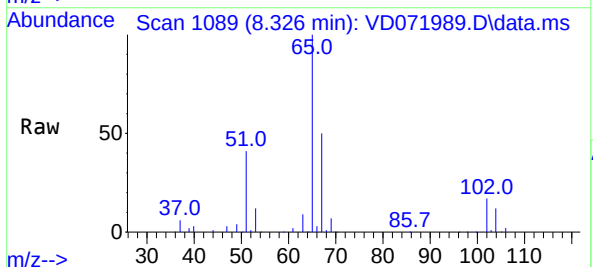




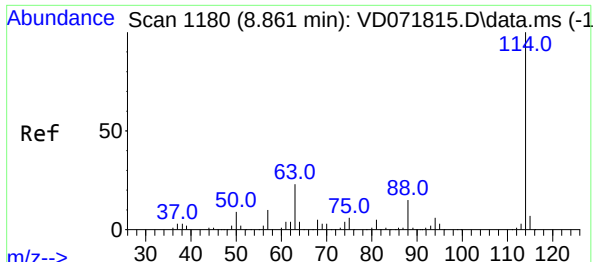


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44

Instrument :
MSVOA_D
ClientSampleId :
BU-03-021522

Tgt Ion:114 Resp: 726898




Ion	Ratio	Lower	Upper
114	100		
63	23.7	0.0	46.6
88	16.6	0.0	33.2

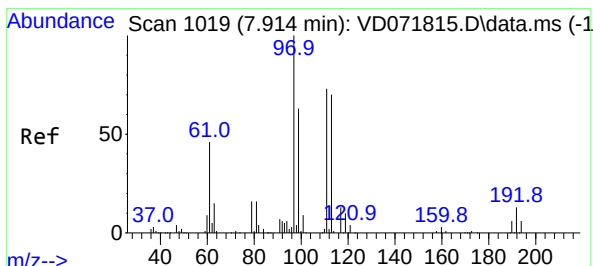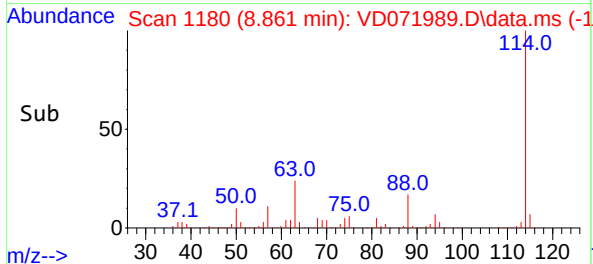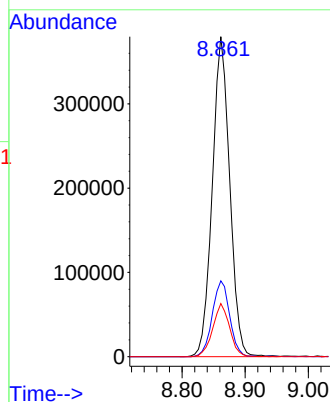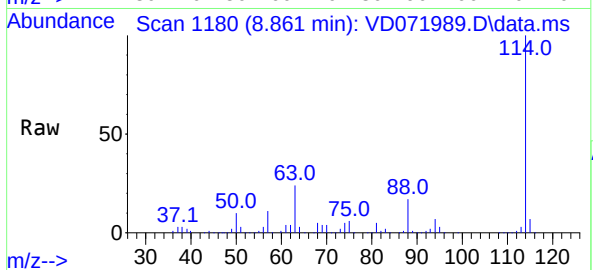


#35
Dibromofluoromethane
Concen: 48.122 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44

Tgt Ion:113 Resp: 229933

Ion	Ratio	Lower	Upper
113	100		
111	103.2	83.8	125.6
192	16.7	14.6	21.8


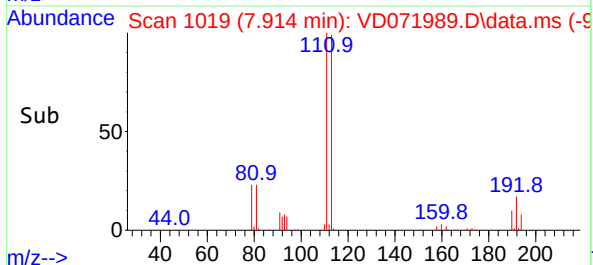
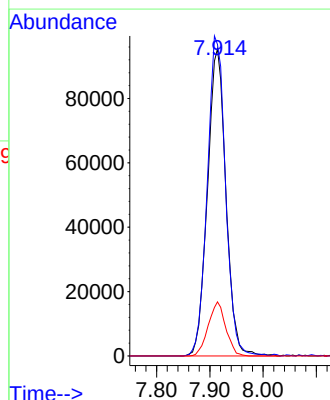
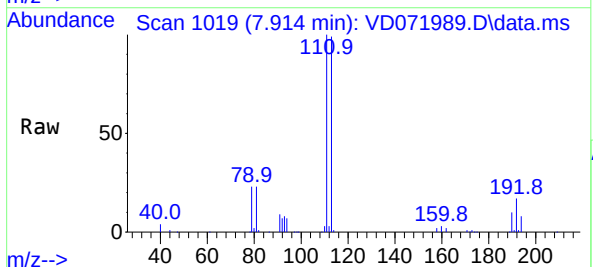


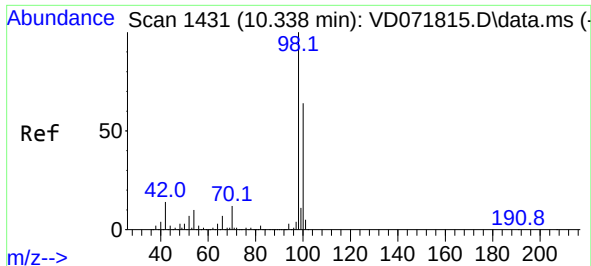

#50
Toluene-d8
Concen: 52.264 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44




Instrument :
MSVOA_D
ClientSampleId :
BU-03-021522


Tgt Ion: 98 Resp: 932624
Ion Ratio Lower Upper
98 100
100 65.9 52.4 78.6

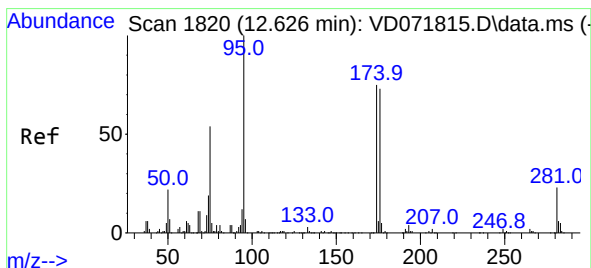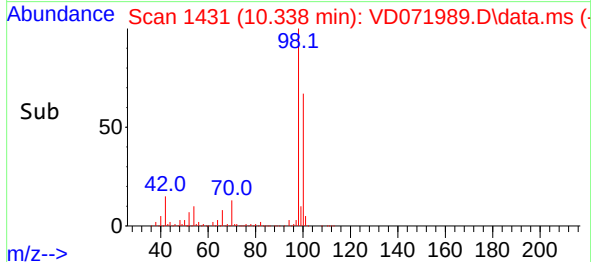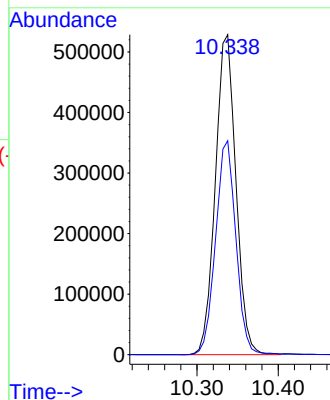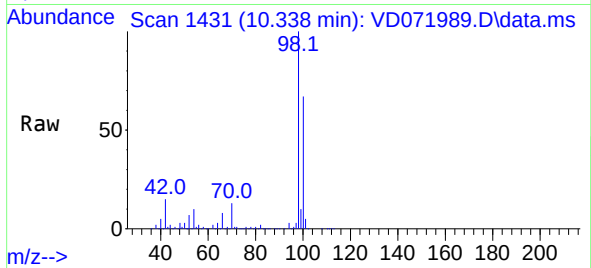

#62
4-Bromofluorobenzene
Concen: 49.095 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44

Tgt Ion: 95 Resp: 305939
Ion Ratio Lower Upper
95 100
174 75.0 0.0 152.8
176 71.4 0.0 145.4


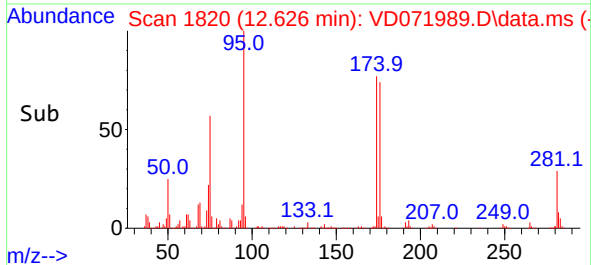
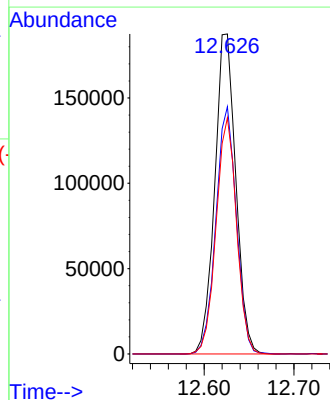
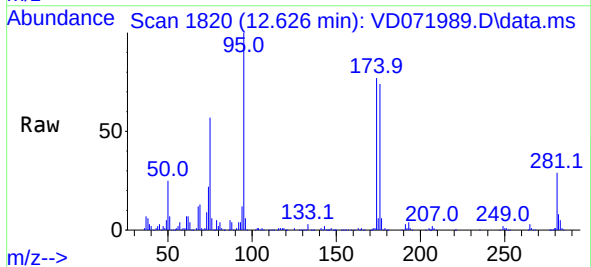


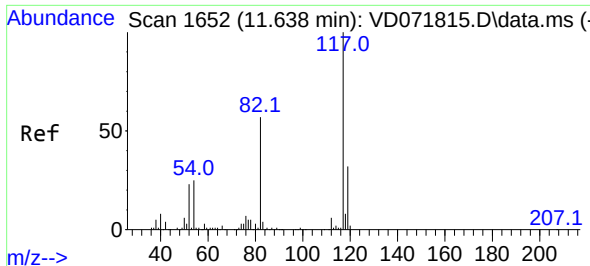

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44

Instrument :
MSVOA_D
ClientSampleId :
BU-03-021522

Tgt Ion:117 Resp: 683691
Ion Ratio Lower Upper
117 100
82 57.7 45.3 67.9
119 31.5 26.6 40.0

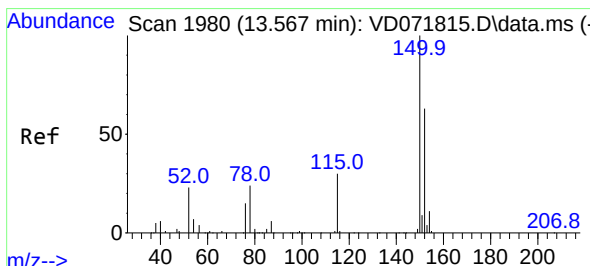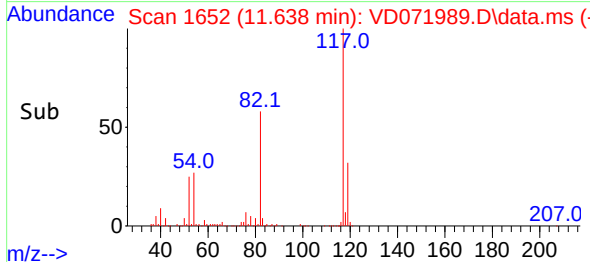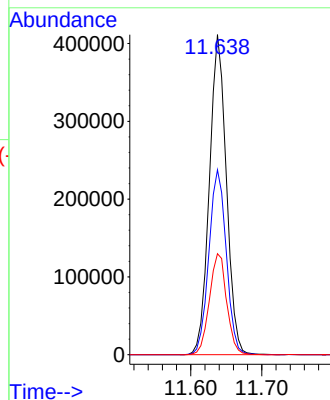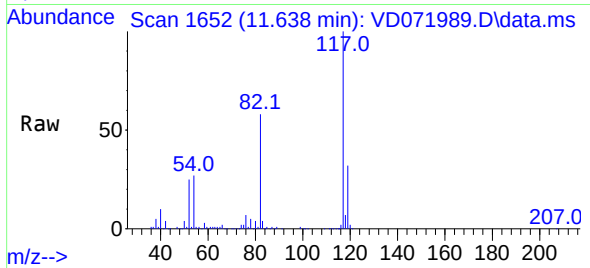

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD071989.D
Acq: 16 Feb 2022 13:44

Tgt Ion:152 Resp: 288511
Ion Ratio Lower Upper
152 100
115 62.5 31.3 93.8
150 158.0 0.0 348.6

