
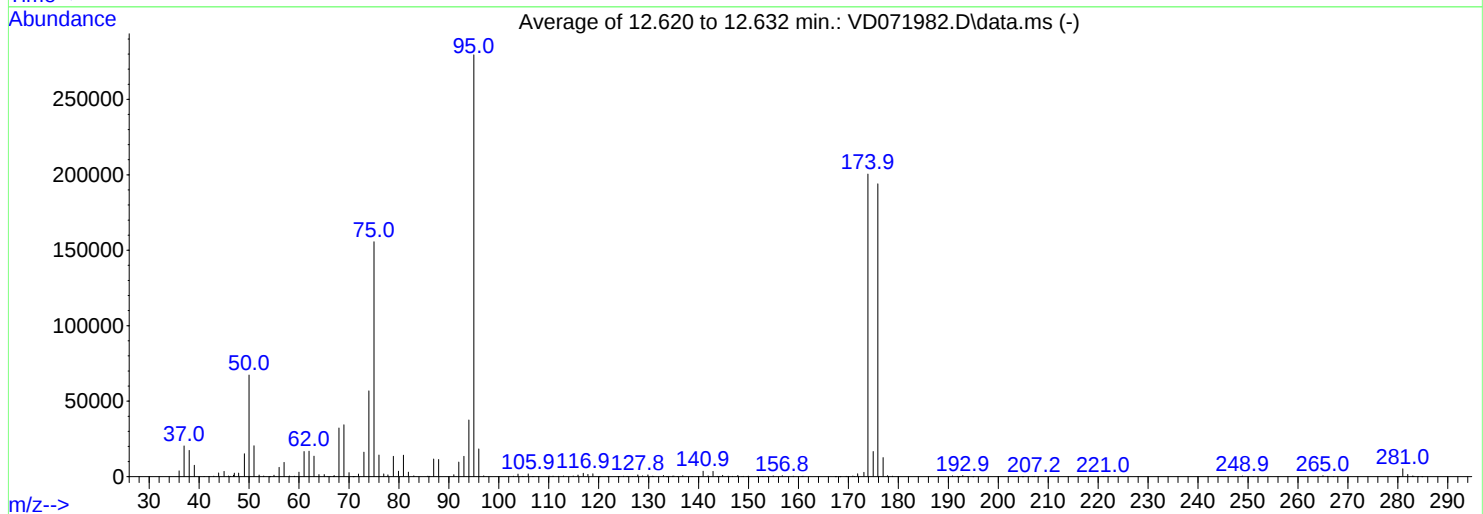


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021622\
 Data File : VD071982.D
 Acq On : 16 Feb 2022 09:07
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Title : SW846 8260
 Last Update : Thu Jan 27 06:04:38 2022

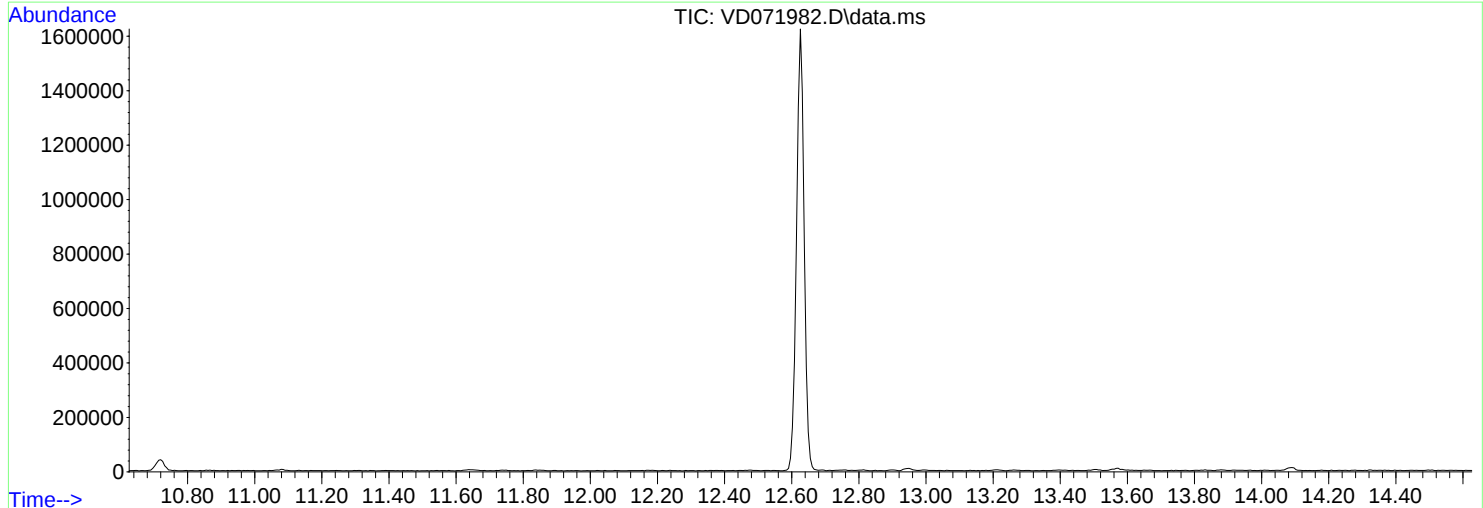

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	67296	PASS
75	95	30	60	55.7	155691	PASS
95	95	100	100	100.0	279488	PASS
96	95	5	9	6.6	18395	PASS
173	174	0.00	2	1.4	2843	PASS
174	95	50	100	71.7	200491	PASS
175	174	5	9	8.3	16702	PASS
176	174	95	101	96.8	194027	PASS
177	176	5	9	6.5	12618	PASS