
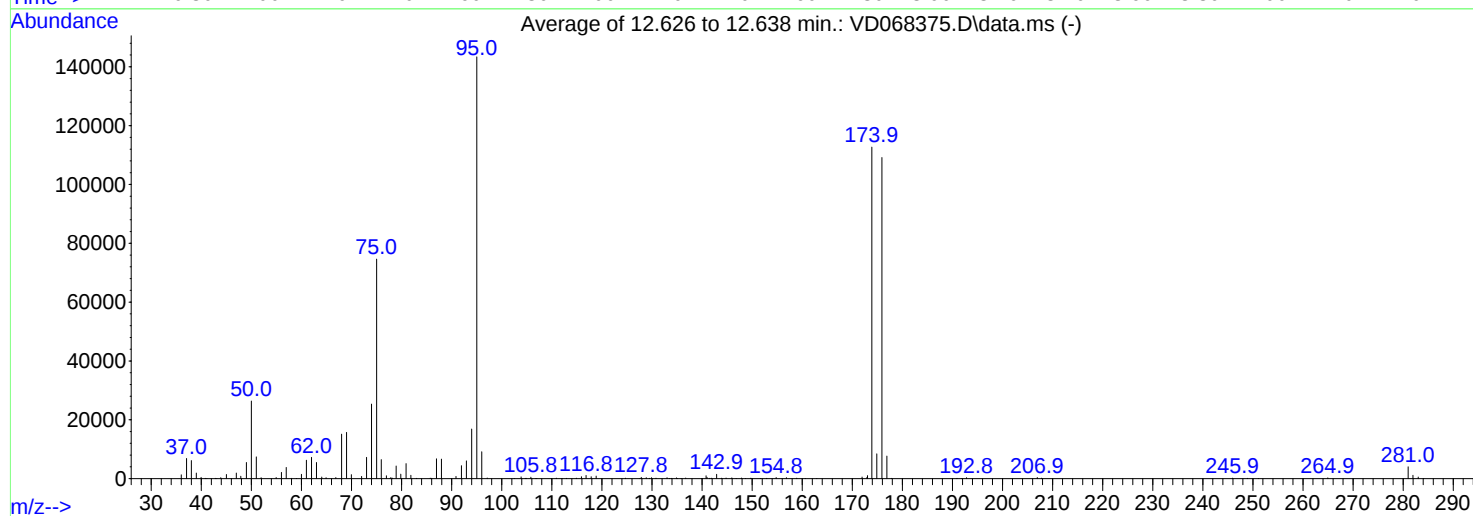


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021721\
Data File : VD068375.D
Acq On : 17 Feb 2021 09:58
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
Title : SW846 8260
Last Update : Fri Feb 12 13:30:51 2021

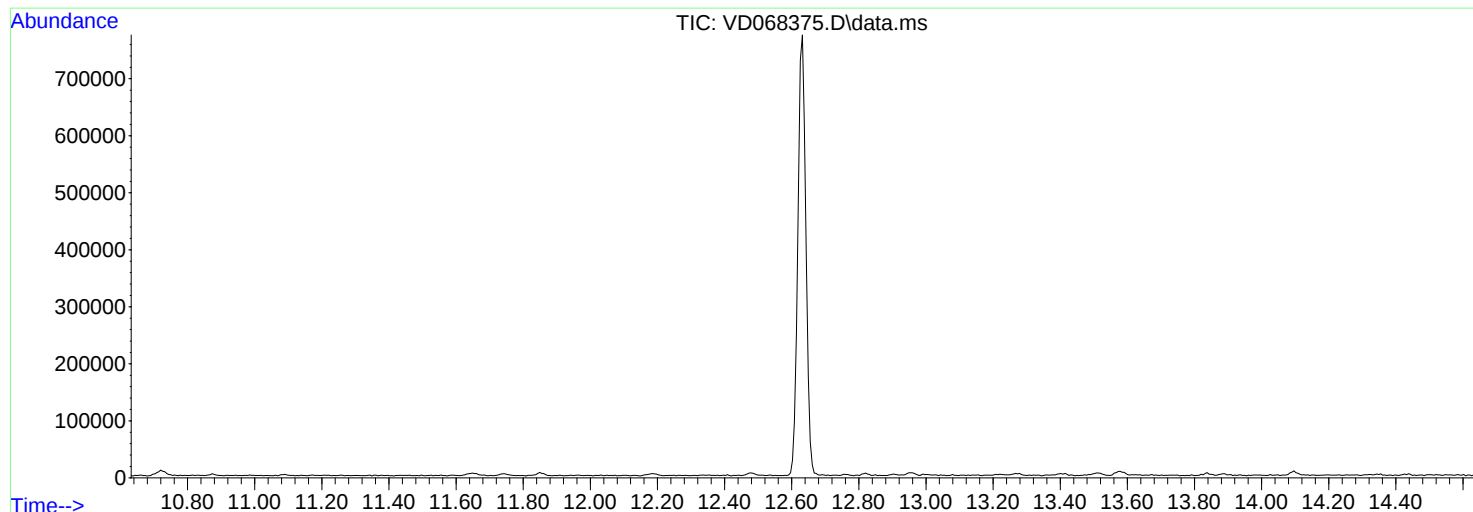

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	26392	PASS
75	95	30	60	52.1	74648	PASS
95	95	100	100	100.0	143387	PASS
96	95	5	9	6.4	9141	PASS
173	174	0.00	2	0.9	1050	PASS
174	95	50	100	78.6	112696	PASS
175	174	5	9	7.5	8459	PASS
176	174	95	101	96.8	109136	PASS
177	176	5	9	7.0	7650	PASS