



Methylene Chloride

Response Ratio

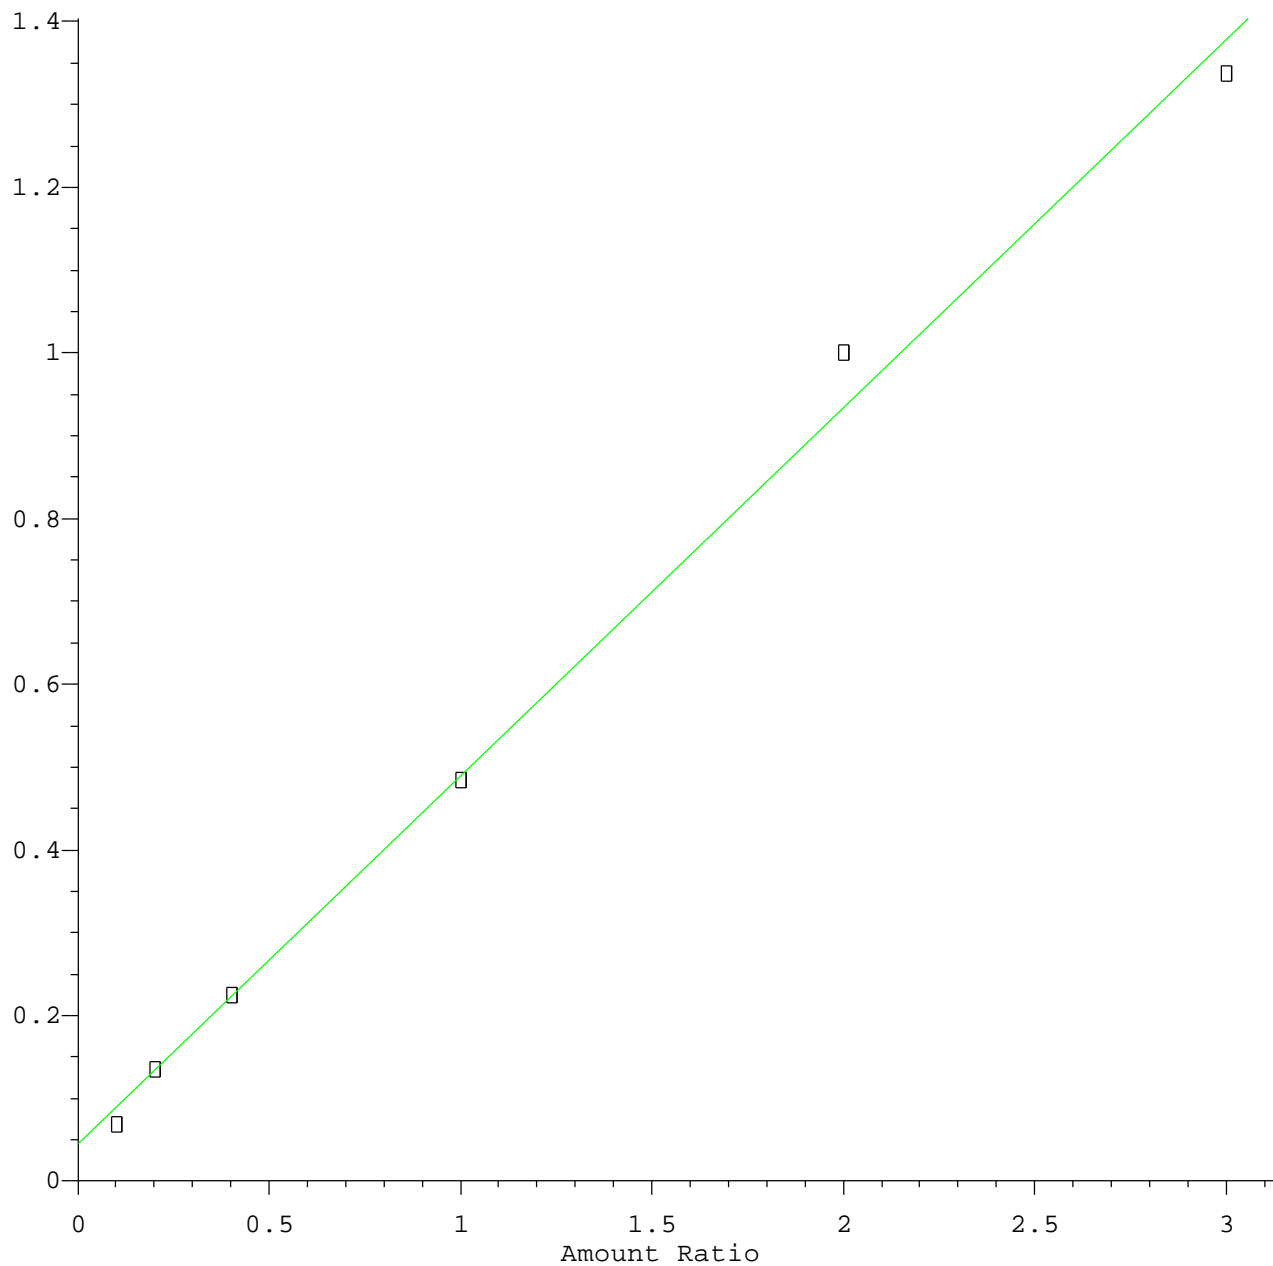

Resp Ratio = $4.44 \times 10^{-1} \times \text{Amt} + 4.51 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
Calibration Table Last Updated: Wed Feb 19 03:26:54 2020

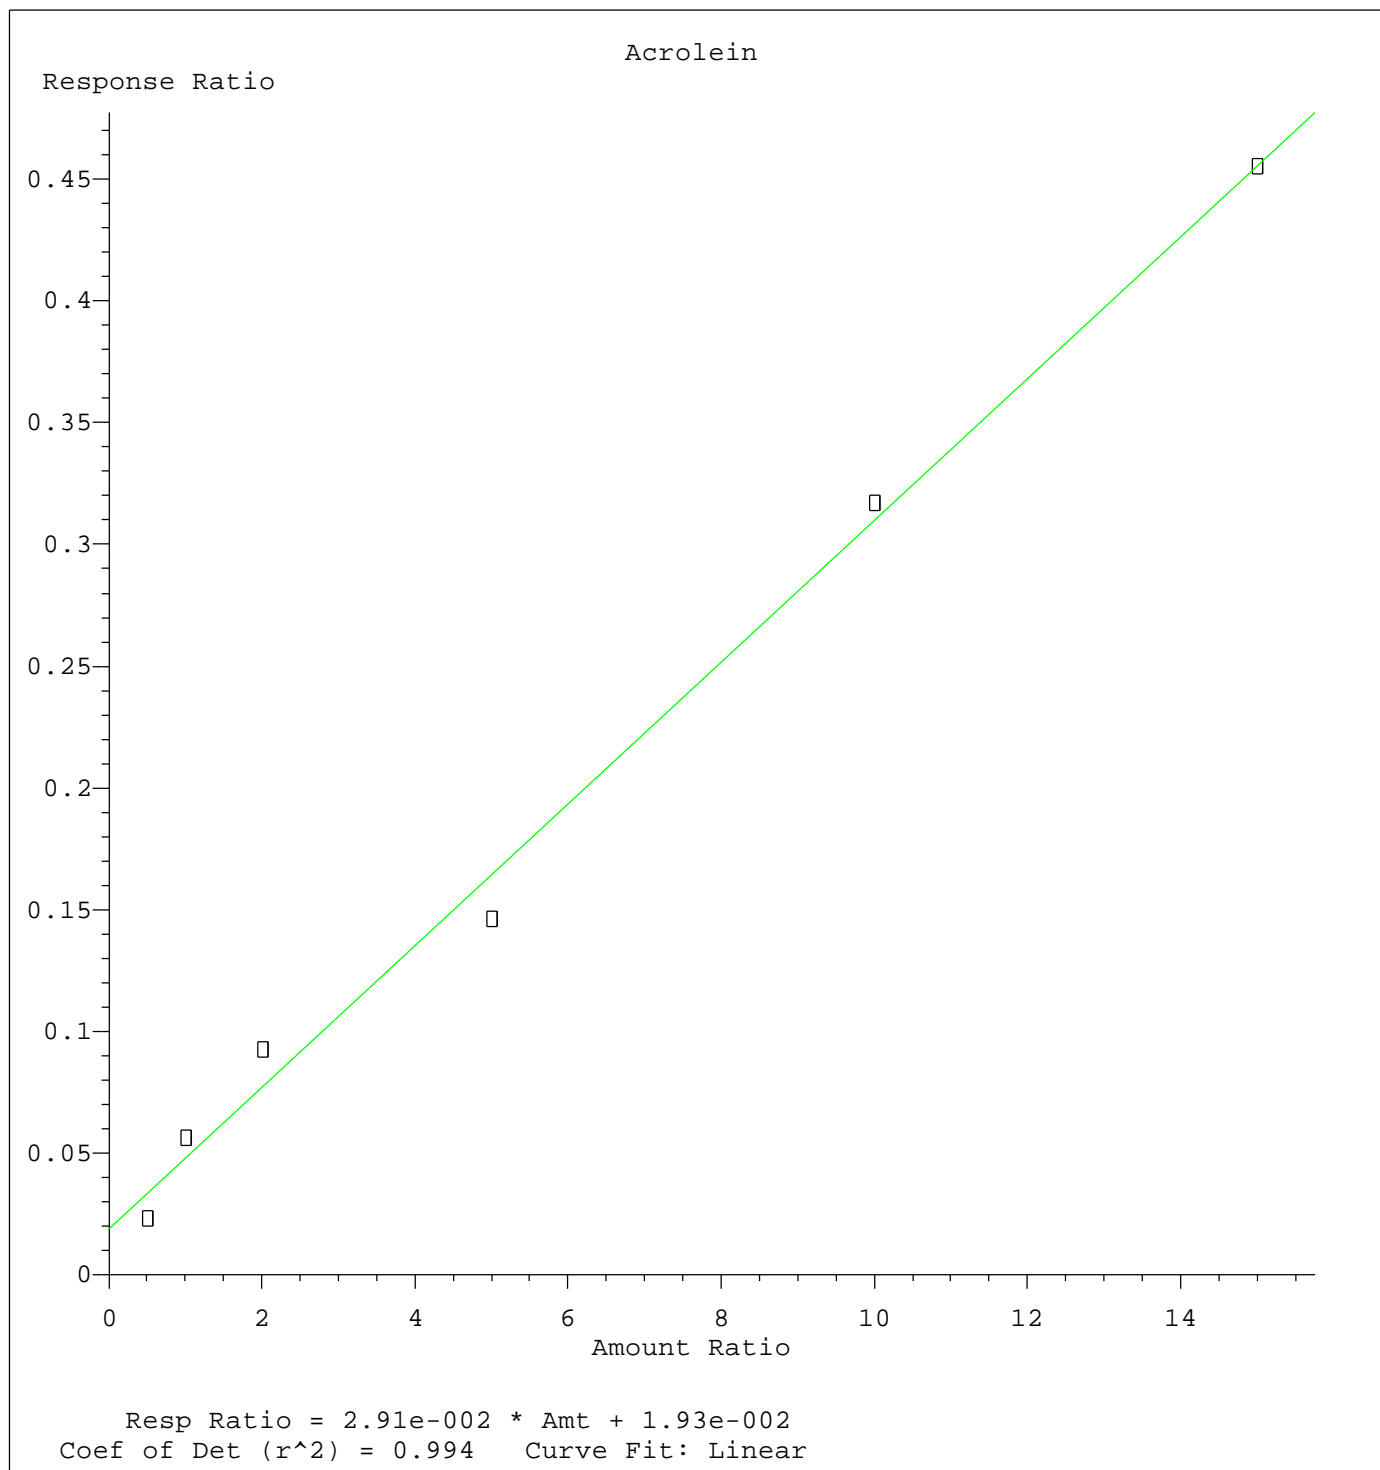

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
Calibration Table Last Updated: Wed Feb 19 03:26:54 2020