
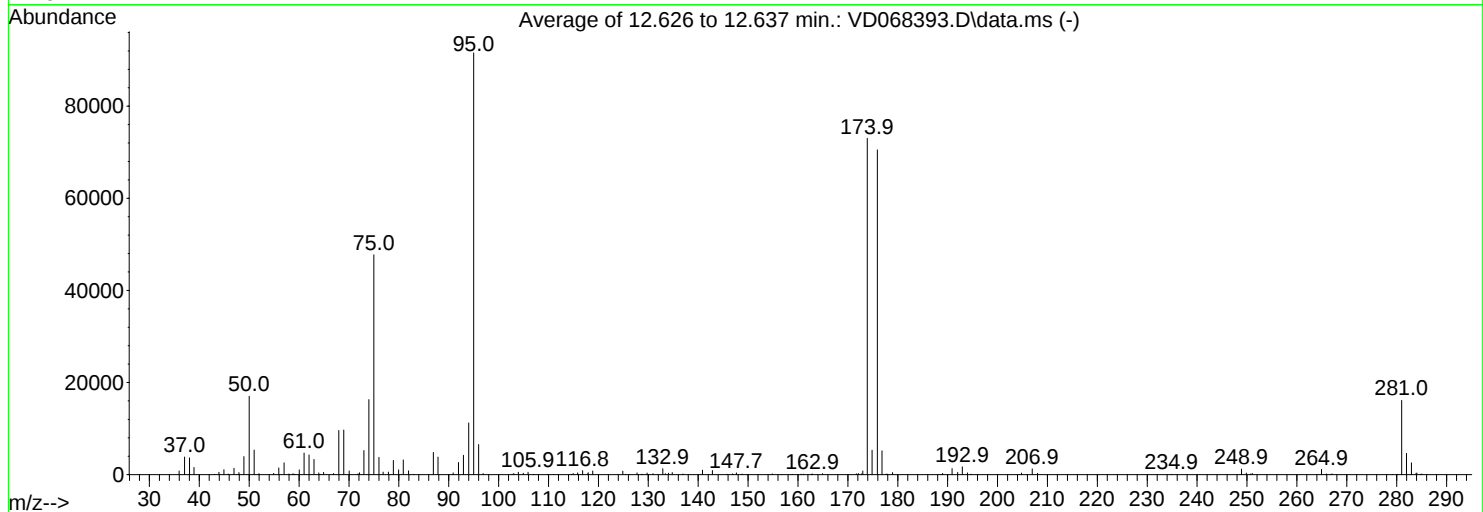


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021921\
Data File : VD068393.D
Acq On : 19 Feb 2021 11:23
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
Title : SW846 8260
Last Update : Fri Feb 12 13:30:51 2021

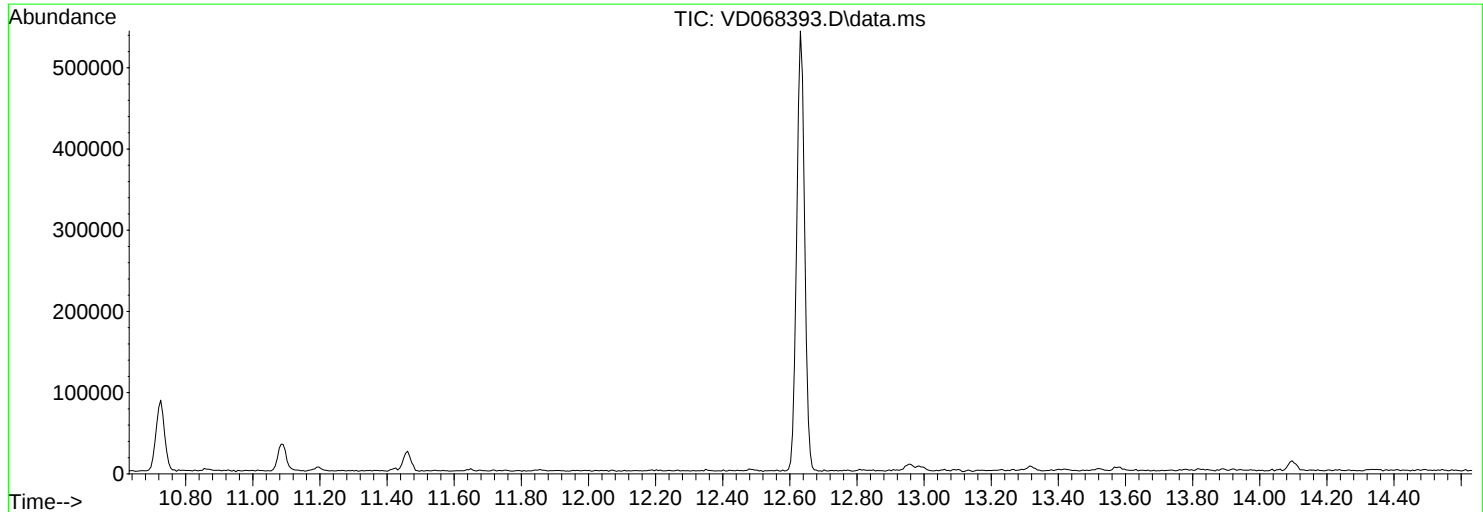

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	17034	PASS
75	95	30	60	52.1	47741	PASS
95	95	100	100	100.0	91584	PASS
96	95	5	9	7.1	6531	PASS
173	174	0.00	2	1.1	807	PASS
174	95	50	100	79.7	73021	PASS
175	174	5	9	7.3	5326	PASS
176	174	95	101	96.6	70541	PASS
177	176	5	9	7.4	5185	PASS