


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD022119\
Data File : VD060884.D
Acq On : 21 Feb 2019 13:13
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D022119S.M
Title : SW846 8260
Last Update : Fri Feb 22 07:56:08 2019

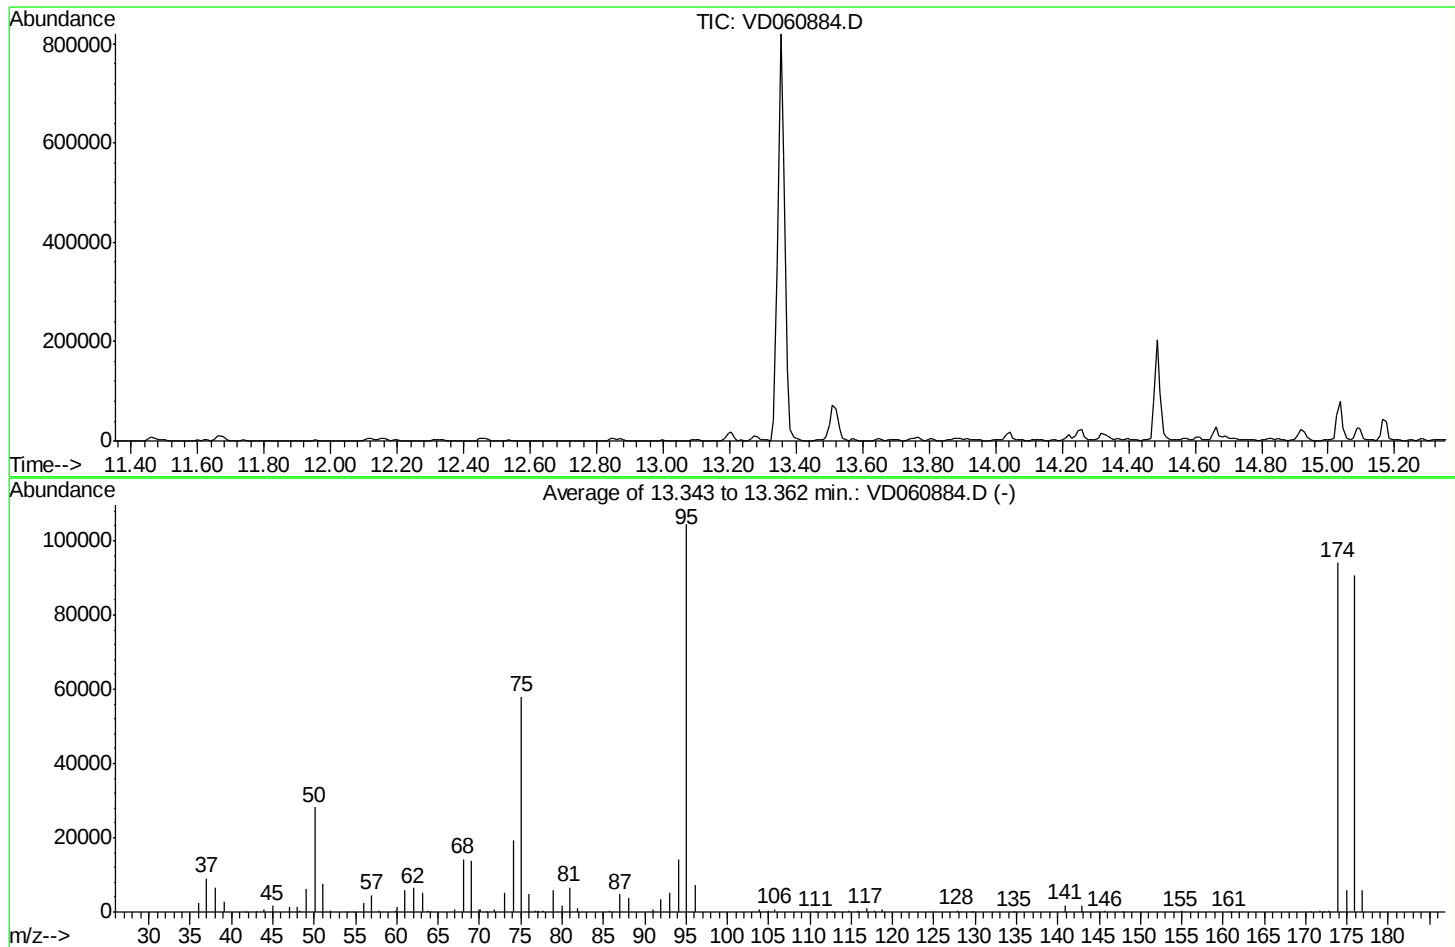

AutoFind: Scans 1251, 1252, 1253; Background Corrected with Scan 1247

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.1	28258	PASS
75	95	30	60	55.6	58098	PASS
95	95	100	100	100.0	104442	PASS
96	95	5	9	7.0	7329	PASS
173	174	0.00	2	0.2	201	PASS
174	95	50	100	90.1	94085	PASS
175	174	5	9	6.3	5973	PASS
176	174	95	101	96.4	90666	PASS
177	176	5	9	6.4	5790	PASS