

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022123\
 Data File : VD075389.D
 Acq On : 21 Feb 2023 19:06
 Operator : KP/SY
 Sample : 01613-06RE
 Misc : 5.04G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BP-VPB-RW10-GW-838-840RE

Quant Time: Feb 22 00:54:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022123S.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 21 16:26:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	41537	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	72511	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.580	117	62142	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	22920	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	24281	69.104	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	138.200%
35) Dibromofluoromethane	7.810	113	26127	60.696	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	121.400%
50) Toluene-d8	10.269	98	81711	52.598	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	105.200%
62) 4-Bromofluorobenzene	12.575	95	24126	46.250	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	92.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022123\
Data File : VD075389.D
Acq On : 21 Feb 2023 19:06
Operator : KP/SY
Sample : 01613-06RE
Misc : 5.04G/5.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BP-VPB-RW10-GW-838-840RE

Quant Time: Feb 22 00:54:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022123S.M
Quant Title : SW846 8260
QLast Update : Tue Feb 21 16:26:04 2023
Response via : Initial Calibration




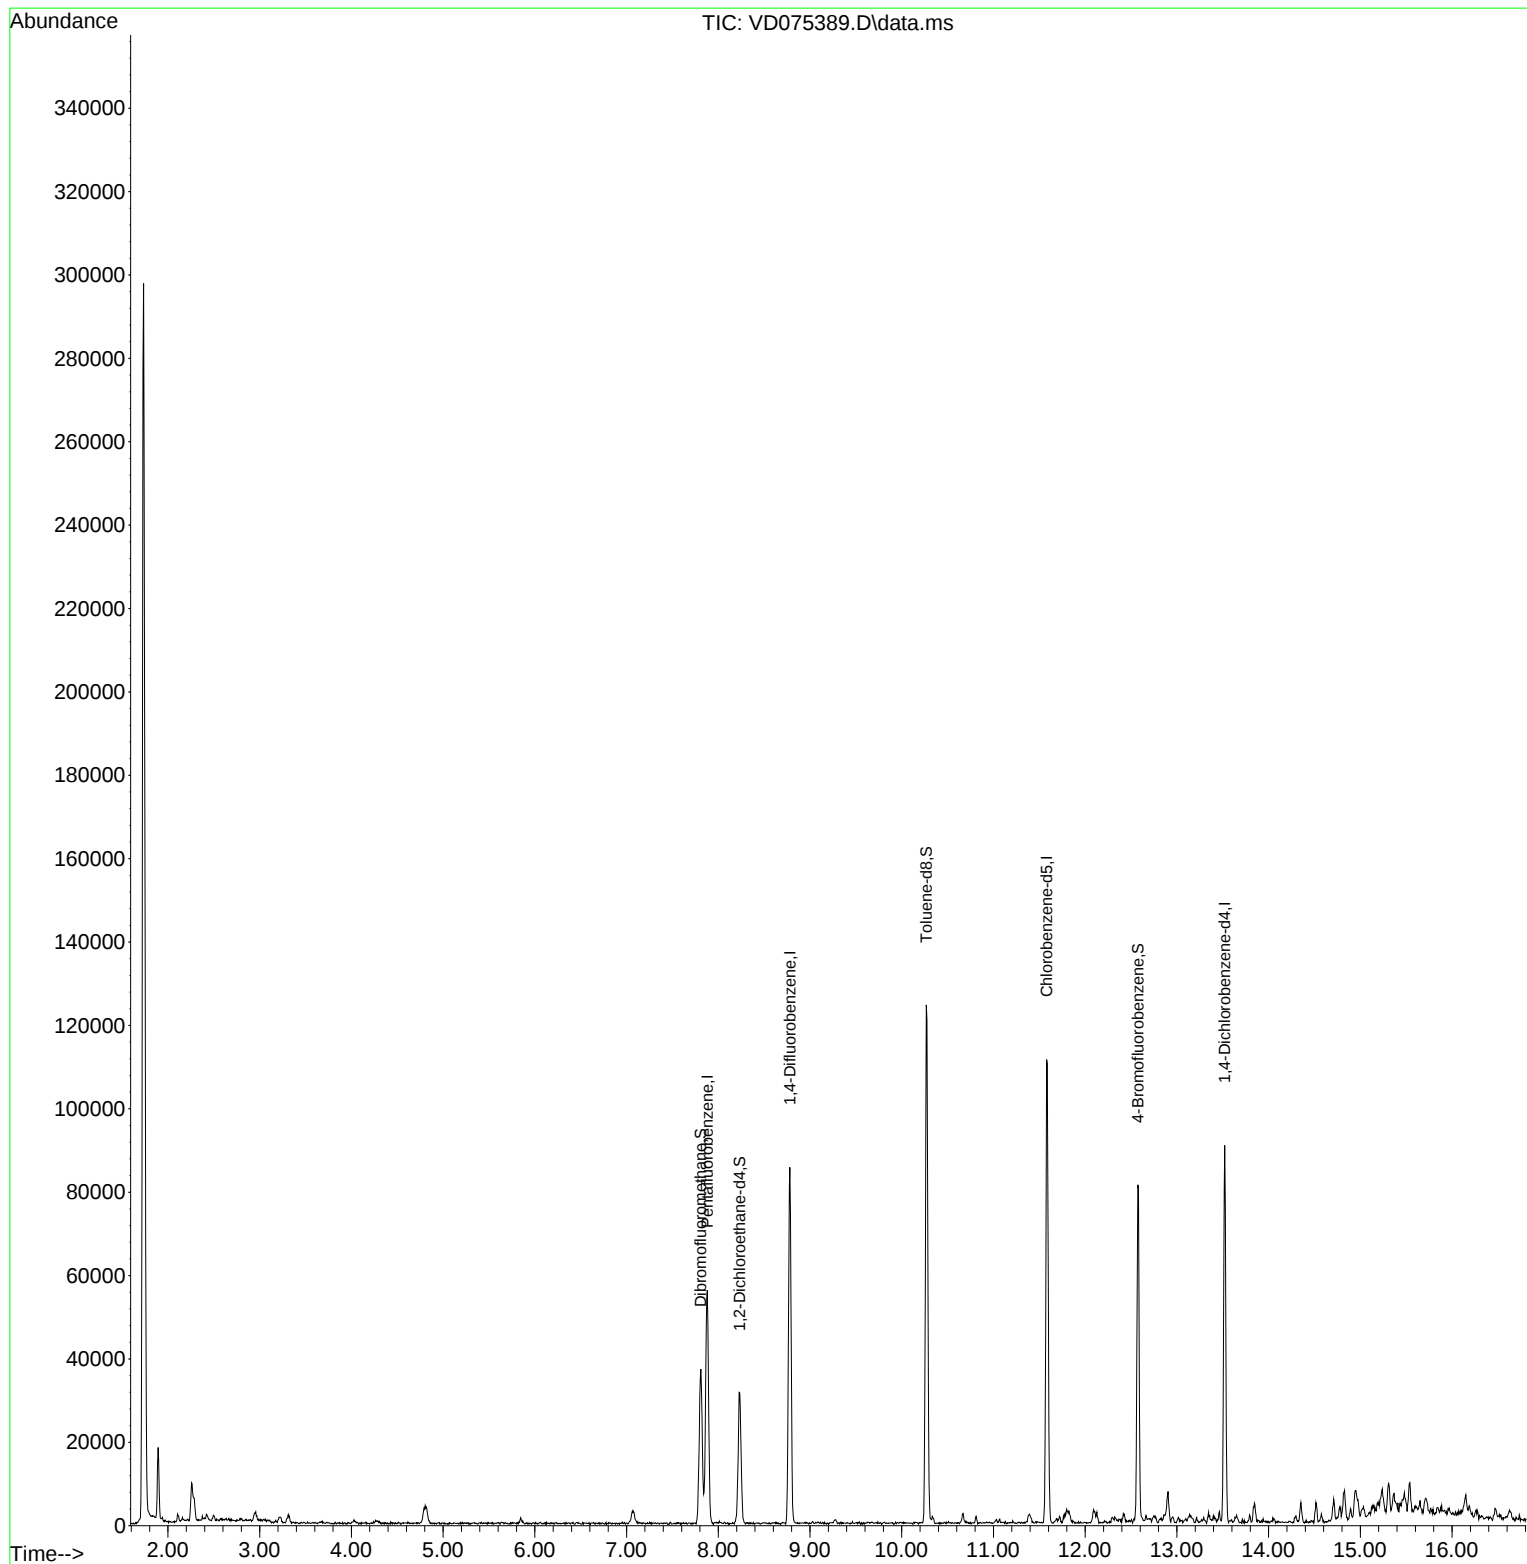


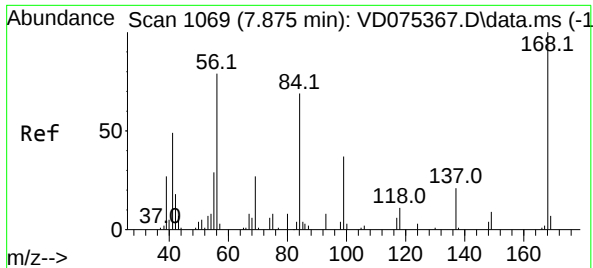

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1069
Delta R.T. 0.006 min
Lab File: VD075389.D
Acq: 21 Feb 2023 19:06




Instrument :
MSVOA_D
ClientSampleId :
BP-VPB-RW10-GW-838-840RE


Tgt Ion:168 Resp: 41537
Ion Ratio Lower Upper
168 100
99 59.2 43.8 65.6

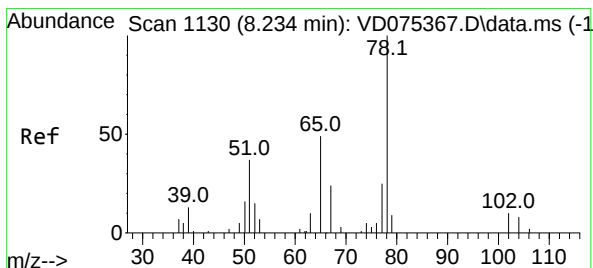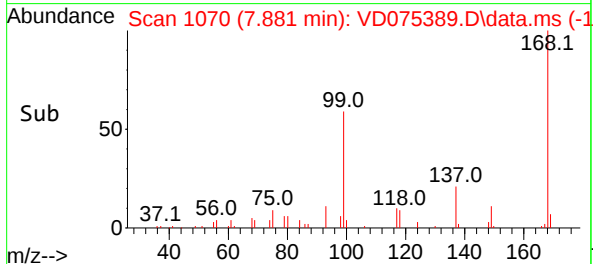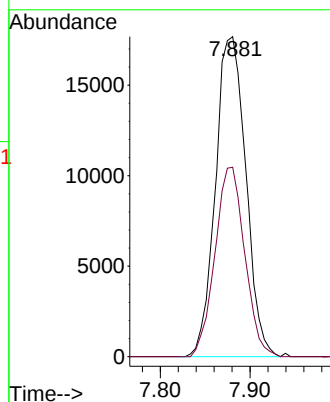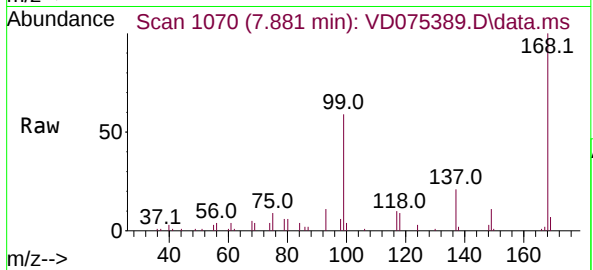

#33
1,2-Dichloroethane-d4
Concen: 69.104 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VD075389.D
Acq: 21 Feb 2023 19:06

Tgt Ion: 65 Resp: 24281
Ion Ratio Lower Upper
65 100
67 51.6 0.0 102.2

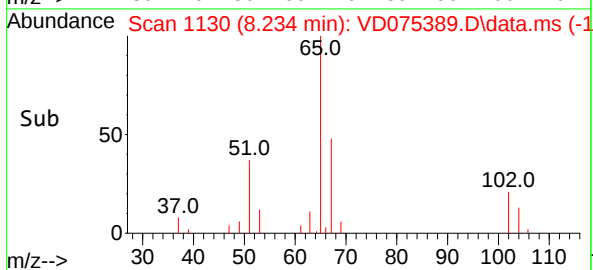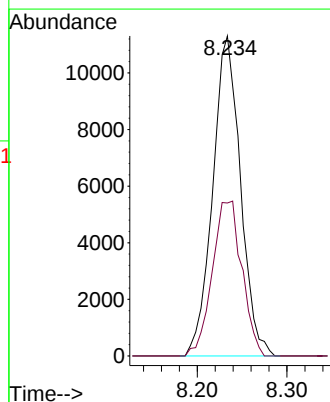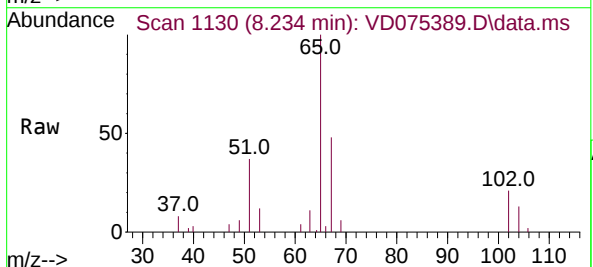

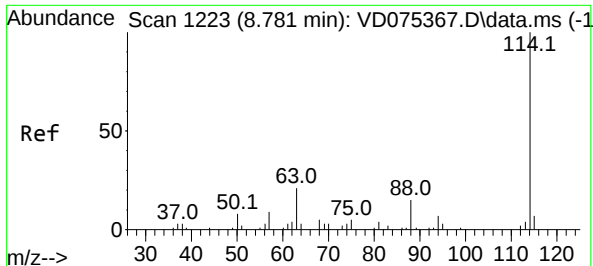

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD075389.D

Acq: 21 Feb 2023 19:06

Instrument :

MSVOA_D

ClientSampleId :

BP-VPB-RW10-GW-838-840RE





Tgt Ion:114 Resp: 72511

Ion Ratio Lower Upper

114 100

63 20.6 0.0 41.6

88 14.1 0.0 30.6

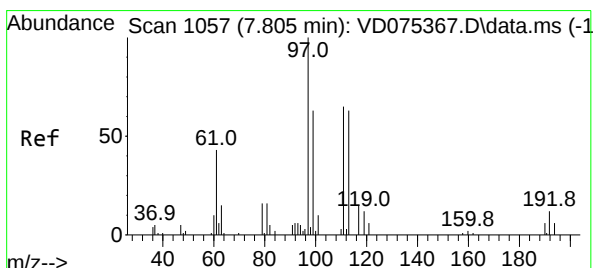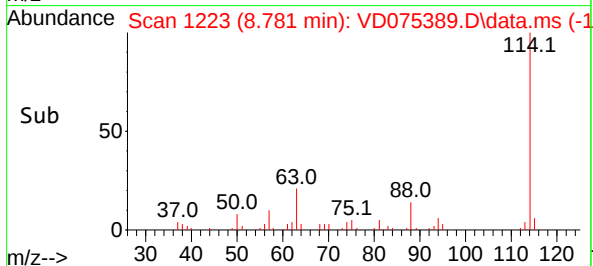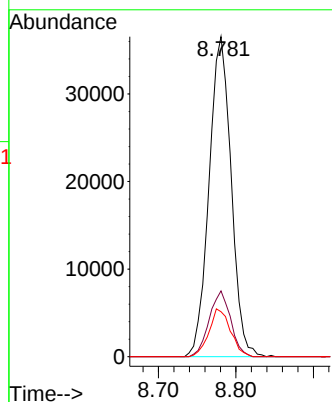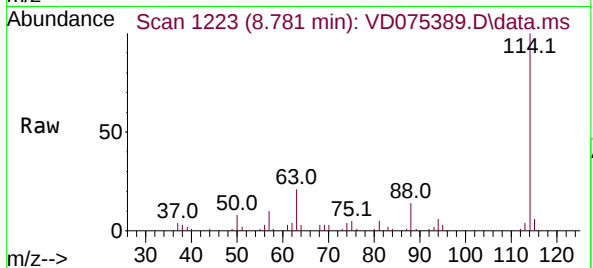

#35

Dibromofluoromethane

Concen: 60.696 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.005 min

Lab File: VD075389.D

Acq: 21 Feb 2023 19:06




Tgt Ion:113 Resp: 26127


Ion Ratio Lower Upper

113 100

111 102.4 81.4 122.0

192 18.2 15.2 22.8


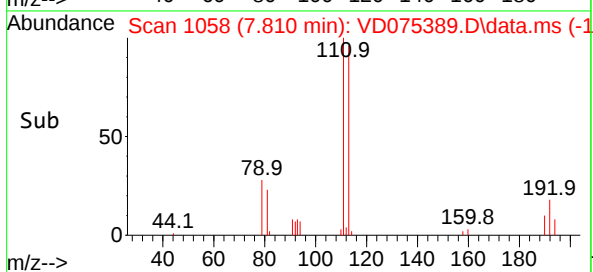
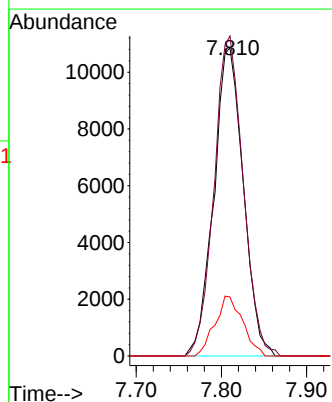
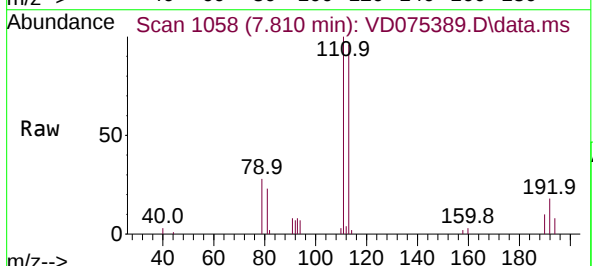


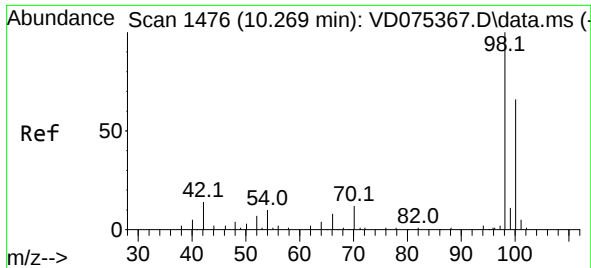

#50
Toluene-d8
Concen: 52.598 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD075389.D
Acq: 21 Feb 2023 19:06




Instrument :
MSVOA_D
ClientSampleId :
BP-VPB-RW10-GW-838-840RE


Tgt Ion: 98 Resp: 81711
Ion Ratio Lower Upper
98 100
100 64.2 52.1 78.1

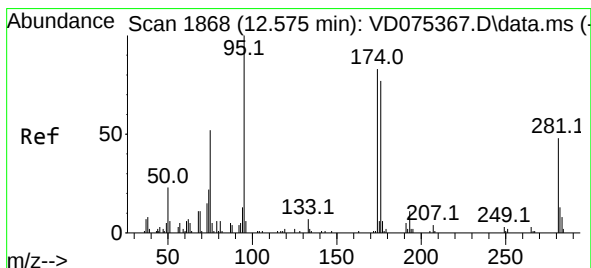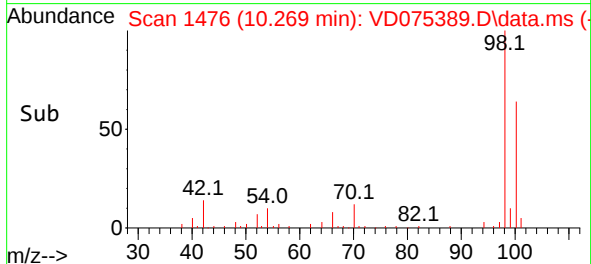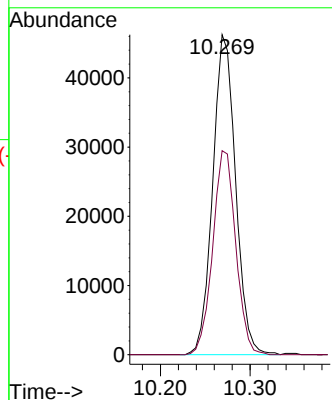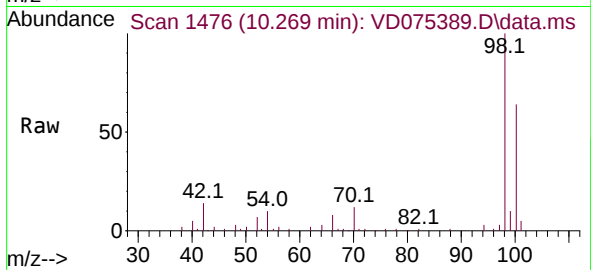

#62
4-Bromofluorobenzene
Concen: 46.250 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD075389.D
Acq: 21 Feb 2023 19:06

Tgt Ion: 95 Resp: 24126
Ion Ratio Lower Upper
95 100
174 88.0 0.0 164.0
176 81.0 0.0 156.8


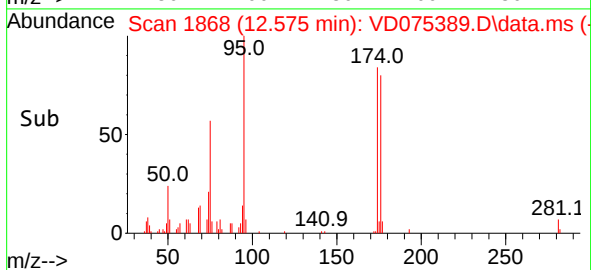
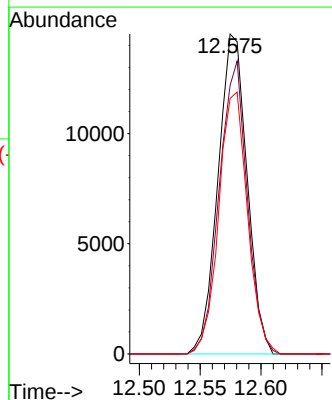
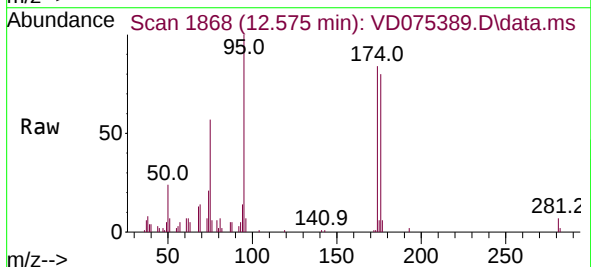


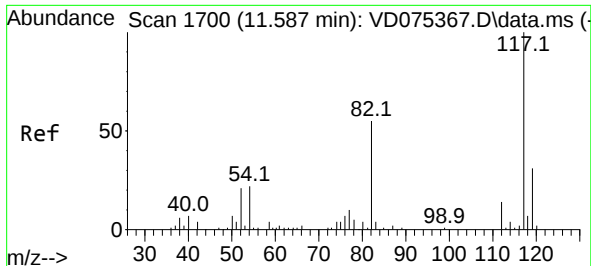

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.580 min Scan# 11
Delta R.T. -0.007 min
Lab File: VD075389.D
Acq: 21 Feb 2023 19:06

Instrument :
MSVOA_D
ClientSampleId :
BP-VPB-RW10-GW-838-840RE

Tgt Ion:117 Resp: 62142
Ion Ratio Lower Upper
117 100
82 52.7 44.0 66.0
119 30.9 25.1 37.7

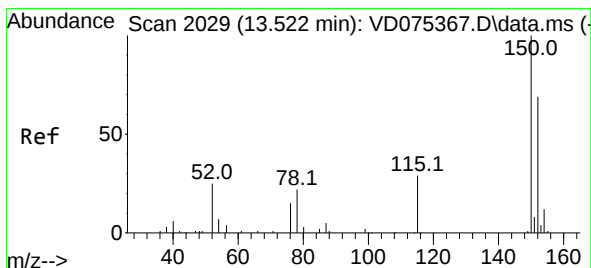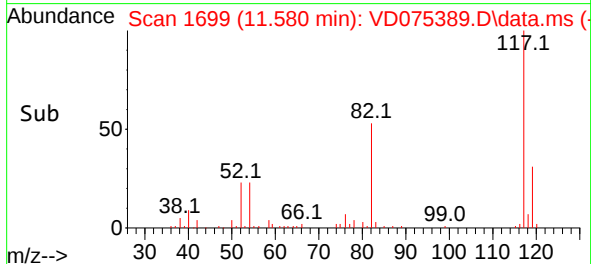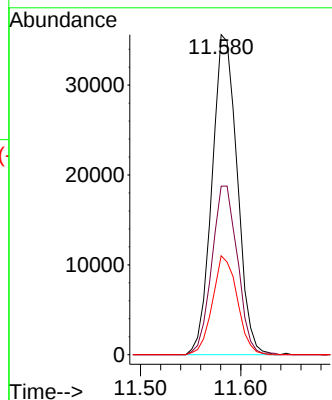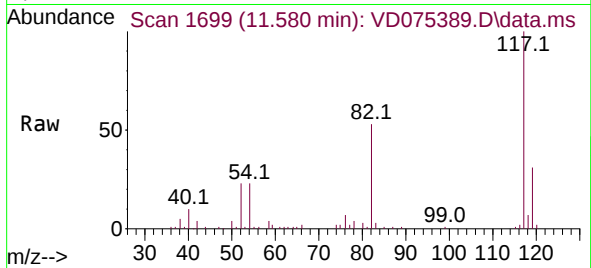

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD075389.D
Acq: 21 Feb 2023 19:06

Tgt Ion:152 Resp: 22920
Ion Ratio Lower Upper
152 100
115 58.5 30.1 90.3
150 148.8 0.0 364.8

