
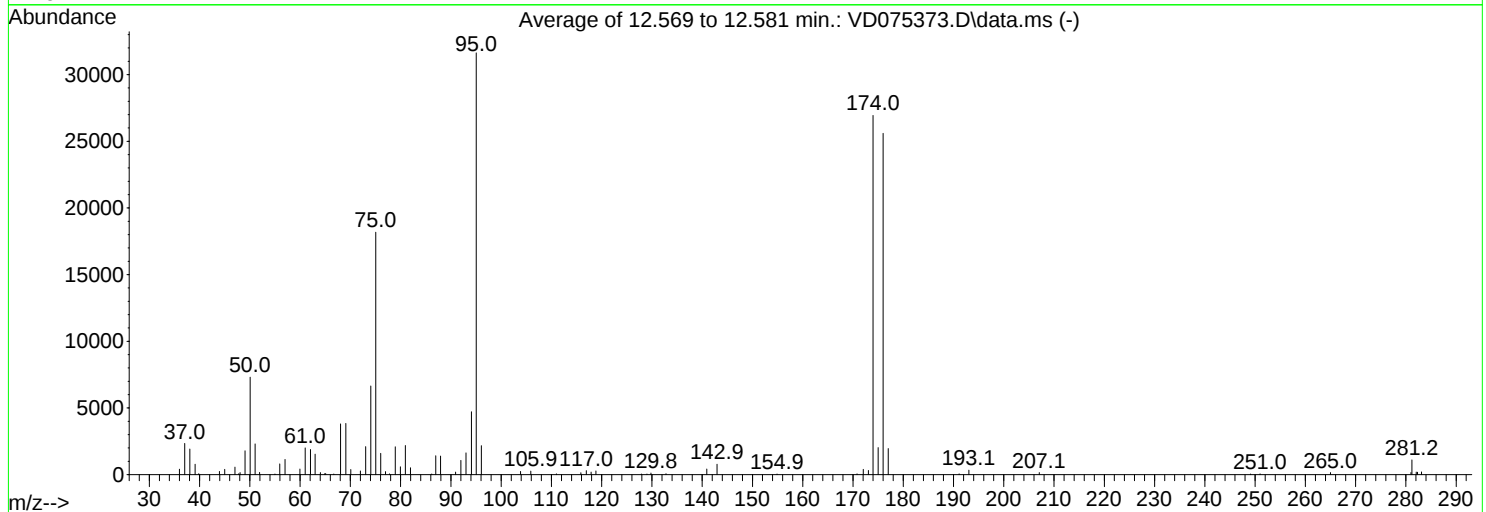


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022123\
Data File : VD075373.D
Acq On : 21 Feb 2023 09:51
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022123S.M
Title : SW846 8260
Last Update : Tue Feb 21 16:26:04 2023

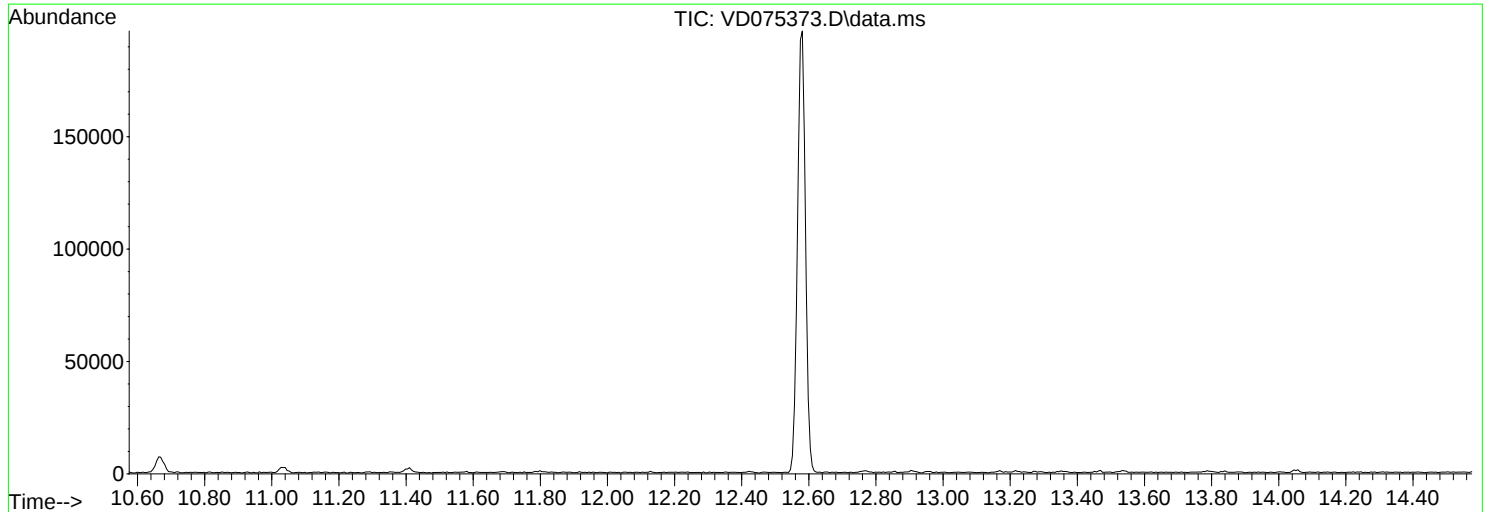

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.1	7305	PASS
75	95	30	60	57.5	18187	PASS
95	95	100	100	100.0	31635	PASS
96	95	5	9	6.9	2173	PASS
173	174	0.00	2	1.2	310	PASS
174	95	50	100	85.2	26944	PASS
175	174	5	9	7.5	2026	PASS
176	174	95	101	95.0	25603	PASS
177	176	5	9	7.6	1955	PASS