
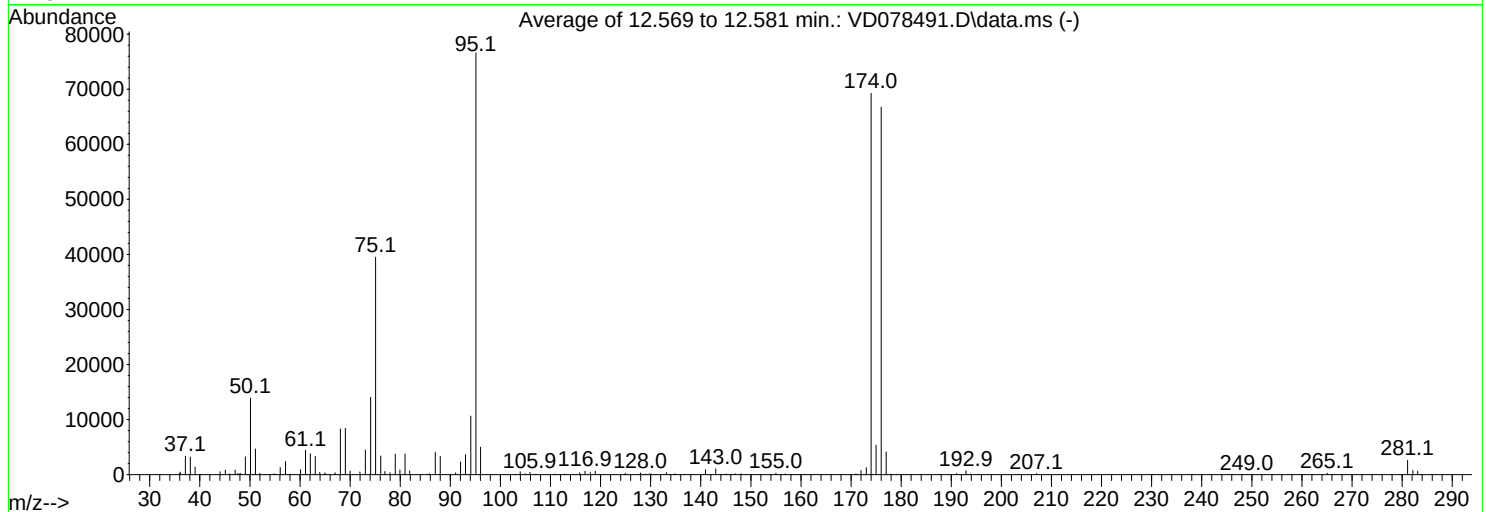


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022124\
Data File : VD078491.D
Acq On : 21 Feb 2024 08:52
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021324S.M
Title : SW846 8260
Last Update : Wed Feb 14 01:16:20 2024

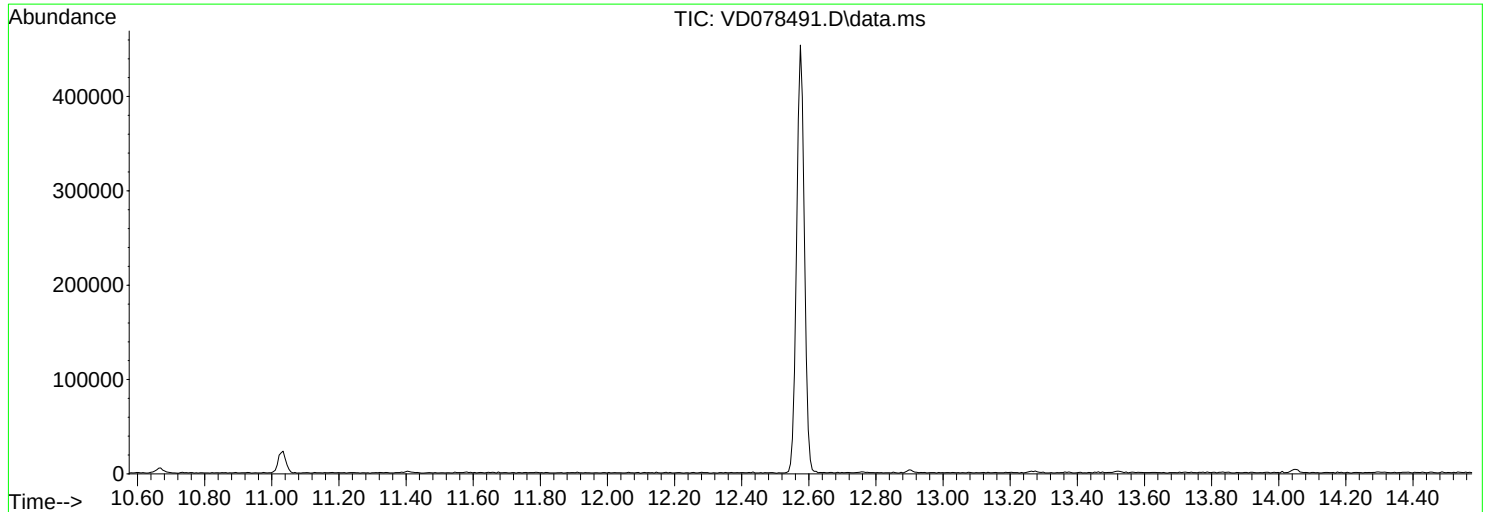

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	13888	PASS
75	95	30	60	51.6	39509	PASS
95	95	100	100	100.0	76611	PASS
96	95	5	9	6.5	5001	PASS
173	174	0.00	2	1.8	1280	PASS
174	95	50	100	90.4	69264	PASS
175	174	5	9	7.8	5368	PASS
176	174	95	101	96.4	66749	PASS
177	176	5	9	6.2	4139	PASS