

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022221\
 Data File : VD068414.D
 Acq On : 22 Feb 2021 12:29
 Operator : VA/SY
 Sample : M1442-01RE
 Misc : 10.17G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Feb 22 15:18:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 12 13:30:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.979	168	295196	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	553341	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.649	117	496945	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	218120	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	183640	60.85	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 121.70%			
35) Dibromofluoromethane	7.914	113	176337	53.69	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 107.38%			
50) Toluene-d8	10.343	98	716495	52.63	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 105.26%			
62) 4-Bromofluorobenzene	12.631	95	249477	56.26	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 112.52%			
Target Compounds					Qvalue	
16) Acetone	4.161	43	37234	79.97	ug/l	99
20) Methylene Chloride	4.955	84	3898	Below Cal	#	86
25) 2-Butanone	7.220	43	2161	3.32	ug/l	93
39) Methylcyclohexane	9.355	83	102683	17.10	ug/l	96
48) Methyl methacrylate	9.396	41	5982	3.78	ug/l	# 27
51) 4-Methyl-2-Pentanone	10.232	43	2556	1.57	ug/l	# 82
55) 1,1,2-Trichloroethane	10.779	97	185334	72.58	ug/l	# 23
56) Ethyl methacrylate	10.679	69	38942	12.85	ug/l	# 4
59) 2-Hexanone	10.955	43	178747	162.54	ug/l	# 25
67) Ethyl Benzene	11.743	91	32663	1.91	ug/l	93
68) m/p-Xylenes	11.855	106	16097	2.49	ug/l	# 66
69) o-Xylene	12.184	106	37211	6.26	ug/l	89
73) Isopropylbenzene	12.484	105	153738	9.65	ug/l	89
74) N-amyl acetate	12.273	43	480011	170.62	ug/l	# 58
75) 1,1,2,2-Tetrachloroethane	12.708	83	37649	13.64	ug/l	# 39
76) 1,2,3-Trichloropropane	12.914	75	6454	3.11	ug/l	# 100
78) n-propylbenzene	12.820	91	119404	6.26	ug/l	94
79) 2-Chlorotoluene	12.914	91	87999	8.33	ug/l	# 42
80) 1,3,5-Trimethylbenzene	12.961	105	924191	70.99	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.631	75	106975	129.19	ug/l	# 22
82) 4-Chlorotoluene	12.961	91	116702	10.45	ug/l	# 55
83) tert-Butylbenzene	13.226	119	28632	2.54	ug/l	70
84) 1,2,4-Trimethylbenzene	13.267	105	60680	4.68	ug/l	96
85) sec-Butylbenzene	13.402	105	479720	30.37	ug/l	93
86) p-Isopropyltoluene	13.514	119	408592	28.81	ug/l	99
89) n-Butylbenzene	13.808	91	609681	44.06	ug/l	# 1
90) Hexachloroethane	14.120	117	419131	162.79	ug/l	# 10
92) 1,2-Dibromo-3-Chloropr...	14.520	75	13554	33.57	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.167	180	10542	2.70	ug/l	# 1
95) Naphthalene	15.367	128	80786	11.11	ug/l	# 1
96) 1,2,3-Trichlorobenzene	15.555	180	56894	16.68	ug/l	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022221\
Data File : VD068414.D
Acq On : 22 Feb 2021 12:29
Operator : VA/SY
Sample : M1442-01RE
Misc : 10.17G/5.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Feb 22 15:18:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 12 13:30:51 2021
Response via : Initial Calibration




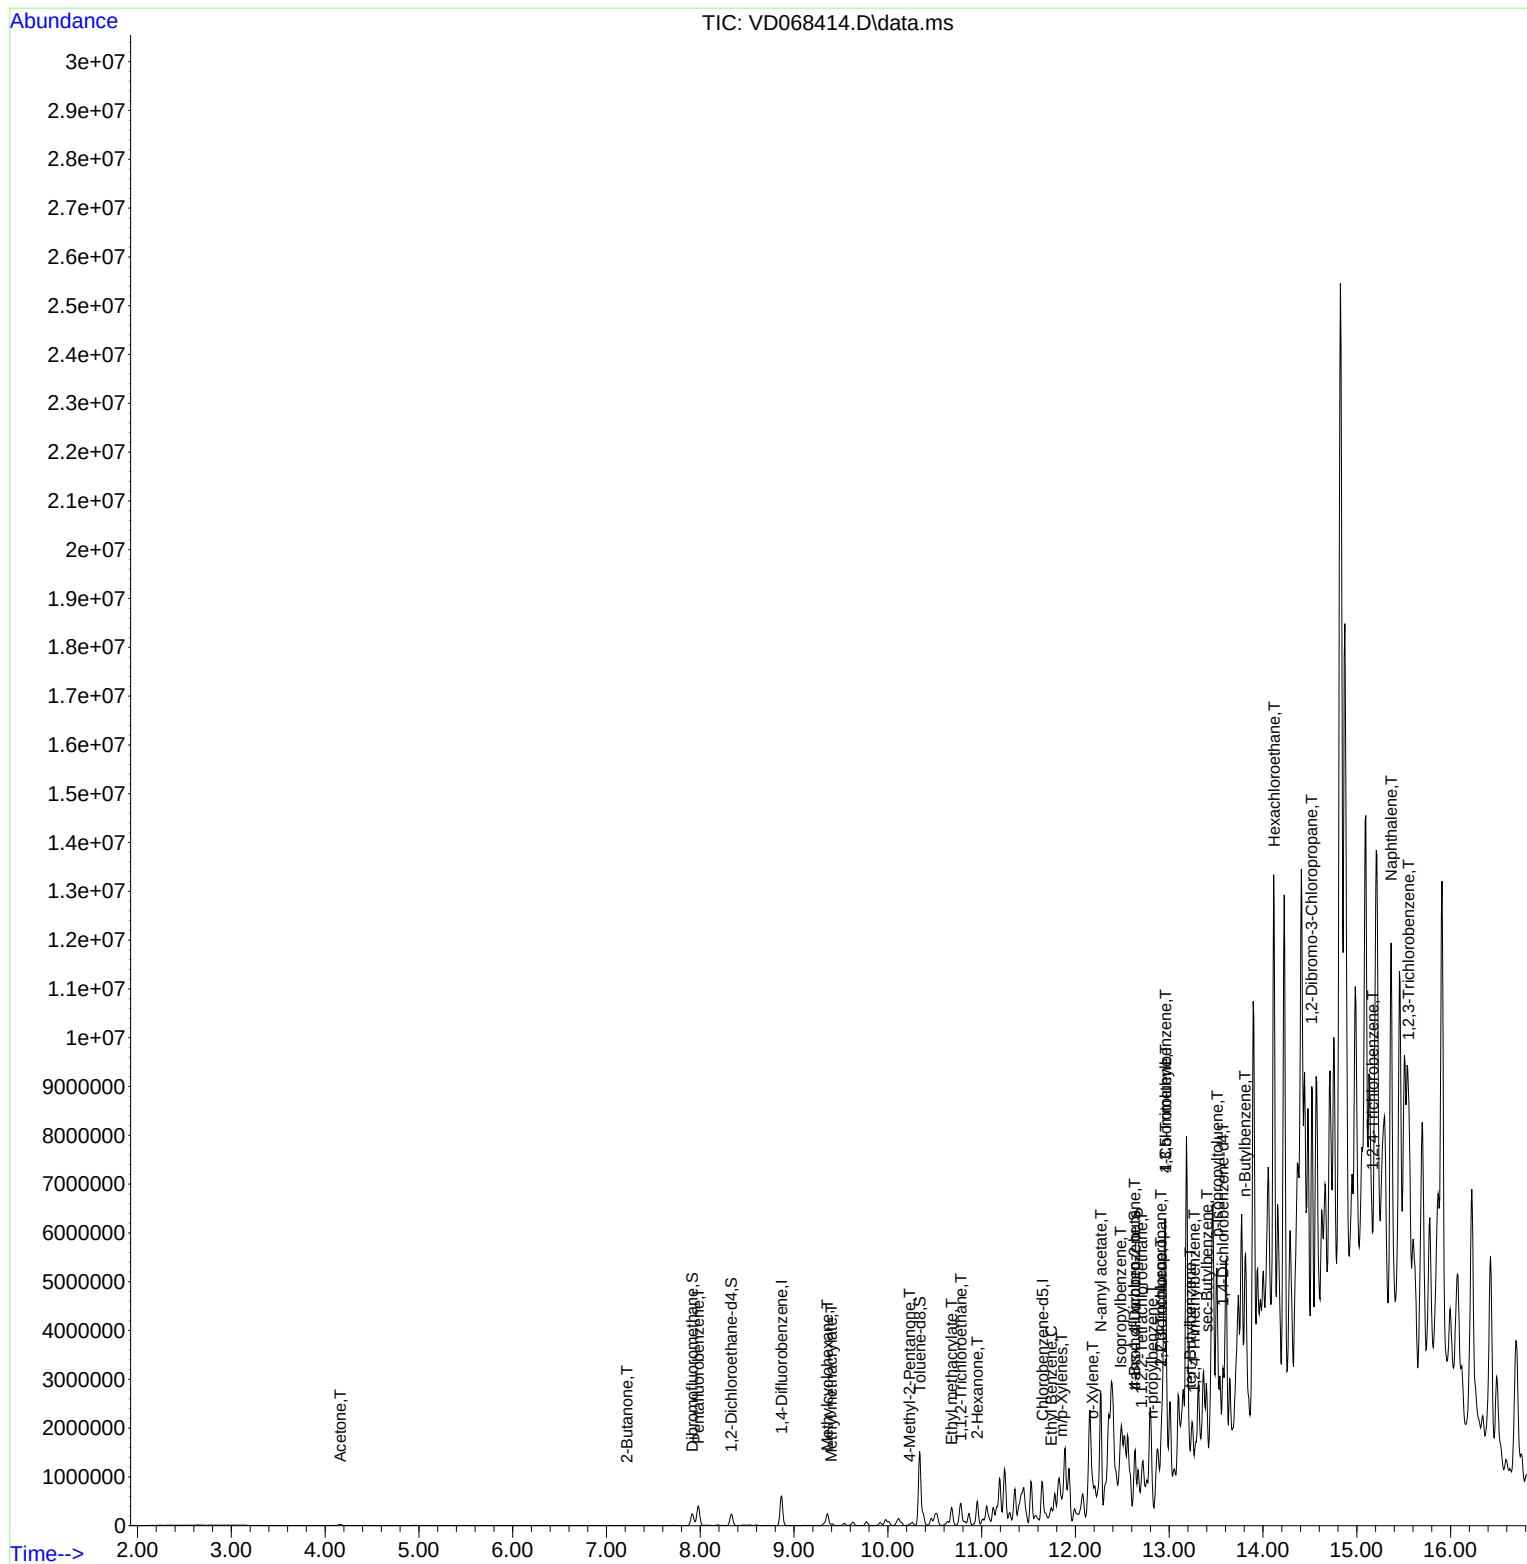


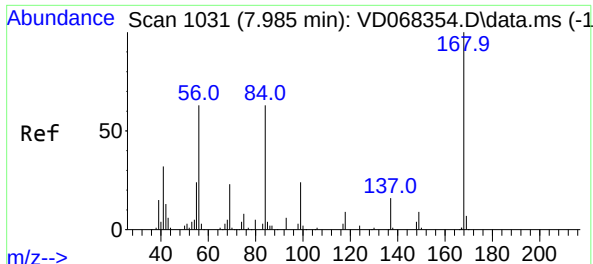

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:168 Resp: 295196
Ion Ratio Lower Upper
168 100
99 55.8 43.5 65.3

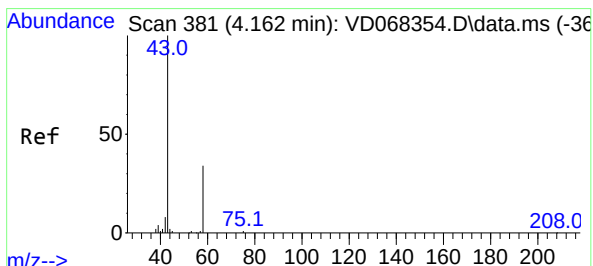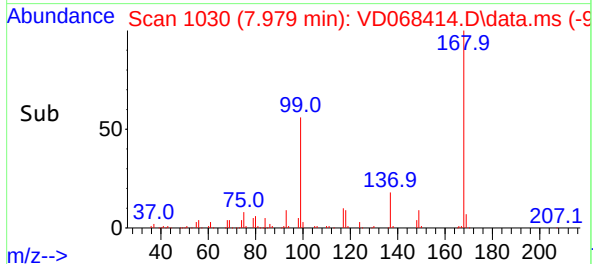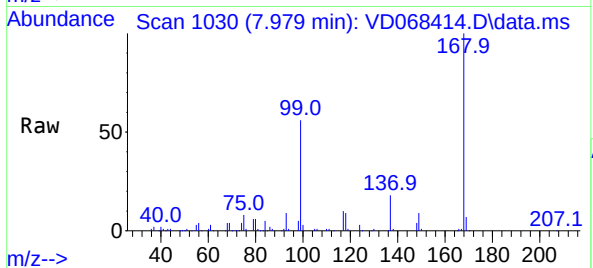

#16
Acetone
Concen: 79.97 ug/l
RT: 4.161 min Scan# 381
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29


Tgt Ion: 43 Resp: 37234
Ion Ratio Lower Upper
43 100
58 29.9 24.2 36.4

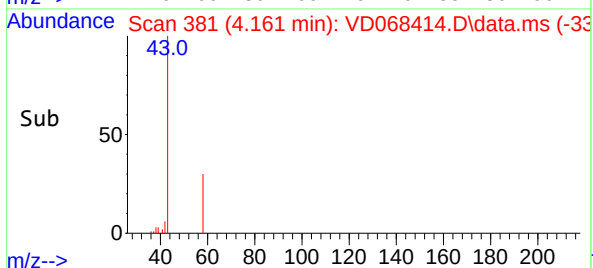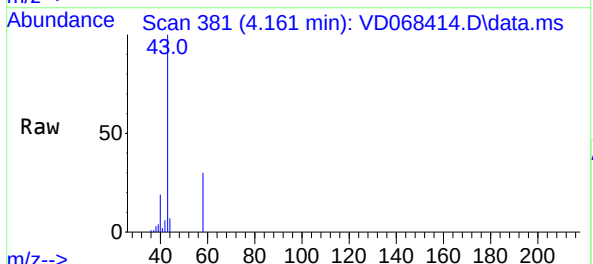






#20
Methylene Chloride
Concen: Below Cal
RT: 4.955 min Scan# 516
Delta R.T. -0.018 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion: 84 Resp: 3898
Ion Ratio Lower Upper
84 100
49 75.0 77.4 116.2#
51 29.6 26.1 39.1
86 58.8 51.8 77.8




#25
2-Butanone
Concen: 3.32 ug/l
RT: 7.220 min Scan# 901
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

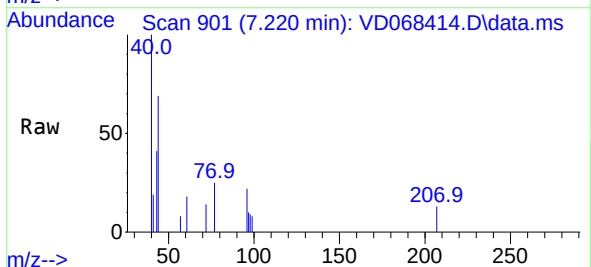

Tgt Ion: 43 Resp: 2161
Ion Ratio Lower Upper
43 100
72 35.0 25.1 37.7







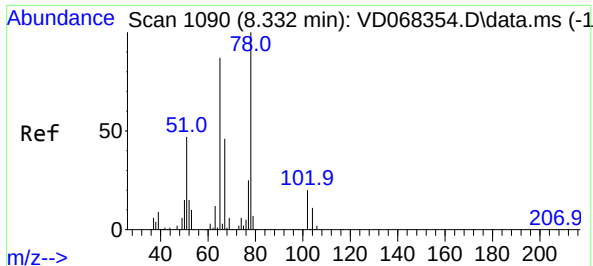

#33
1,2-Dichloroethane-d4
Concen: 60.85 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 65 Resp: 183640
Ion Ratio Lower Upper
65 100
67 55.0 0.0 105.0

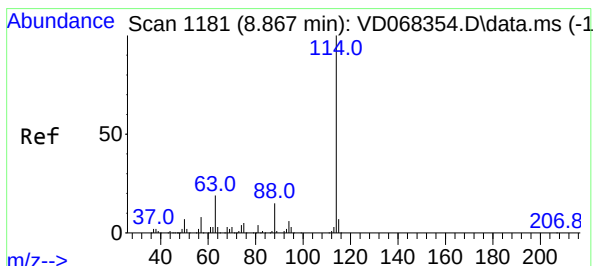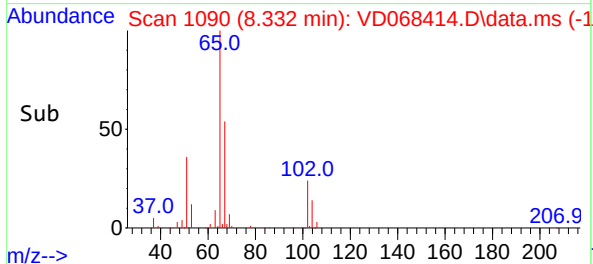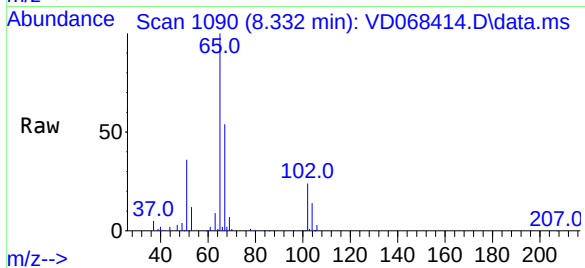

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion:114 Resp: 553341
Ion Ratio Lower Upper
114 100
63 19.7 0.0 34.8
88 15.8 0.0 31.6

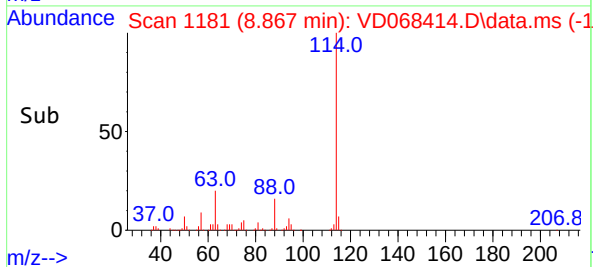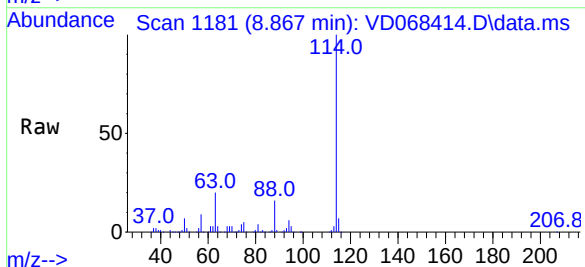

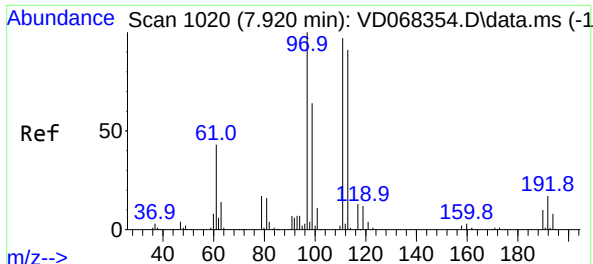

#35

Dibromofluoromethane

Concen: 53.69 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.006 min

Lab File: VD068414.D

Acq: 22 Feb 2021 12:29





Tgt Ion:113 Resp: 176337

Ion Ratio Lower Upper

113 100

111 101.2 81.4 122.0

192 18.8 16.1 24.1

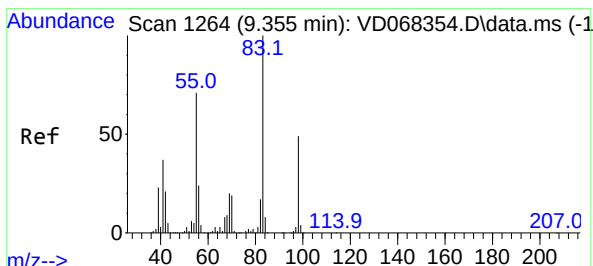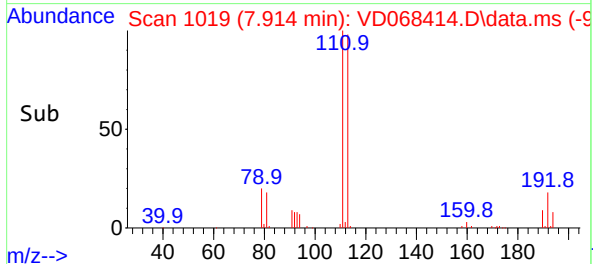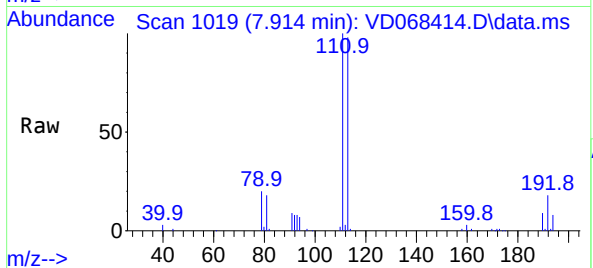

#39

Methylcyclohexane

Concen: 17.10 ug/l

RT: 9.355 min Scan# 1264

Delta R.T. -0.000 min

Lab File: VD068414.D

Acq: 22 Feb 2021 12:29




Tgt Ion: 83 Resp: 102683


Ion Ratio Lower Upper

83 100

55 71.5 55.2 82.8

98 53.3 39.1 58.7

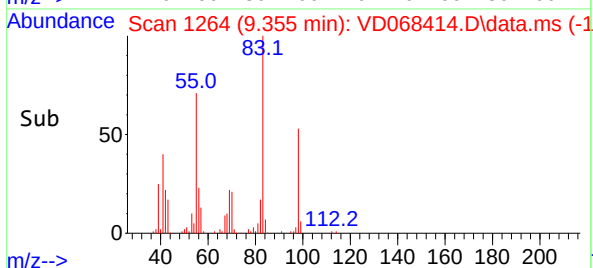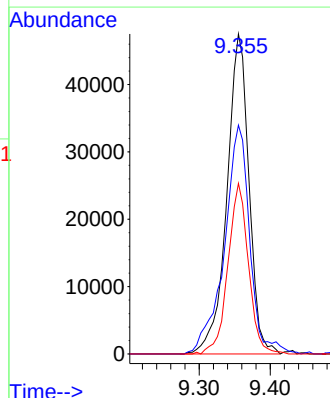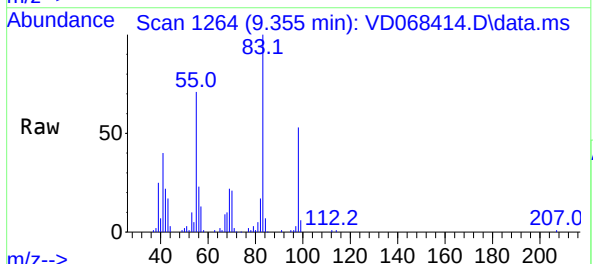

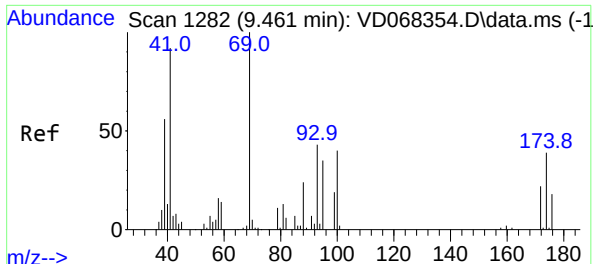

#48

Methyl methacrylate

Concen: 3.78 ug/l

RT: 9.396 min Scan# 1271

Delta R.T. -0.065 min

Lab File: VD068414.D

Acq: 22 Feb 2021 12:29

Tgt Ion: 41 Resp: 5982

Ion Ratio Lower Upper

41 100


69 0.0 77.1 115.7#

39 34.6 41.5 62.3#

Instrument :

MSVOA_D

ClientSampleId :

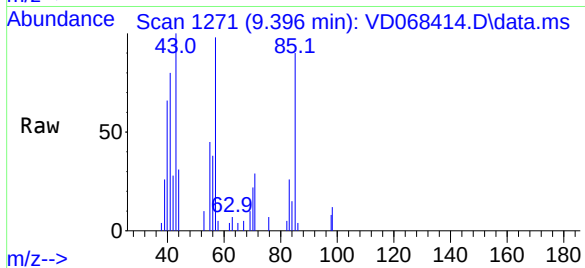

Abundance




15000

10000

5000

0

Time-->

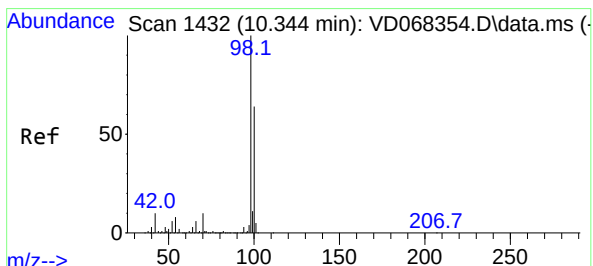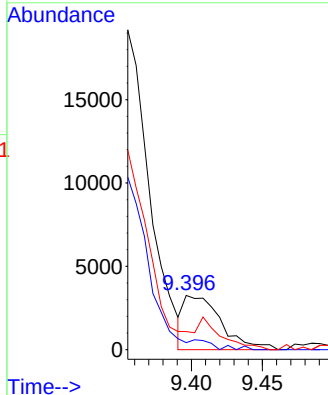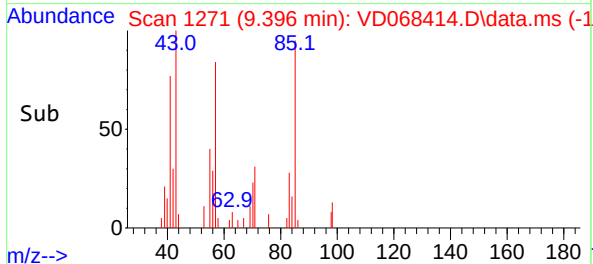

#50

Toluene-d8

Concen: 52.63 ug/l

RT: 10.343 min Scan# 1432

Delta R.T. -0.000 min

Lab File: VD068414.D


Acq: 22 Feb 2021 12:29

Tgt Ion: 98 Resp: 716495

Ion Ratio Lower Upper

98 100

100 61.7 53.0 79.4

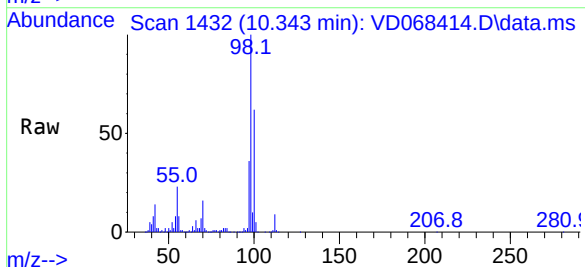

Abundance



300000


200000

100000

0

Time-->



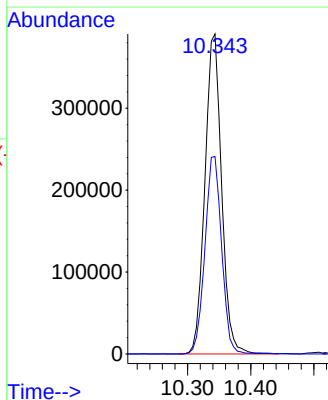
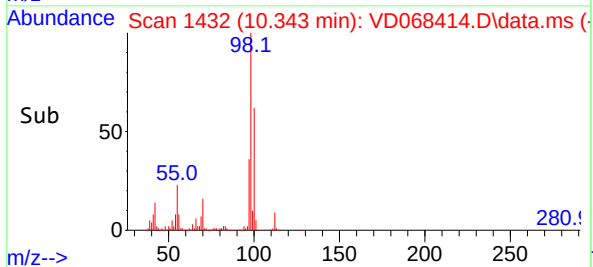




#51
4-Methyl-2-Pentanone
Concen: 1.57 ug/l
RT: 10.232 min Scan# 1413
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 2556
Ion Ratio Lower Upper
43 100
58 33.1 36.1 54.1#

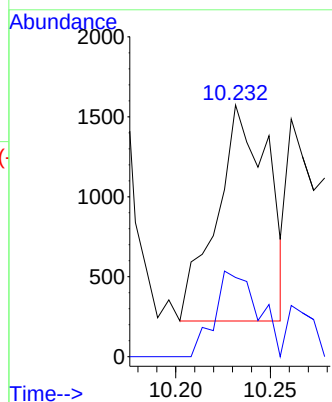

#55
1,1,2-Trichloroethane
Concen: 72.58 ug/l
RT: 10.779 min Scan# 1506
Delta R.T. -0.024 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 97 Resp: 185334
Ion Ratio Lower Upper
97 100
83 8.4 61.8 92.6#
85 2.8 42.2 63.2#
99 0.2 48.3 72.5#


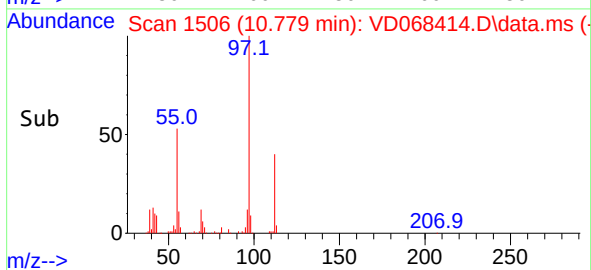

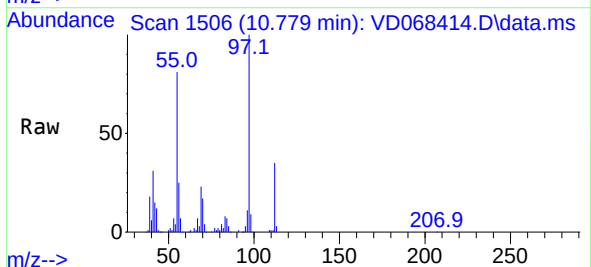


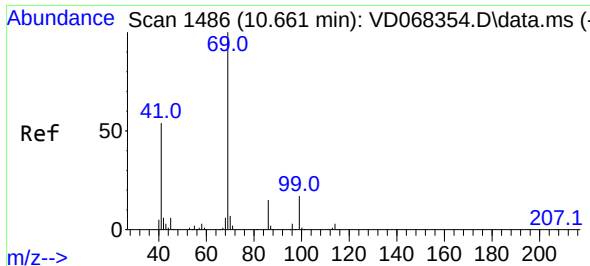

#56
Ethyl methacrylate
Concen: 12.85 ug/l
RT: 10.679 min Scan# 1489
Delta R.T. 0.017 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 69 Resp: 38942
Ion Ratio Lower Upper
69 100
41 125.2 44.9 67.3#
39 79.1 21.9 32.9#

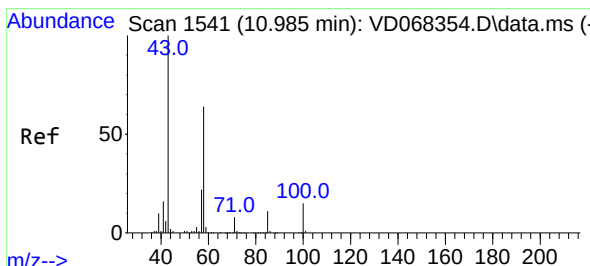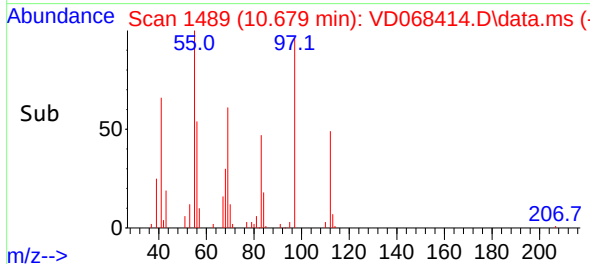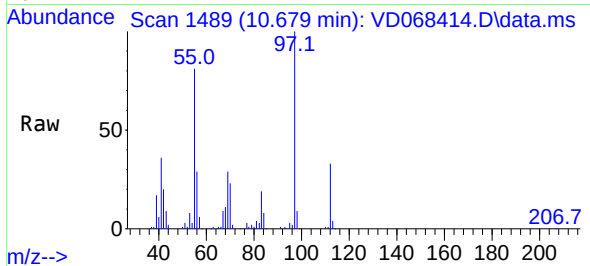

#59
2-Hexanone
Concen: 162.54 ug/l
RT: 10.955 min Scan# 1536
Delta R.T. -0.030 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 43 Resp: 178747
Ion Ratio Lower Upper
43 100
58 4.0 31.0 93.0#


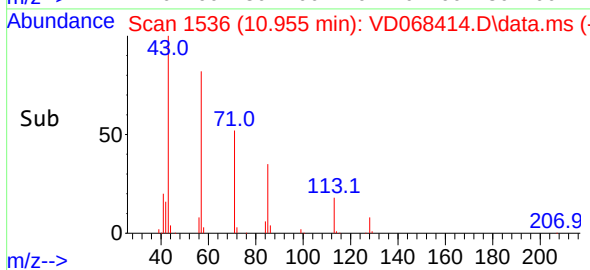

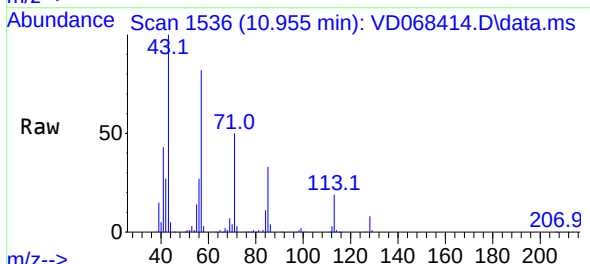




#62
4-Bromofluorobenzene
Concen: 56.26 ug/l
RT: 12.631 min Scan# 1821
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 95 Resp: 249477
Ion Ratio Lower Upper
95 100
174 66.0 0.0 172.4
176 66.5 0.0 168.4

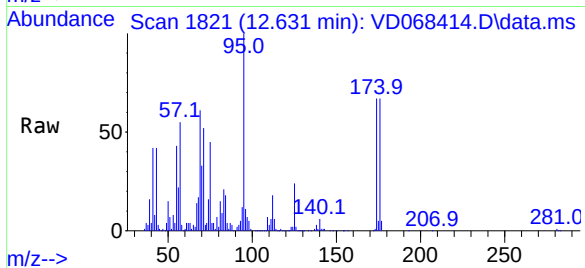

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.649 min Scan# 1654
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion:117 Resp: 496945
Ion Ratio Lower Upper
117 100
82 47.3 41.4 62.0
119 32.2 26.1 39.1


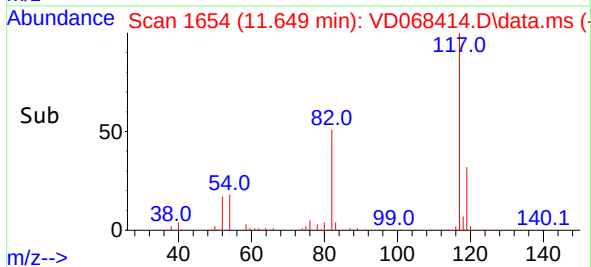

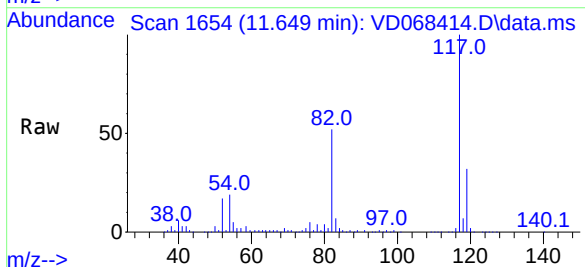




#67
Ethyl Benzene
Concen: 1.91 ug/l
RT: 11.743 min Scan# 1670
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampled :


Tgt Ion: 91 Resp: 32663
Ion Ratio Lower Upper
91 100
106 28.7 25.9 38.9

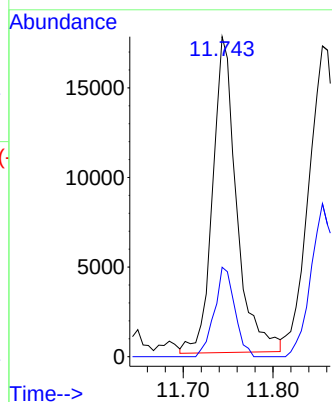

#68
m/p-Xylenes
Concen: 2.49 ug/l
RT: 11.855 min Scan# 1689
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 106 Resp: 16097
Ion Ratio Lower Upper
106 100
91 250.9 159.1 238.7#


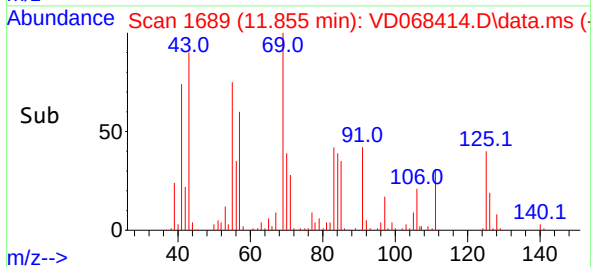
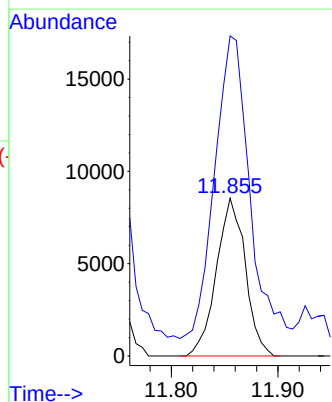
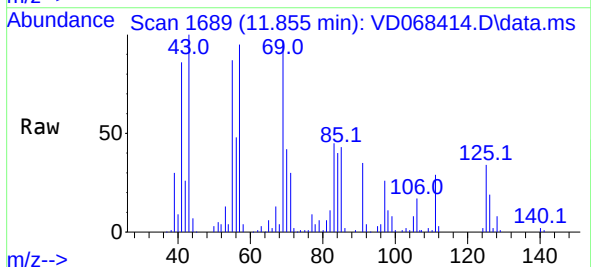




#69
o-Xylene
Concen: 6.26 ug/l
RT: 12.184 min Scan# 1745
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:106 Resp: 37211
Ion Ratio Lower Upper
106 100
91 234.2 108.7 325.9



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion:152 Resp: 218120
Ion Ratio Lower Upper
152 100
115 52.5 28.9 86.8
150 140.3 0.0 344.4


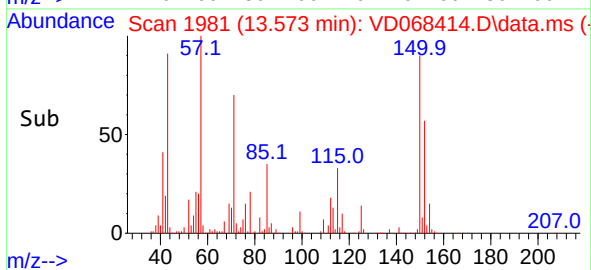






#73
Isopropylbenzene
Concen: 9.65 ug/l
RT: 12.484 min Scan# 1796
Delta R.T. 0.006 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampled :


Tgt Ion:105 Resp: 153738
Ion Ratio Lower Upper
105 100
120 20.9 13.2 39.6

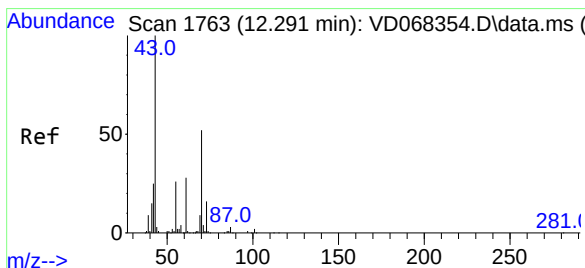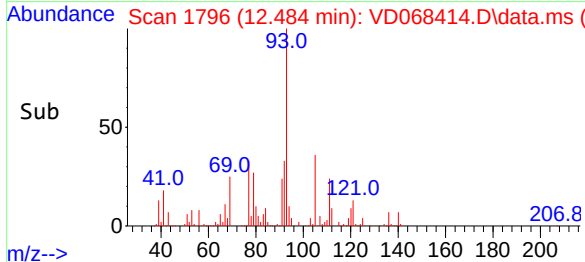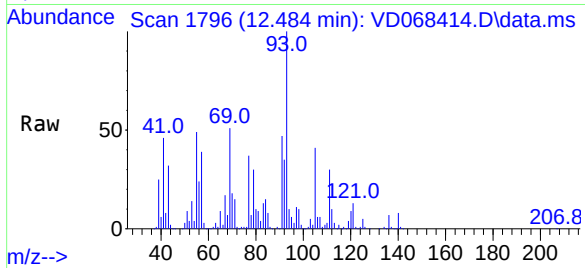

#74
N-ethyl acetate
Concen: 170.62 ug/l
RT: 12.273 min Scan# 1760
Delta R.T. -0.018 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 43 Resp: 480011
Ion Ratio Lower Upper
43 100
70 20.2 41.8 62.8#
55 16.5 24.2 36.4#
61 0.0 21.7 32.5#


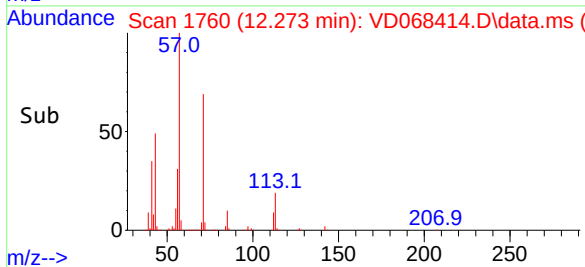
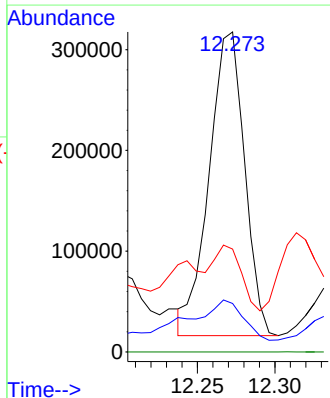
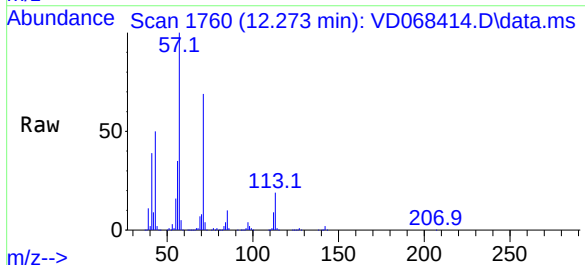




#75
1,1,2,2-Tetrachloroethane
Concen: 13.64 ug/l
RT: 12.708 min Scan# 1834
Delta R.T. -0.024 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 83 Resp: 37649
Ion Ratio Lower Upper
83 100
131 0.0 5.8 17.4#
85 117.4 32.4 97.2#



#76
1,2,3-Trichloropropane
Concen: 3.11 ug/l
RT: 12.914 min Scan# 1869
Delta R.T. 0.129 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 75 Resp: 6454
Ion Ratio Lower Upper
75 100
77 1637.3 0.0 0.0#



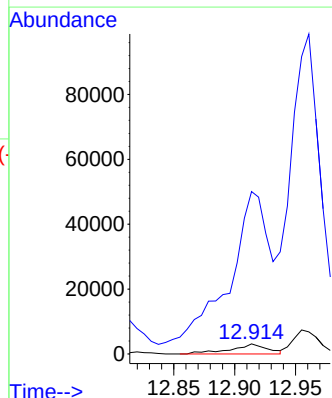





#78
n-propylbenzene
Concen: 6.26 ug/l
RT: 12.820 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampled :


Tgt Ion: 91 Resp: 119404
Ion Ratio Lower Upper
91 100
120 21.0 12.0 36.0



#79
2-Chlorotoluene
Concen: 8.33 ug/l
RT: 12.914 min Scan# 1869
Delta R.T. 0.006 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29


Tgt Ion: 91 Resp: 87999
Ion Ratio Lower Upper
91 100
126 1.5 17.8 53.5#








#80
1,3,5-Trimethylbenzene
Concen: 70.99 ug/l
RT: 12.961 min Scan# 1877
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion:105 Resp: 924191
Ion Ratio Lower Upper
105 100
120 51.2 24.2 72.6




#81
trans-1,4-Dichloro-2-butene
Concen: 129.19 ug/l
RT: 12.631 min Scan# 1821
Delta R.T. 0.106 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

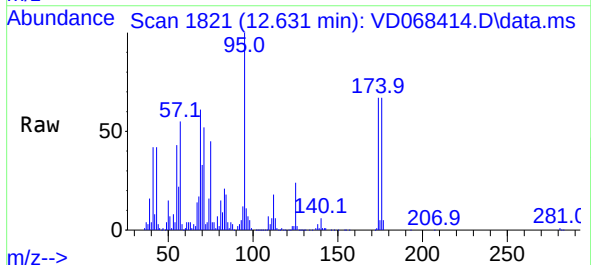

Tgt Ion: 75 Resp: 106975
Ion Ratio Lower Upper
75 100
53 13.0 70.2 105.2#
89 0.2 40.3 60.5#



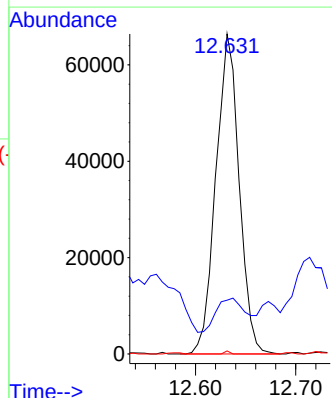
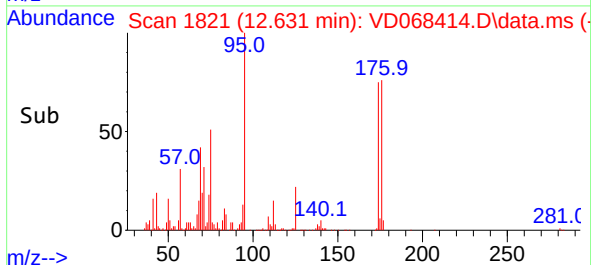




#82
4-Chlorotoluene
Concen: 10.45 ug/l
RT: 12.961 min Scan# 1877
Delta R.T. -0.041 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 91 Resp: 116702
Ion Ratio Lower Upper
91 100
126 8.9 17.7 53.1#

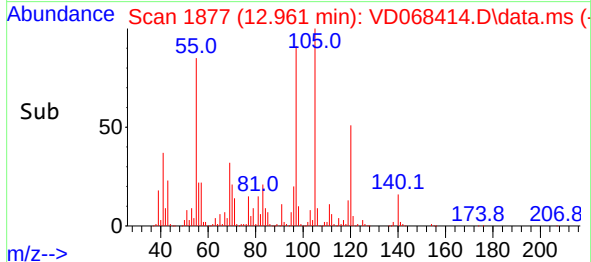

#83
tert-Butylbenzene
Concen: 2.54 ug/l
RT: 13.226 min Scan# 1922
Delta R.T. 0.006 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 119 Resp: 28632
Ion Ratio Lower Upper
119 100
91 93.0 31.1 93.5
134 23.3 13.3 39.8


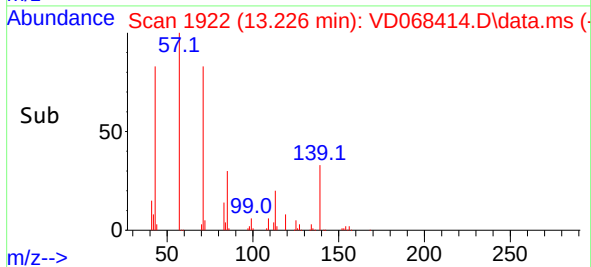

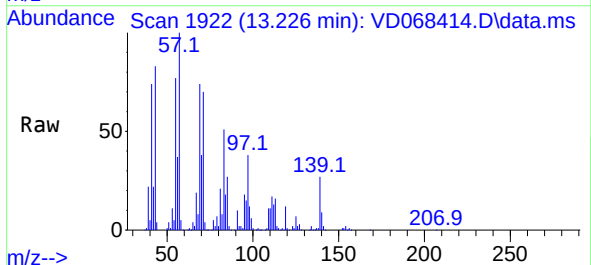




#84
1,2,4-Trimethylbenzene
Concen: 4.68 ug/l
RT: 13.267 min Scan# 1929
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:105 Resp: 60680
Ion Ratio Lower Upper
105 100
120 42.2 22.4 67.0

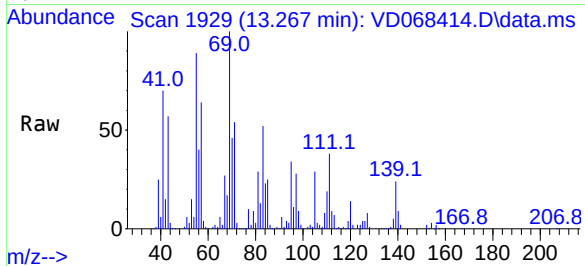

#85
sec-Butylbenzene
Concen: 30.37 ug/l
RT: 13.402 min Scan# 1952
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion:105 Resp: 479720
Ion Ratio Lower Upper
105 100
134 23.7 10.3 30.9


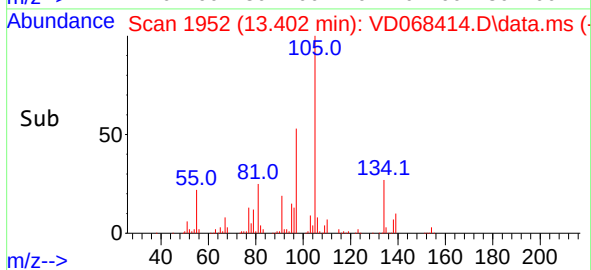

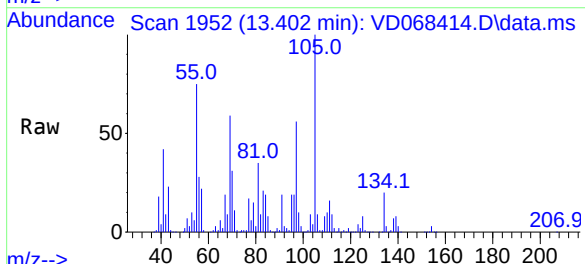




#86
p-Isopropyltoluene
Concen: 28.81 ug/l
RT: 13.514 min Scan# 1971
Delta R.T. -0.000 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:119 Resp: 408592
Ion Ratio Lower Upper
119 100
134 26.3 12.9 38.7
91 23.4 11.7 35.0

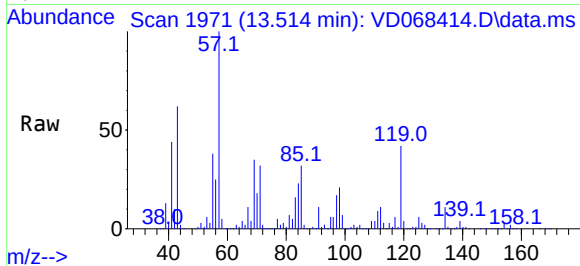

#89
n-Butylbenzene
Concen: 44.06 ug/l
RT: 13.808 min Scan# 2021
Delta R.T. -0.036 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 91 Resp: 609681
Ion Ratio Lower Upper
91 100
92 0.0 27.2 81.6#
134 144.9 13.9 41.7#


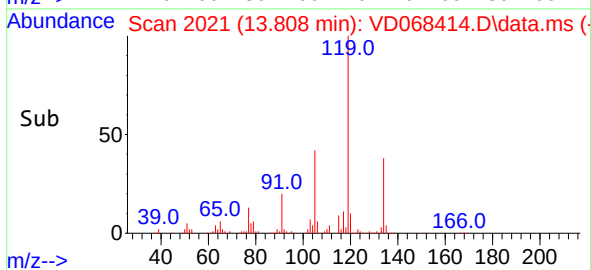

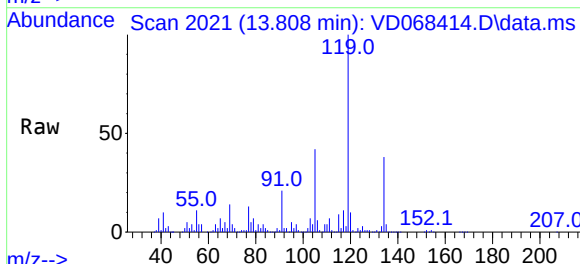




#90
Hexachloroethane
Concen: 162.79 ug/l
RT: 14.120 min Scan# 2074
Delta R.T. 0.011 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:117 Resp: 419131
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

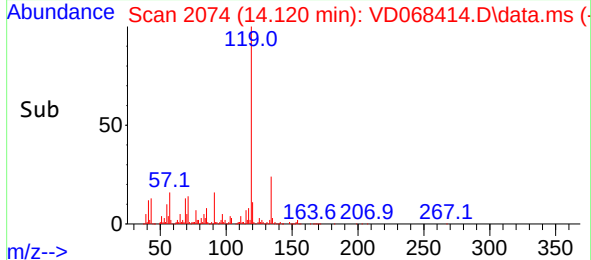

#92
1,2-Dibromo-3-Chloropropane
Concen: 33.57 ug/l
RT: 14.520 min Scan# 2142
Delta R.T. 0.017 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion: 75 Resp: 13554
Ion Ratio Lower Upper
75 100
155 28.5 48.0 144.2#
157 0.0 65.0 194.8#


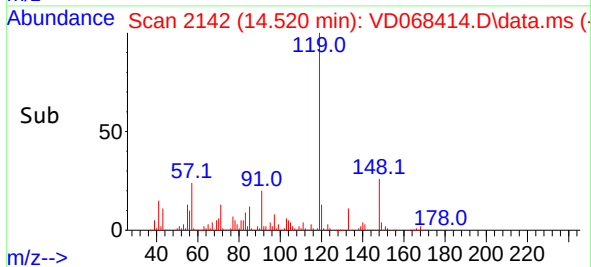

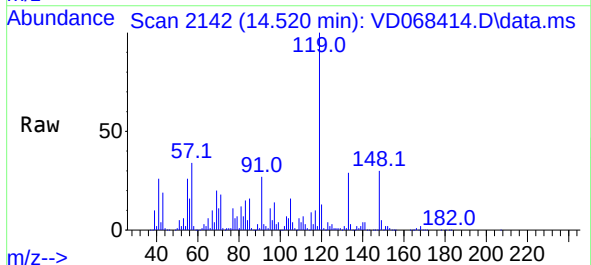




#93
1,2,4-Trichlorobenzene
Concen: 2.70 ug/l
RT: 15.167 min Scan# 2252
Delta R.T. 0.006 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29




Instrument :
MSVOA_D
ClientSampled :


Tgt Ion:180 Resp: 10542
Ion Ratio Lower Upper
180 100
182 282.7 46.8 140.4#
145 6748.1 15.2 45.5#

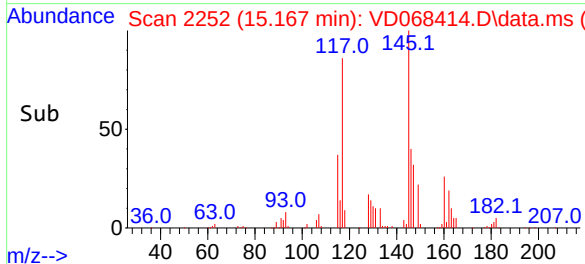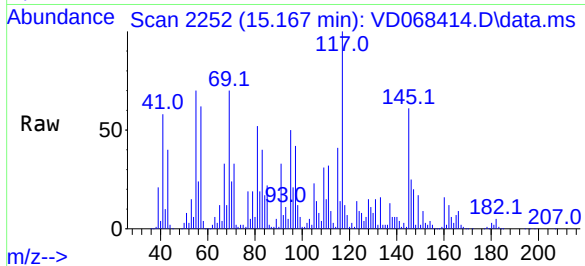

#95
Naphthalene
Concen: 11.11 ug/l
RT: 15.367 min Scan# 2286
Delta R.T. -0.030 min
Lab File: VD068414.D
Acq: 22 Feb 2021 12:29

Tgt Ion:128 Resp: 80786
Ion Ratio Lower Upper
128 100
127 94.7 10.2 15.2#
129 107.1 8.8 13.2#

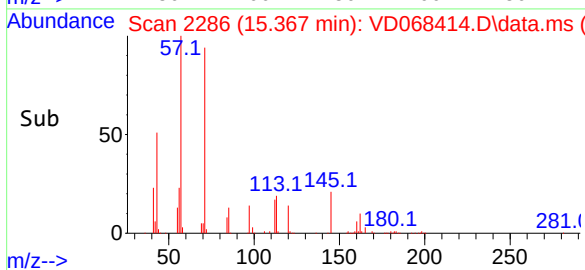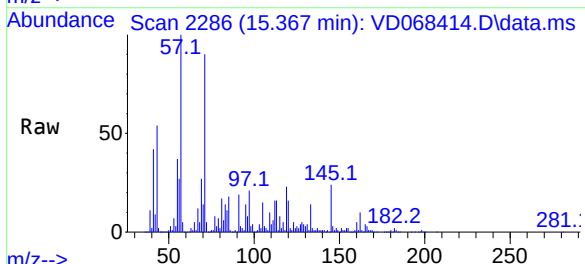



#96
 1,2,3-Trichlorobenzene
 Concen: 16.68 ug/l
 RT: 15.555 min Scan# 2318
 Delta R.T. -0.036 min
 Lab File: VD068414.D
 Acq: 22 Feb 2021 12:29

Instrument :
 MSVOA_D
 ClientSampleId :

Tgt Ion:180 Resp: 56894
 Ion Ratio Lower Upper
 180 100
 182 12.0 48.3 144.8#
 145 698.1 16.7 50.1#

