
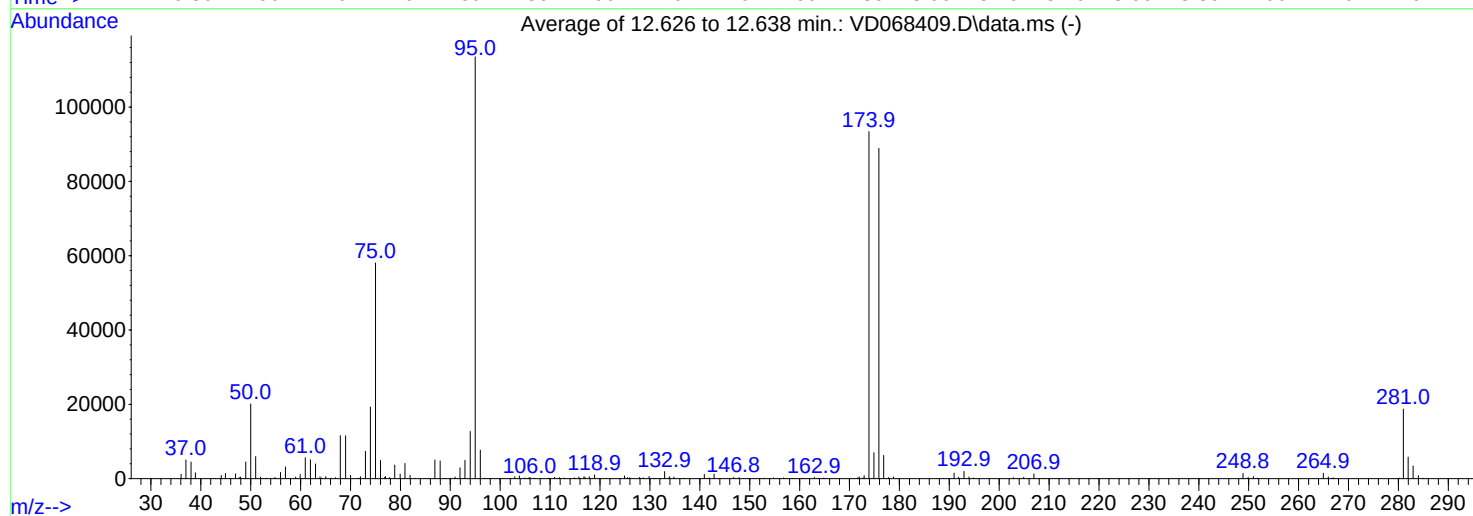


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022221\
 Data File : VD068409.D
 Acq On : 22 Feb 2021 09:21
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
 Title : SW846 8260
 Last Update : Fri Feb 12 13:30:51 2021

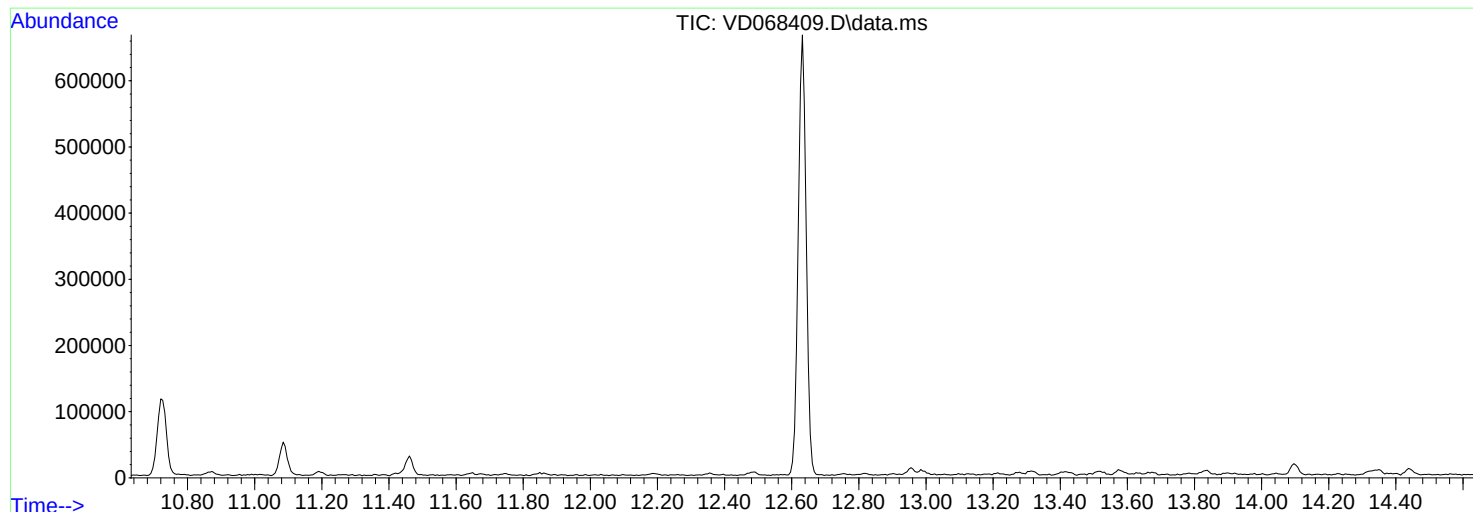

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	20096	PASS
75	95	30	60	51.1	58040	PASS
95	95	100	100	100.0	113515	PASS
96	95	5	9	6.8	7667	PASS
173	174	0.00	2	0.9	802	PASS
174	95	50	100	82.3	93397	PASS
175	174	5	9	7.5	6969	PASS
176	174	95	101	95.2	88896	PASS
177	176	5	9	7.0	6225	PASS