
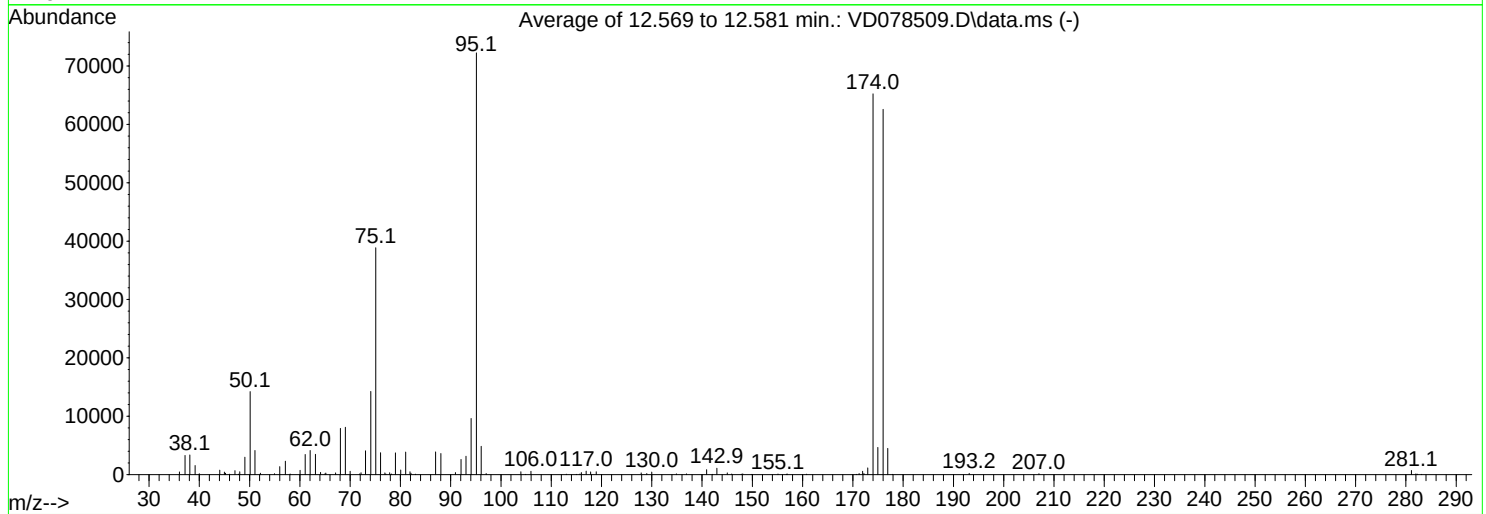


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022224\
Data File : VD078509.D
Acq On : 22 Feb 2024 08:43
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021324S.M
Title : SW846 8260
Last Update : Wed Feb 14 01:16:20 2024

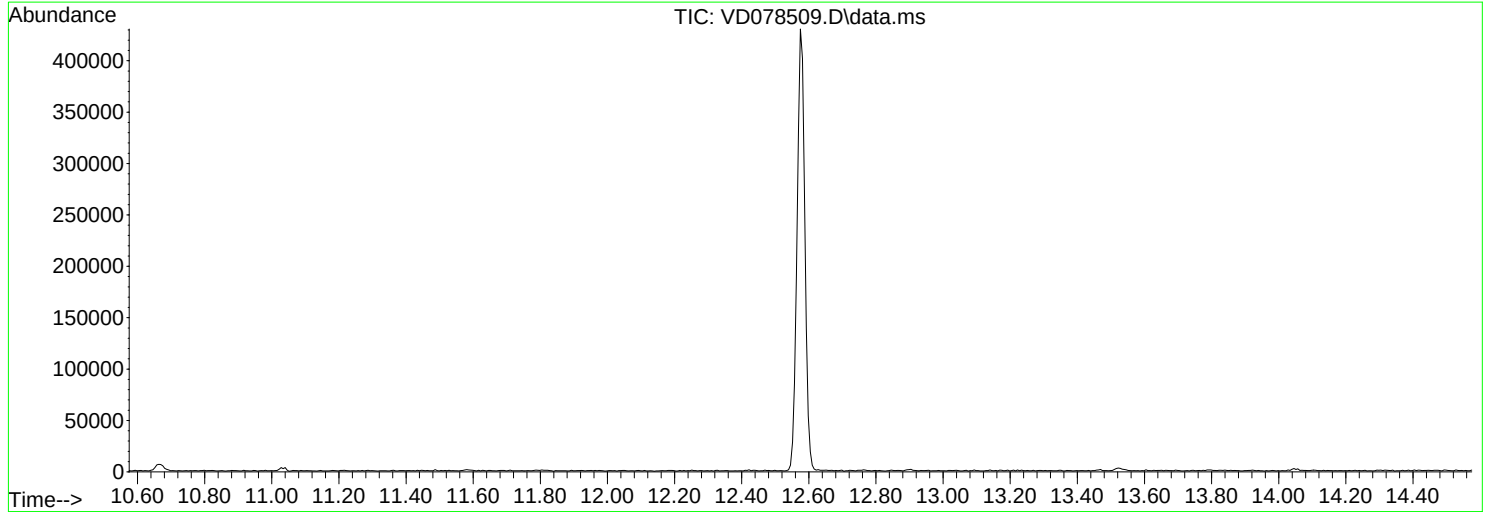

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	14224	PASS
75	95	30	60	53.8	38875	PASS
95	95	100	100	100.0	72253	PASS
96	95	5	9	6.7	4842	PASS
173	174	0.00	2	1.8	1144	PASS
174	95	50	100	90.3	65232	PASS
175	174	5	9	7.1	4656	PASS
176	174	95	101	95.9	62587	PASS
177	176	5	9	7.2	4495	PASS