
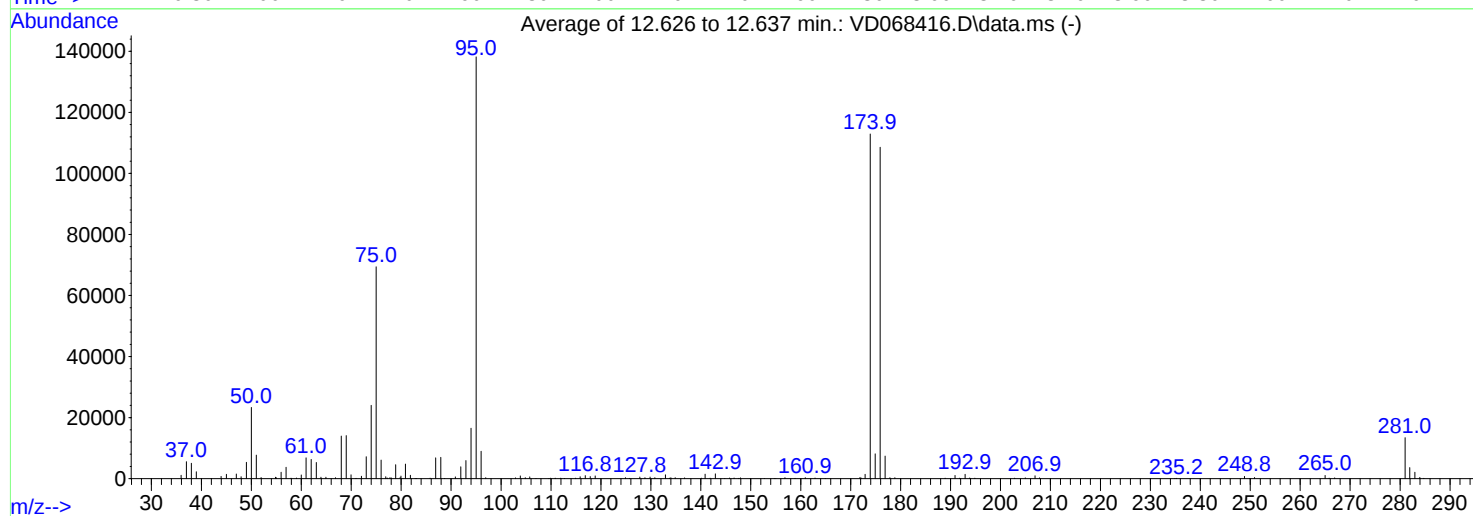


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022321\
 Data File : VD068416.D
 Acq On : 23 Feb 2021 09:39
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
 Title : SW846 8260
 Last Update : Fri Feb 12 13:30:51 2021

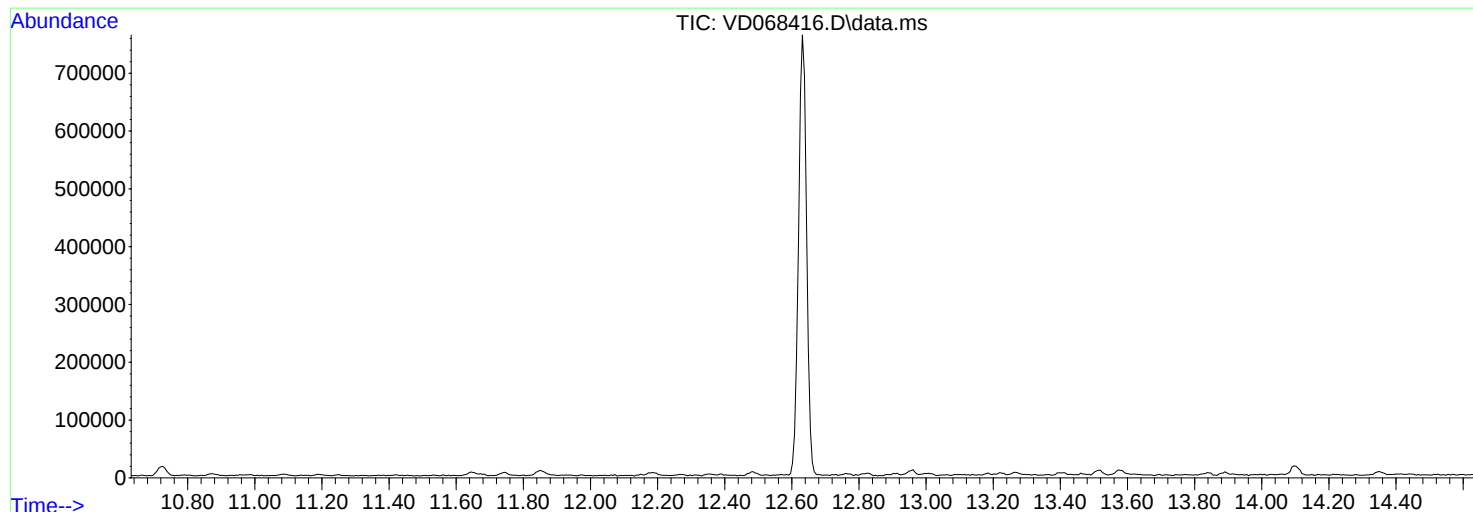

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	23320	PASS
75	95	30	60	50.2	69411	PASS
95	95	100	100	100.0	138195	PASS
96	95	5	9	6.5	8974	PASS
173	174	0.00	2	1.3	1436	PASS
174	95	50	100	81.7	112923	PASS
175	174	5	9	7.2	8139	PASS
176	174	95	101	96.1	108571	PASS
177	176	5	9	6.8	7394	PASS