

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022421\
 Data File : VD068436.D
 Acq On : 24 Feb 2021 15:10
 Operator : VA/SY
 Sample : M1469-01
 Misc : 7.33G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TR-08-022321

Quant Time: Feb 25 00:11:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 12 13:30:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	366157	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	694007	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	624214	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	237774	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.338	65	200141	53.47	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	106.94%
35) Dibromofluoromethane	7.920	113	208383	50.59	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.18%
50) Toluene-d8	10.344	98	863425	50.57	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.14%
62) 4-Bromofluorobenzene	12.632	95	254952	45.84	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	91.68%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022421\
Data File : VD068436.D
Acq On : 24 Feb 2021 15:10
Operator : VA/SY
Sample : M1469-01
Misc : 7.33G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TR-08-022321

Quant Time: Feb 25 00:11:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 12 13:30:51 2021
Response via : Initial Calibration




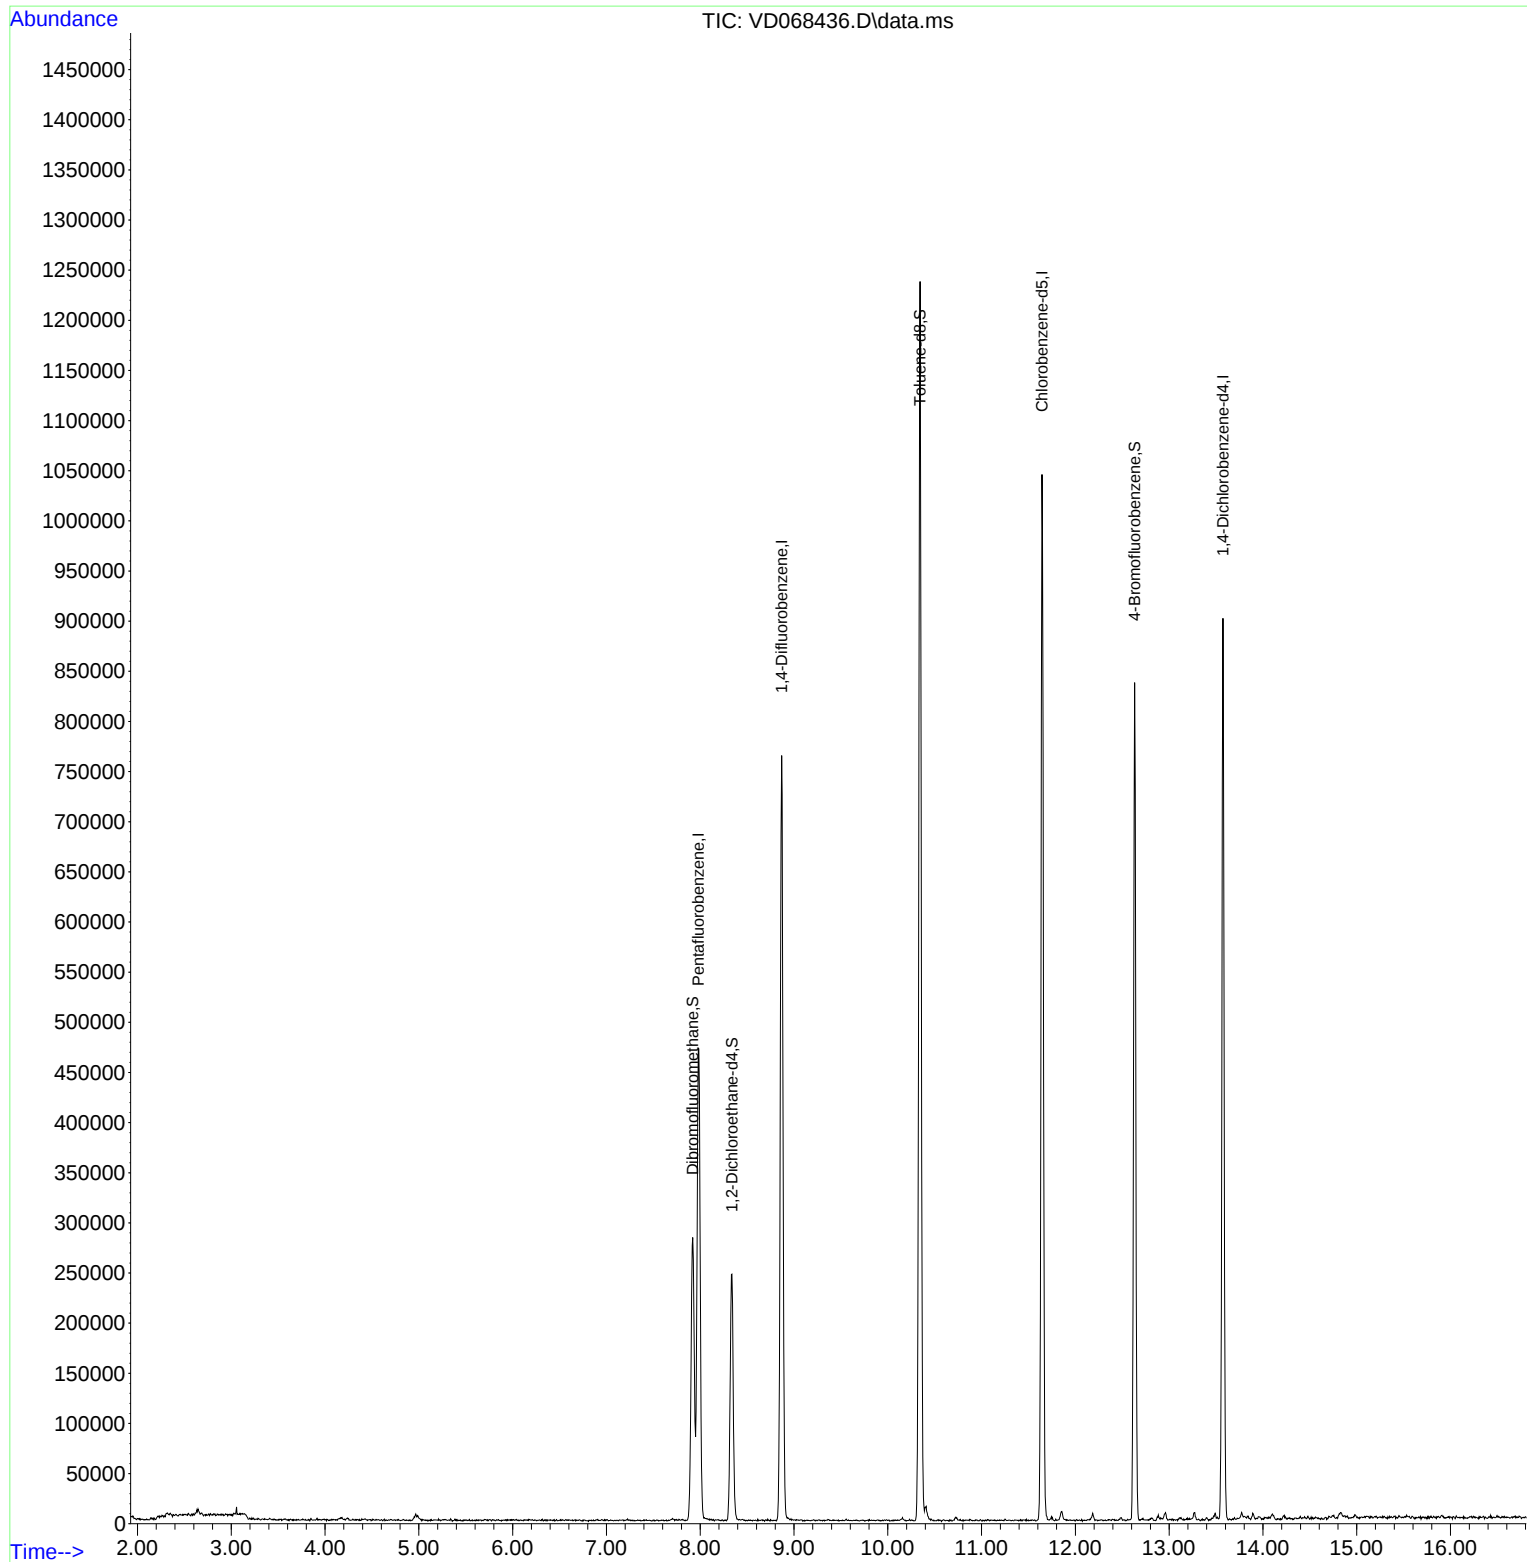


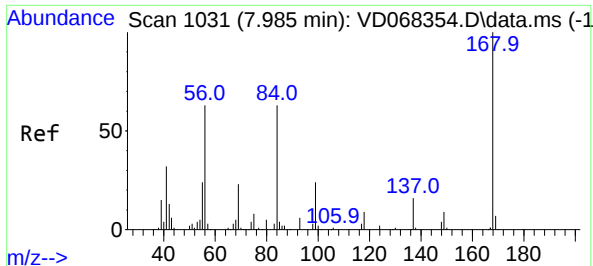

Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10




Instrument :
MSVOA_D
ClientSampleId :
TR-08-022321


Tgt Ion:168 Resp: 366157
Ion Ratio Lower Upper
168 100
99 59.4 43.5 65.3

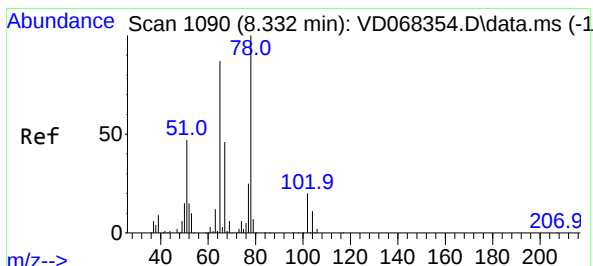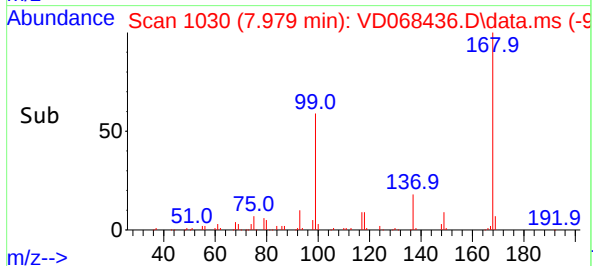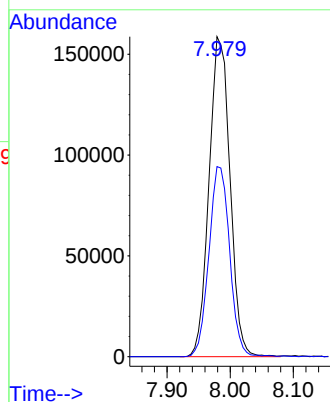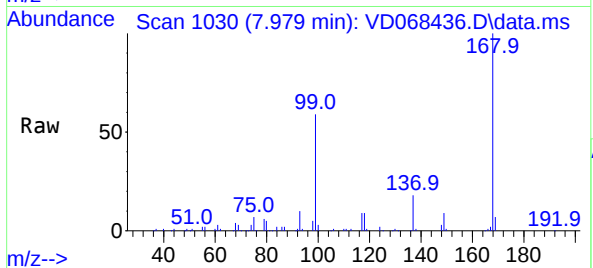

1,2-Dichloroethane-d4
Concen: 53.47 ug/l
RT: 8.338 min Scan# 1091
Delta R.T. 0.006 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10

Tgt Ion: 65 Resp: 200141
Ion Ratio Lower Upper
65 100
67 52.0 0.0 105.0

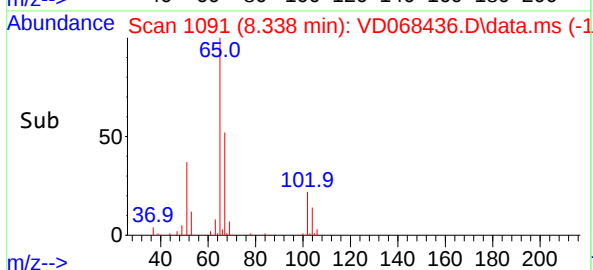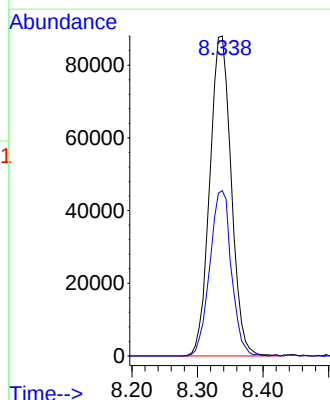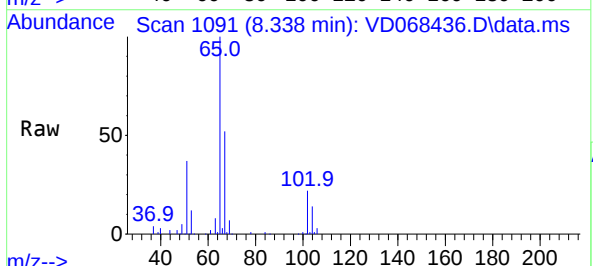

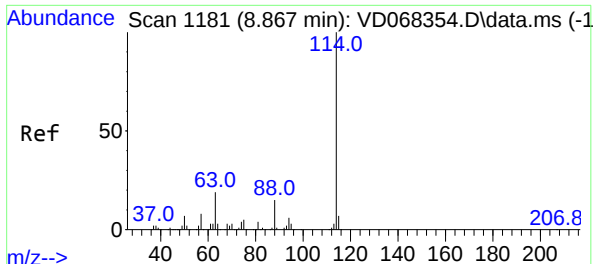





#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10

Instrument :
MSVOA_D
ClientSampleId :
TR-08-022321

Tgt Ion:114 Resp: 694007

Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	34.8
88	15.7	0.0	31.6

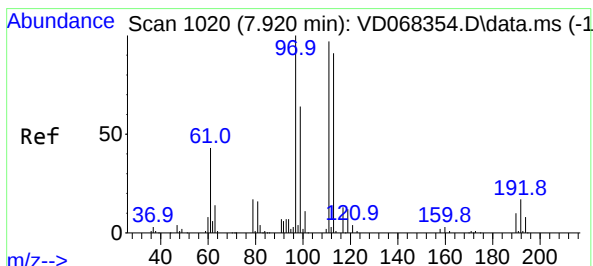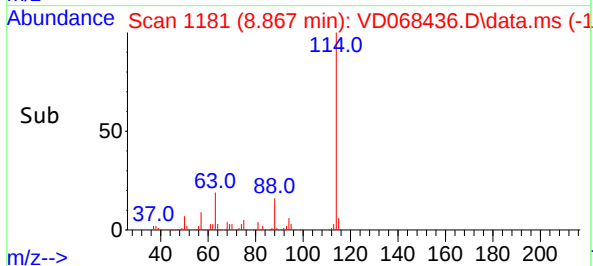
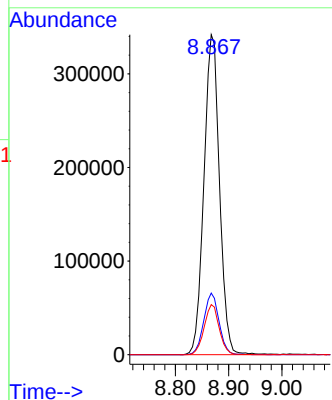
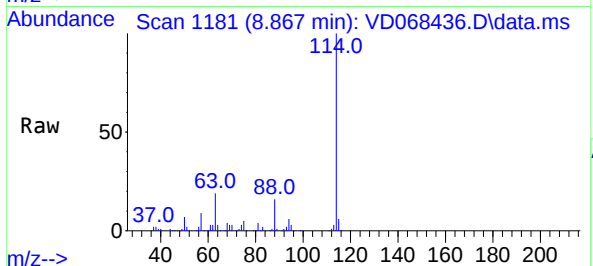



#35

Dibromofluoromethane
Concen: 50.59 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. -0.000 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10

Tgt Ion:113 Resp: 208383

Ion	Ratio	Lower	Upper
113	100		
111	105.3	81.4	122.0
192	18.2	16.1	24.1


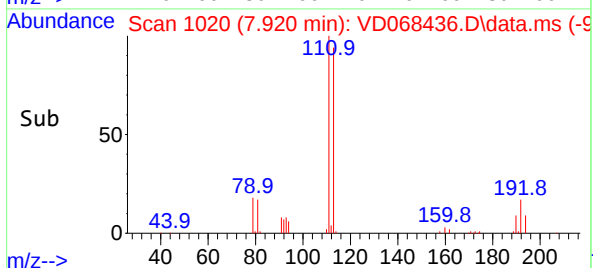
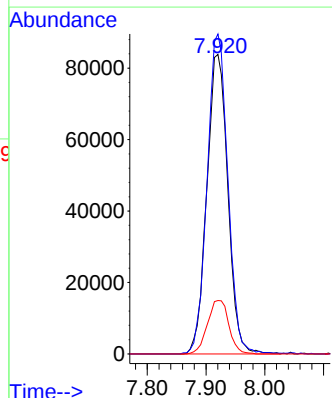
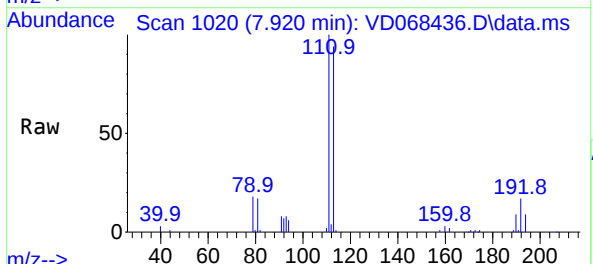


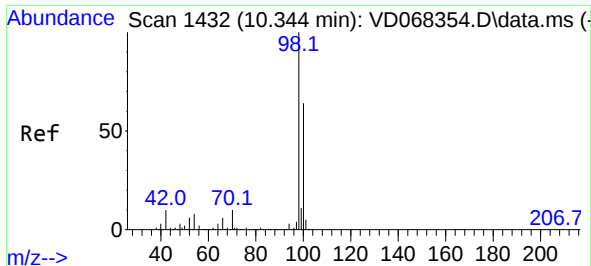

#50
Toluene-d8
Concen: 50.57 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. -0.000 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10




Instrument :
MSVOA_D
ClientSampleId :
TR-08-022321


Tgt Ion: 98 Resp: 863425
Ion Ratio Lower Upper
98 100
100 64.6 53.0 79.4

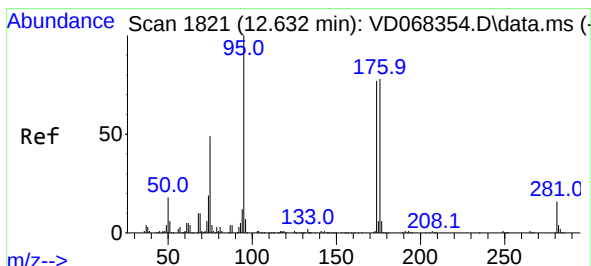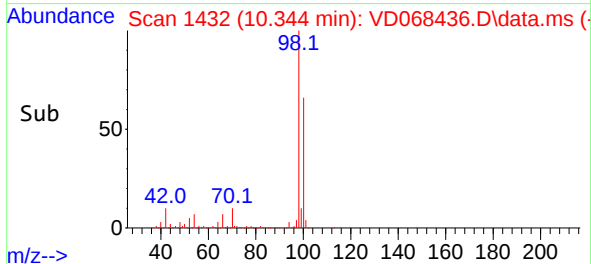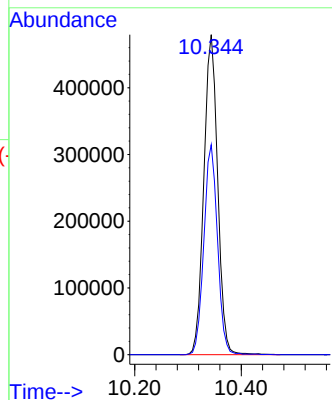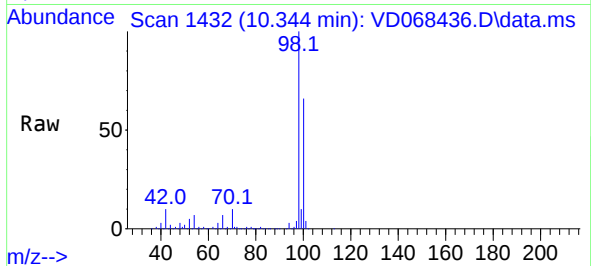

#62
4-Bromofluorobenzene
Concen: 45.84 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.000 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10

Tgt Ion: 95 Resp: 254952
Ion Ratio Lower Upper
95 100
174 79.9 0.0 172.4
176 77.6 0.0 168.4


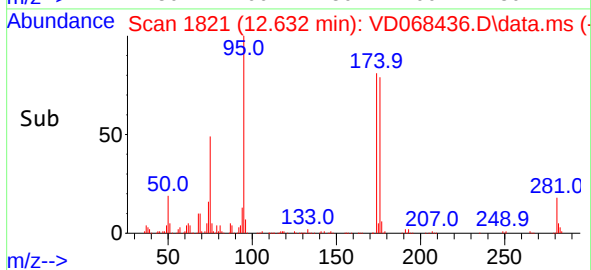
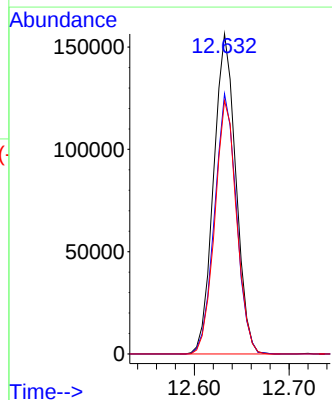
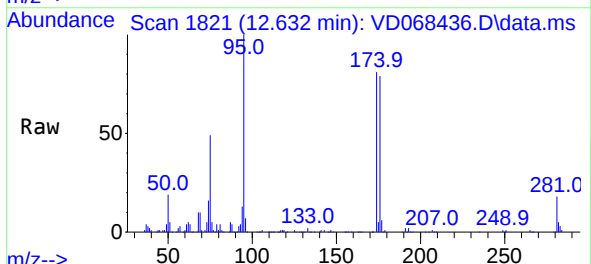


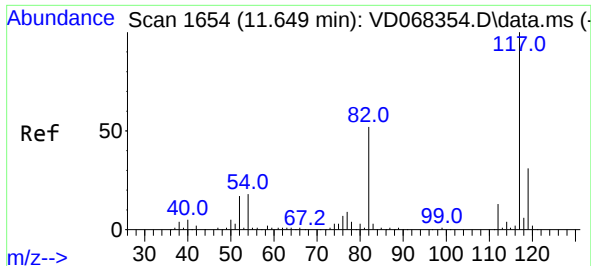

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. -0.006 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10

Instrument :
MSVOA_D
ClientSampleId :
TR-08-022321

Tgt Ion:117 Resp: 624214
Ion Ratio Lower Upper
117 100
82 54.3 41.4 62.0
119 31.2 26.1 39.1

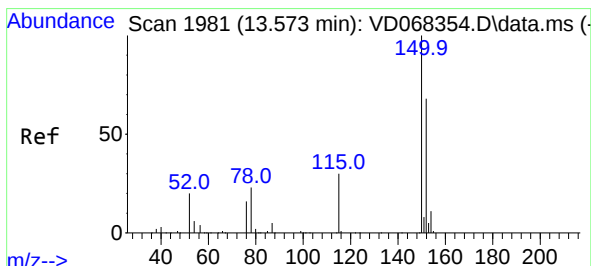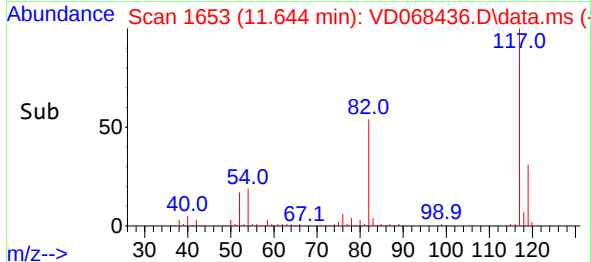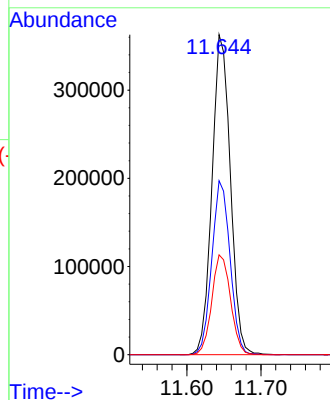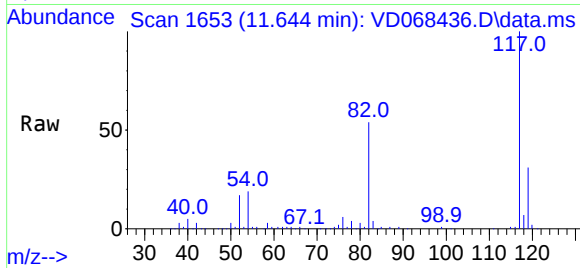

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.000 min
Lab File: VD068436.D
Acq: 24 Feb 2021 15:10

Tgt Ion:152 Resp: 237774
Ion Ratio Lower Upper
152 100
115 59.0 28.9 86.8
150 156.6 0.0 344.4

