
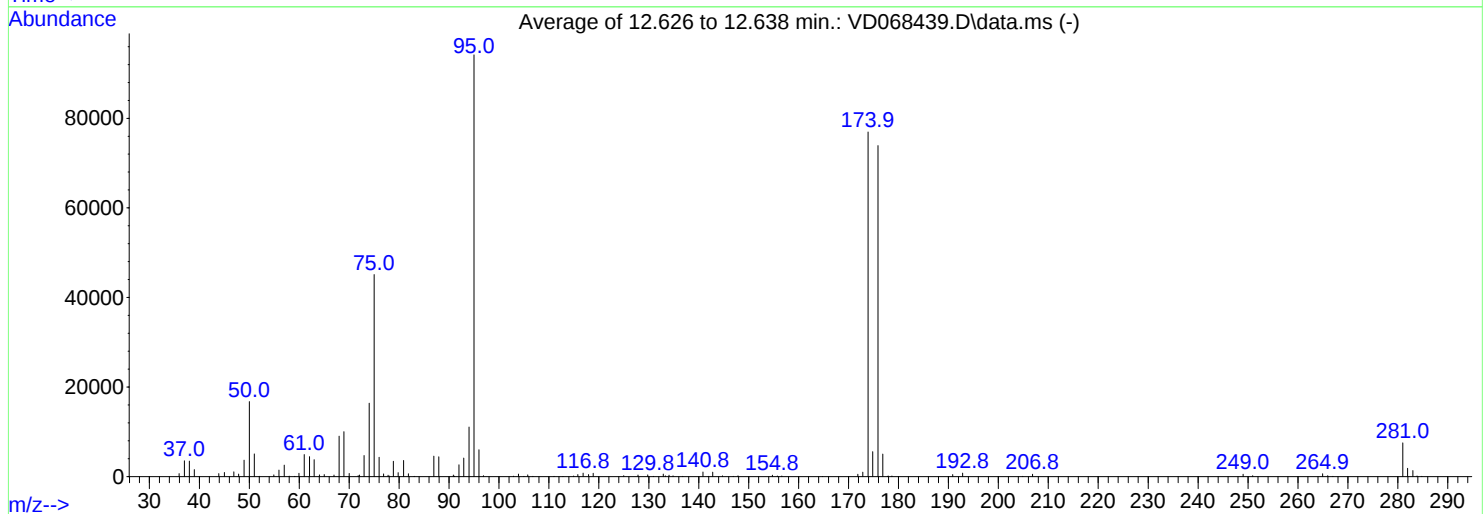


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022521\
Data File : VD068439.D
Acq On : 25 Feb 2021 09:33
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021221S.M
Title : SW846 8260
Last Update : Fri Feb 12 13:30:51 2021

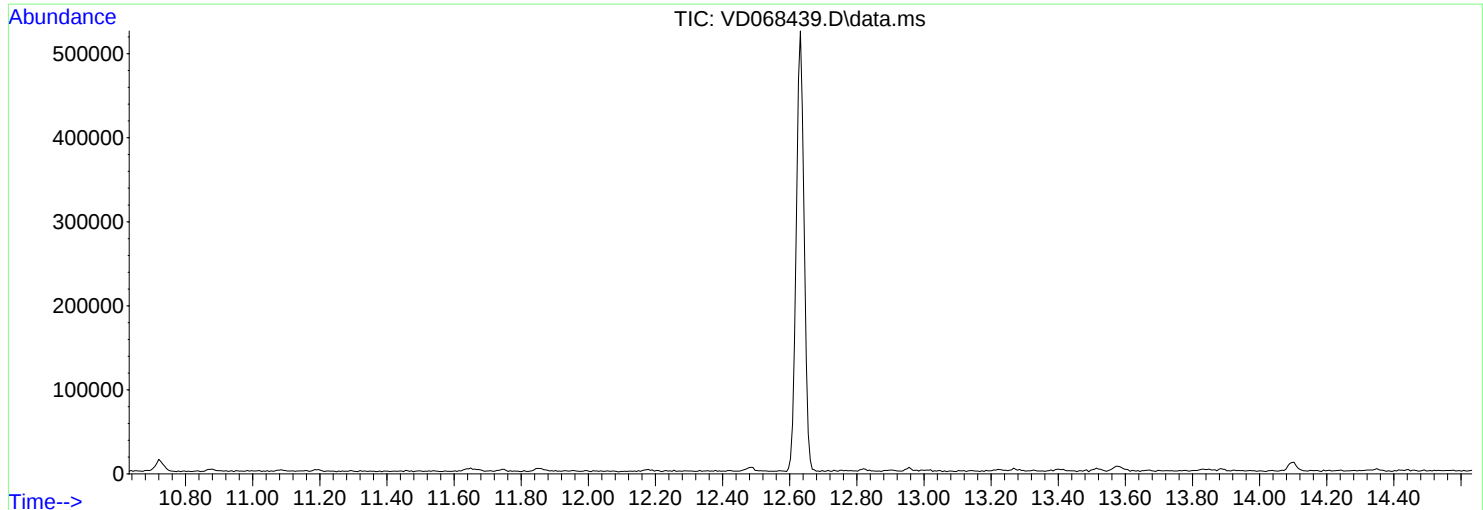

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	16752	PASS
75	95	30	60	47.9	45112	PASS
95	95	100	100	100.0	94171	PASS
96	95	5	9	6.4	6001	PASS
173	174	0.00	2	1.3	1008	PASS
174	95	50	100	81.7	76939	PASS
175	174	5	9	7.2	5564	PASS
176	174	95	101	96.1	73920	PASS
177	176	5	9	6.8	5039	PASS