
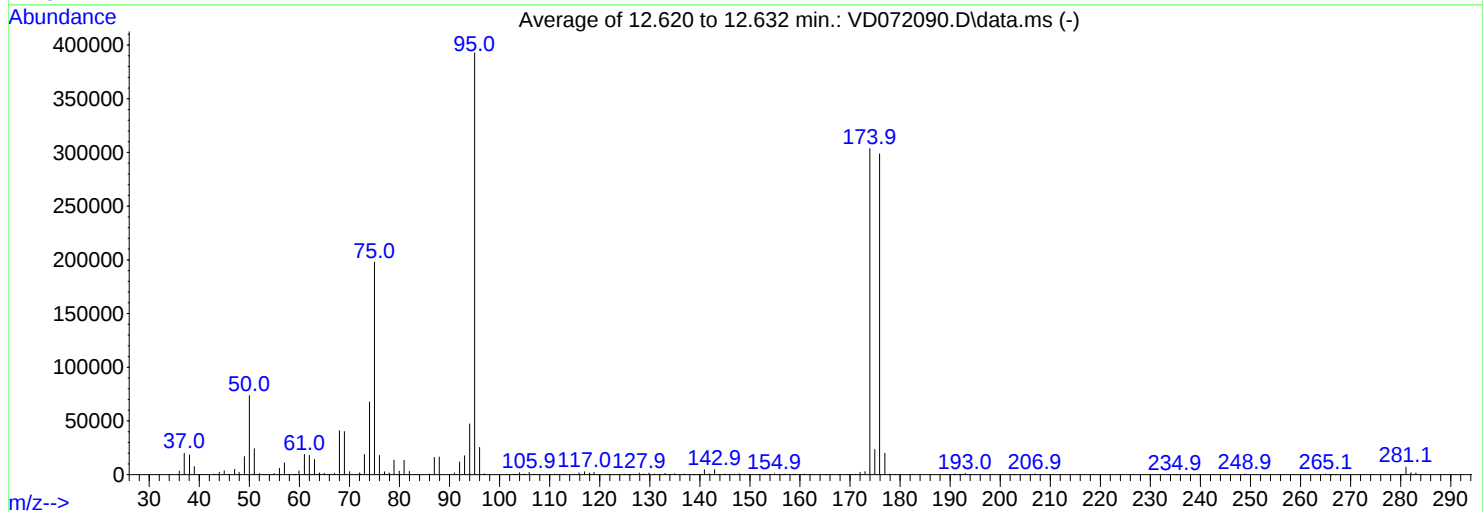


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022522\
 Data File : VD072090.D
 Acq On : 25 Feb 2022 09:24
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021822S.M
 Title : SW846 8260
 Last Update : Sat Feb 19 04:05:38 2022

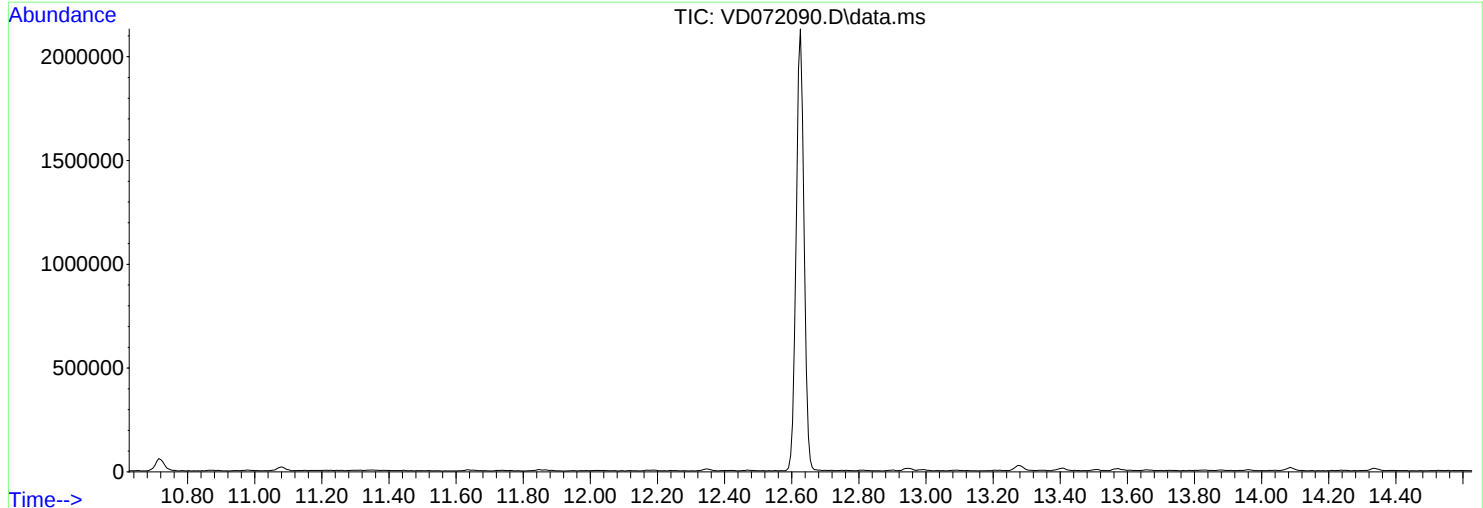

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	73547	PASS
75	95	30	60	50.3	197632	PASS
95	95	100	100	100.0	392747	PASS
96	95	5	9	6.4	25304	PASS
173	174	0.00	2	0.9	2779	PASS
174	95	50	100	77.3	303659	PASS
175	174	5	9	7.7	23392	PASS
176	174	95	101	98.4	298731	PASS
177	176	5	9	6.7	19997	PASS