
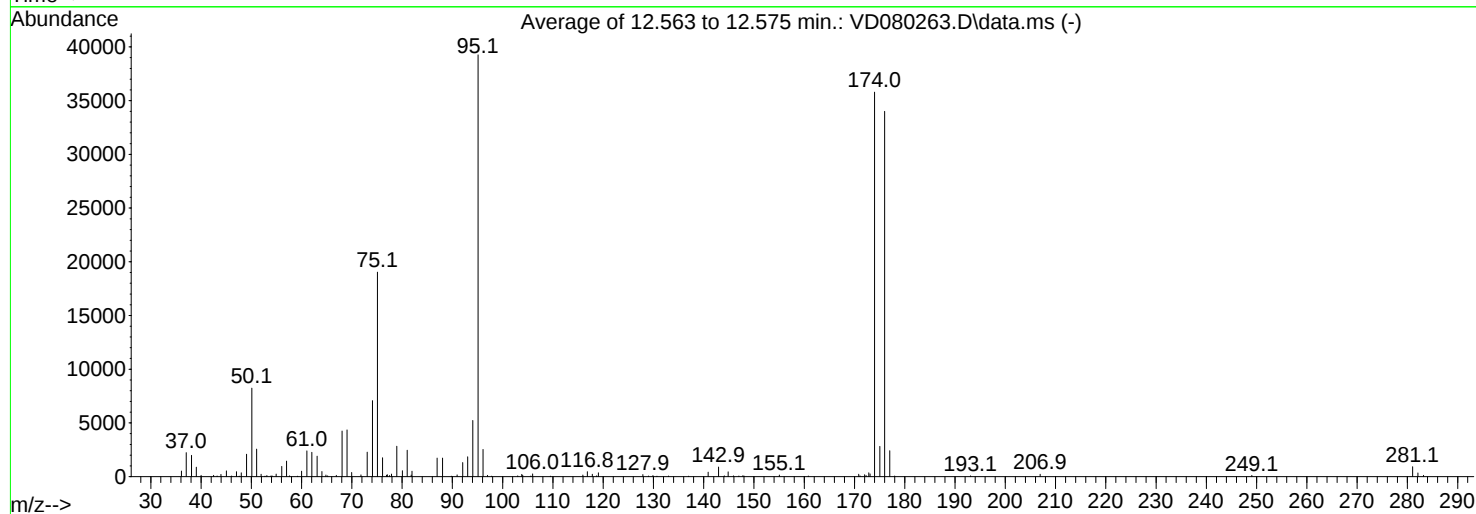


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022525\
Data File : VD080263.D
Acq On : 25 Feb 2025 10:14
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020325S.M
Title : SW846 8260
Last Update : Tue Feb 04 05:44:14 2025

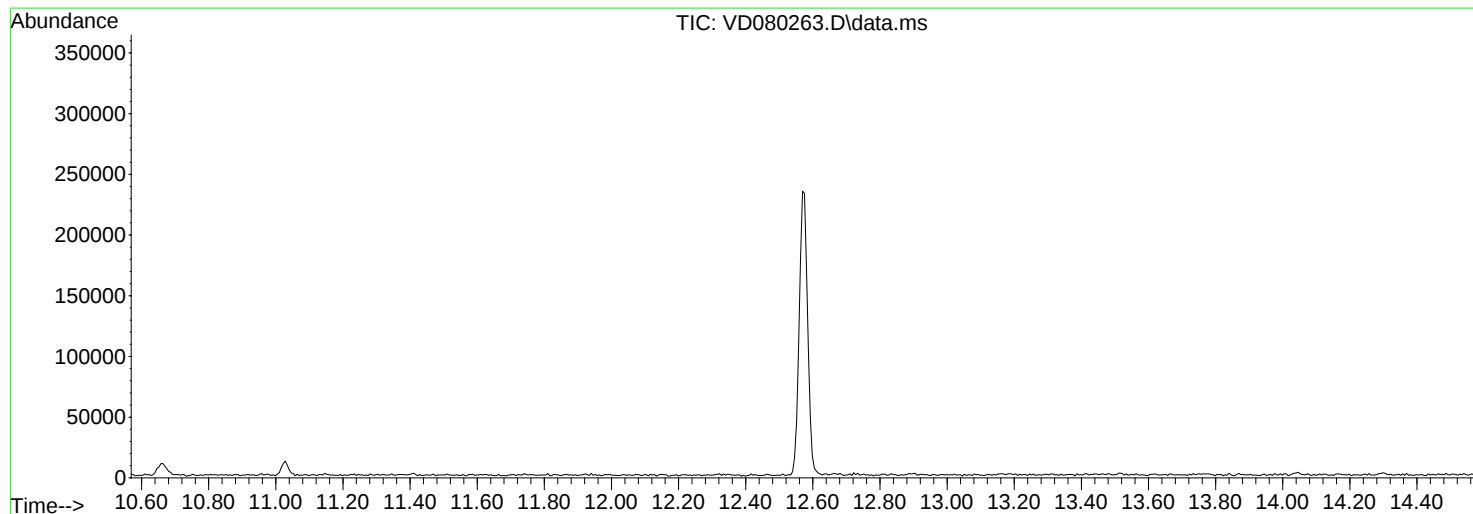

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	8244	PASS
75	95	30	60	48.5	19036	PASS
95	95	100	100	100.0	39264	PASS
96	95	5	9	6.5	2538	PASS
173	174	0.00	2	1.0	364	PASS
174	95	50	100	91.1	35789	PASS
175	174	5	9	7.8	2808	PASS
176	174	95	101	95.0	34011	PASS
177	176	5	9	7.1	2406	PASS