

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD022620\
 Data File : VD065326.D
 Acq On : 26 Feb 2020 14:21
 Operator : VA/SY
 Sample : L1688-02
 Misc : 7.51G/5.00ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 GP-02-022420

Quant Time: Feb 27 08:22:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:26:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.99	168	548707	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	931456	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	821806	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	336260	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	285792	57.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	115.80%	
35) Dibromofluoromethane	7.92	113	297093	52.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.62%	
50) Toluene-d8	10.34	98	1137241	52.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.76%	
62) 4-Bromofluorobenzene	12.64	95	317871	46.21	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.42%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD022620\
Data File : VD065326.D
Acq On : 26 Feb 2020 14:21
Operator : VA/SY
Sample : L1688-02
Misc : 7.51G/5.00ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
GP-02-022420

Quant Time: Feb 27 08:22:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:26:54 2020
Response via : Initial Calibration

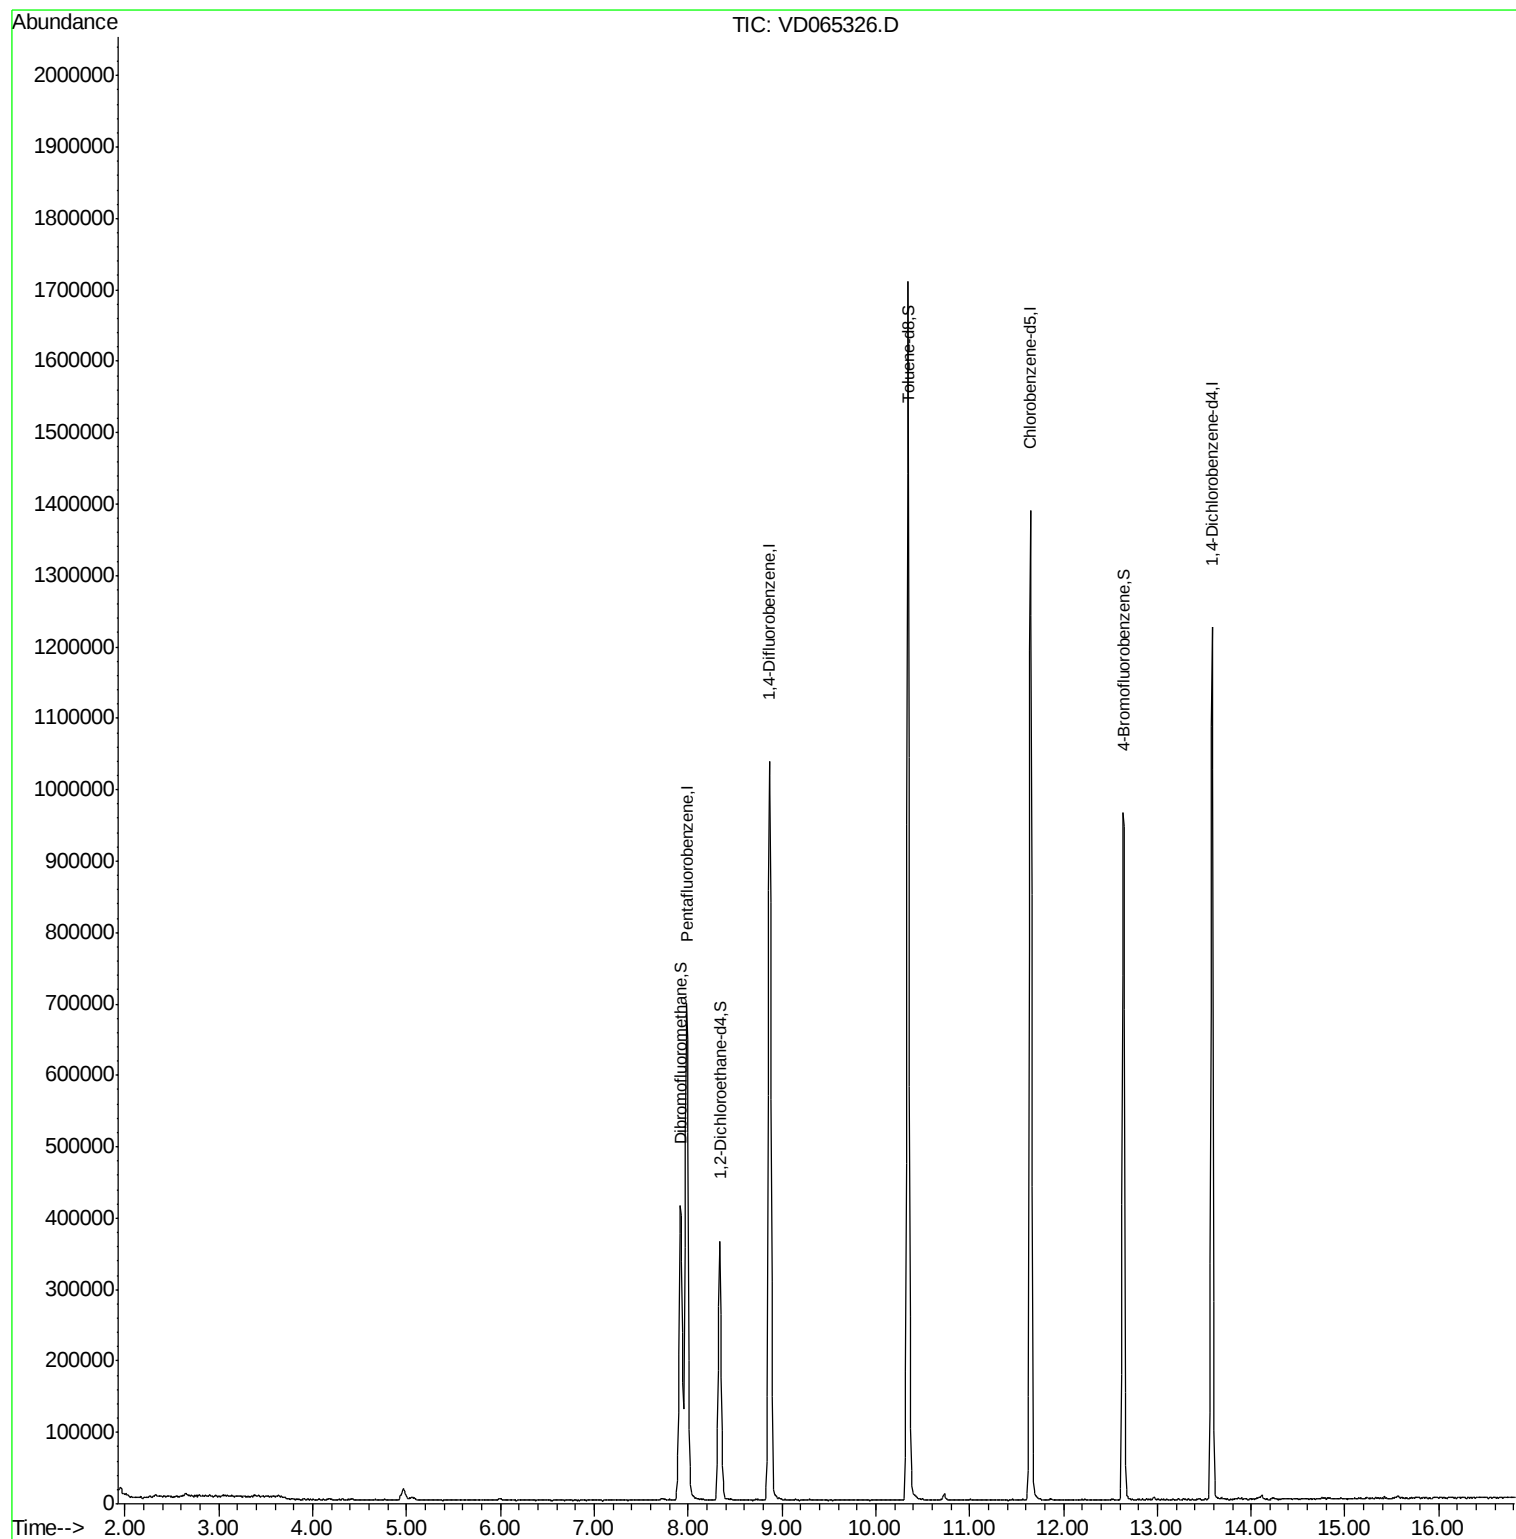

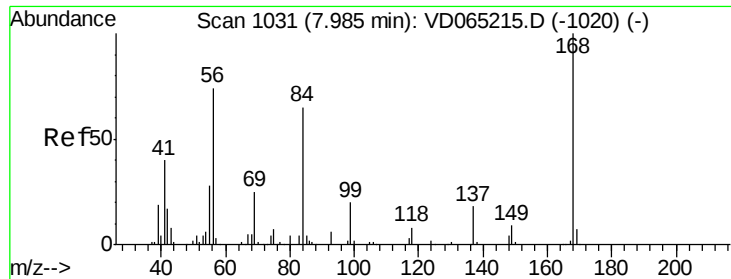

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.99 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21

Instrument :

MSVOA_D

ClientSampleId :


GP-02-022420

Tot Ion:168 Resp: 548707

Ion Ratio Lower Upper




168 100

99 52.4 41.4 62.2

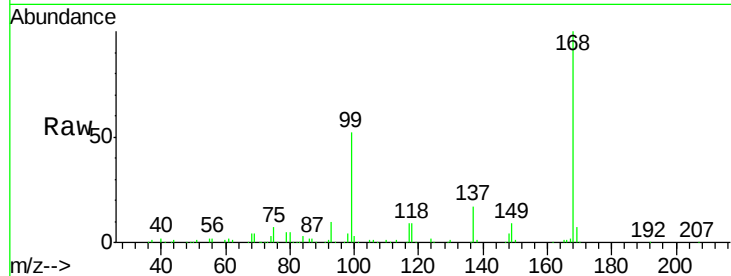

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

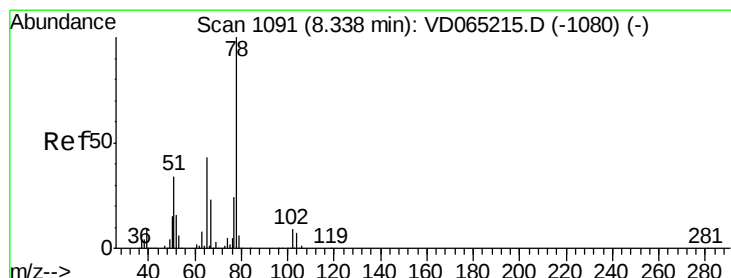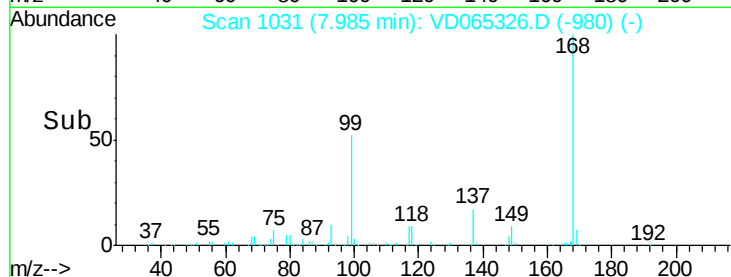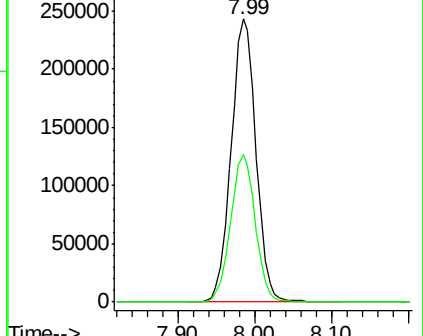

#33

1,2-Dichloroethane-d4

Concen: 57.897 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. 0.00 min

Lab File: VD065326.D


Acq: 26 Feb 2020 14:21

Tgt Ion: 65 Resp: 285792

Ion Ratio Lower Upper



65 100


67 53.5 0.0 106.8

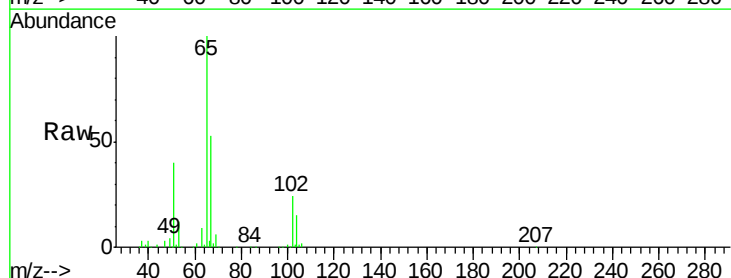

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

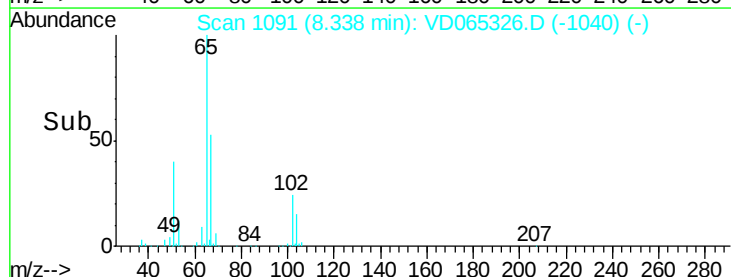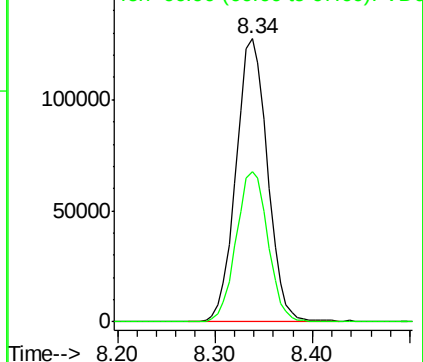

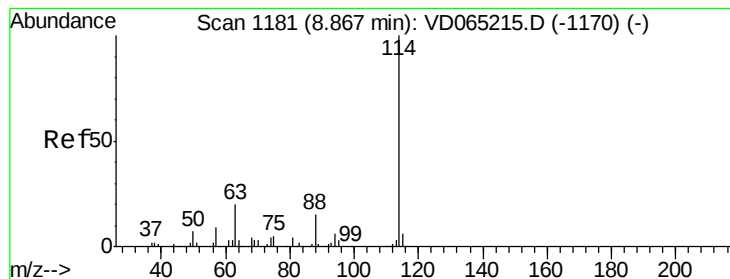

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21

Instrument :

MSVOA_D

ClientSampleId :

GP-02-022420


Tot Ion:114 Resp: 931456

Ion Ratio Lower Upper

114 100

63 20.8 0.0 39.4




88 15.7 0.0 30.4

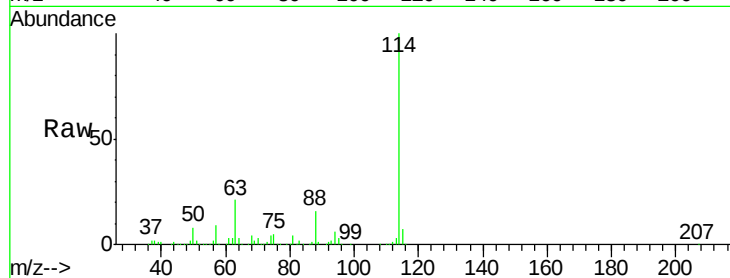

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

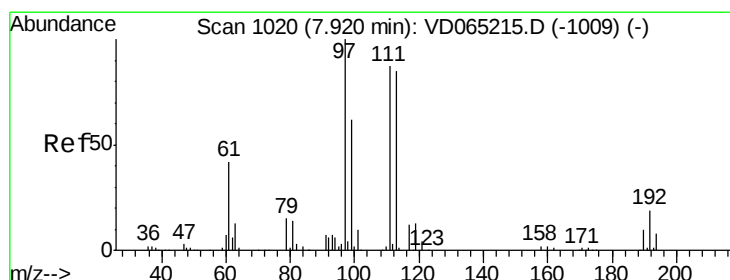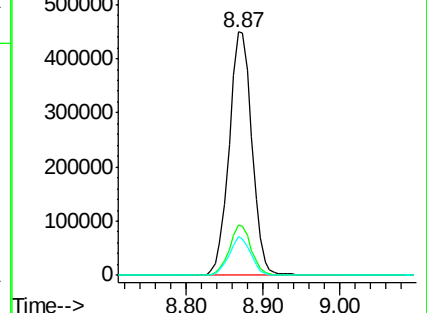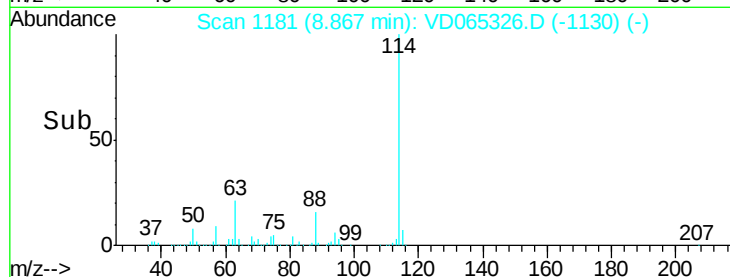

#35

Dibromofluoromethane

Concen: 52.310 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21


Tgt Ion:113 Resp: 297093

Ion Ratio Lower Upper

113 100

111 103.3 82.9 124.3



192 22.1 17.3 25.9

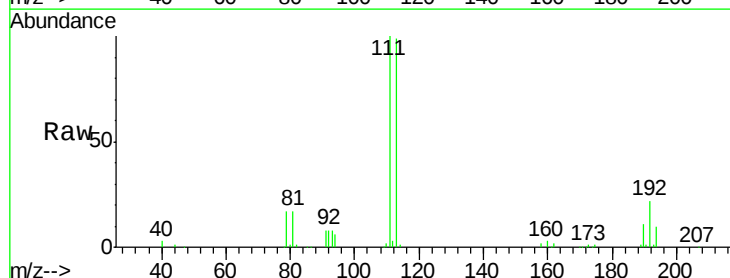


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

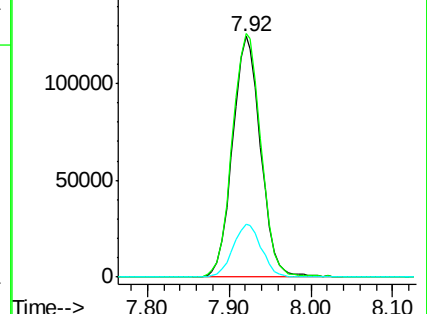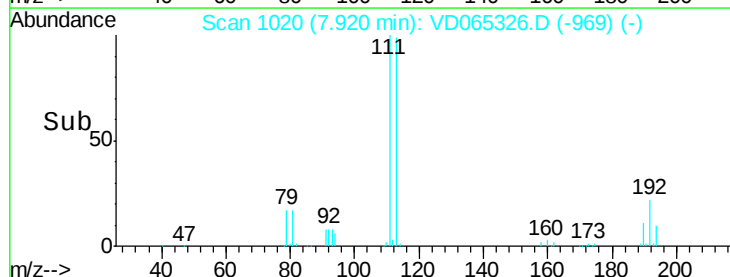

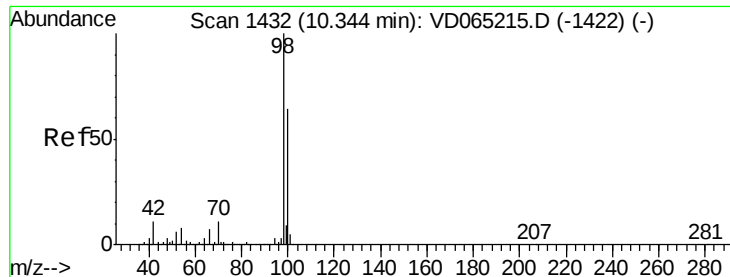

#50

Toluene-d8

Concen: 52.378 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21

Instrument :

MSVOA_D

ClientSampleId :





GP-02-022420

Tot Ion: 98 Resp: 1137241

Ion Ratio Lower Upper

98 100

100 65.2 52.0 78.0

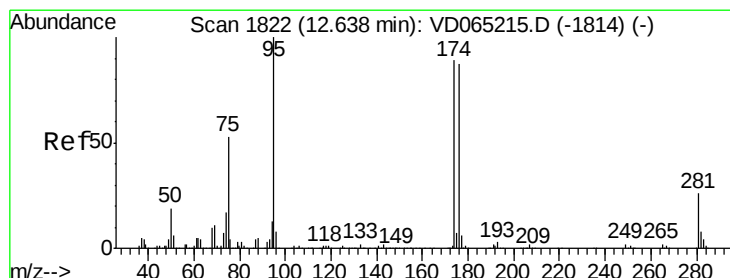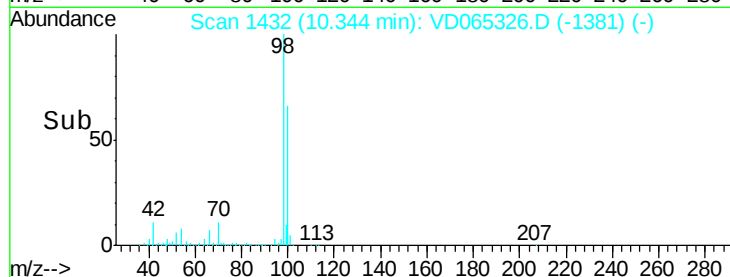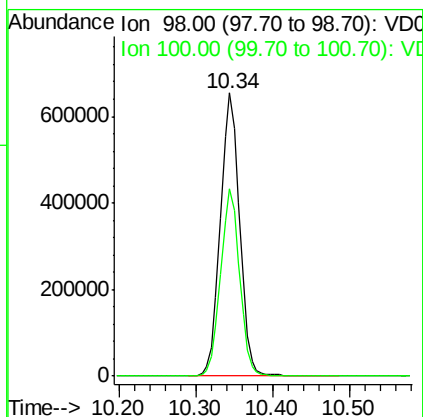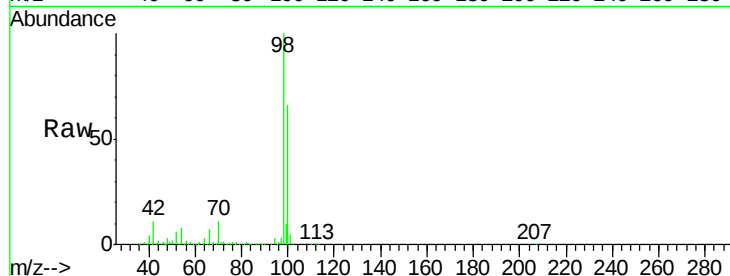

#62

4-Bromofluorobenzene

Concen: 46.214 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21




Tgt Ion: 95 Resp: 317871


Ion Ratio Lower Upper

95 100

174 90.3 0.0 178.0

176 85.8 0.0 174.4

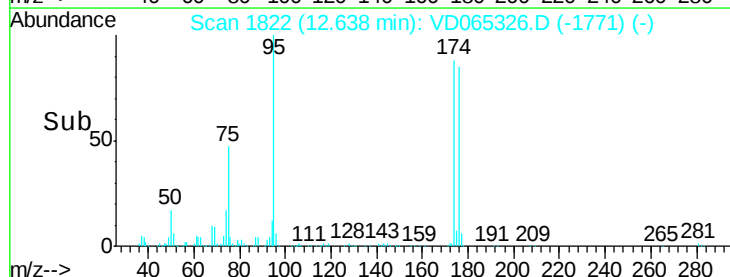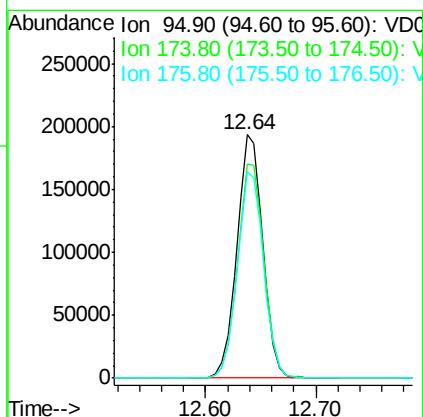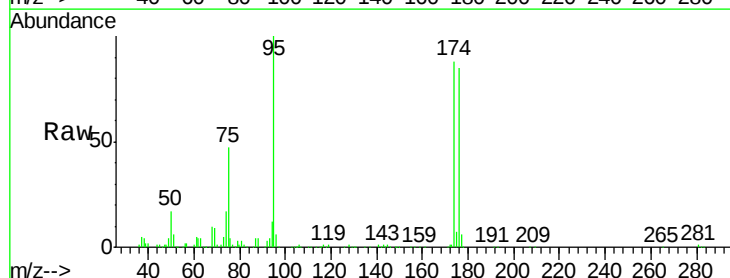

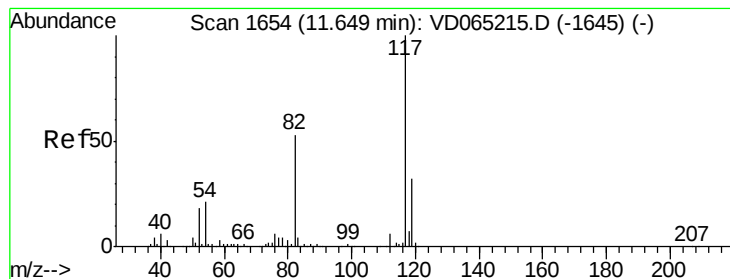

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.65 min Scan# 1654

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21

Instrument :

MSVOA_D

ClientSampleId :

GP-02-022420


Tot Ion:117 Resp: 821806

Ion Ratio Lower Upper

117 100

82 52.2 42.7 64.1




119 32.2 25.5 38.3

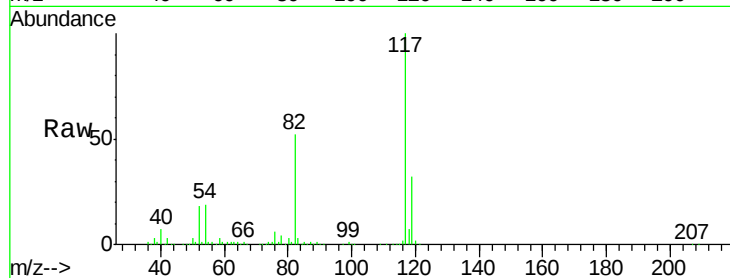

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

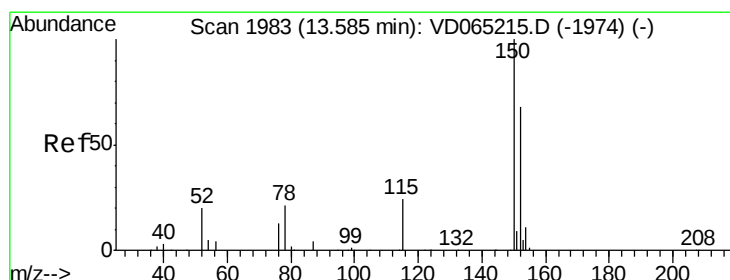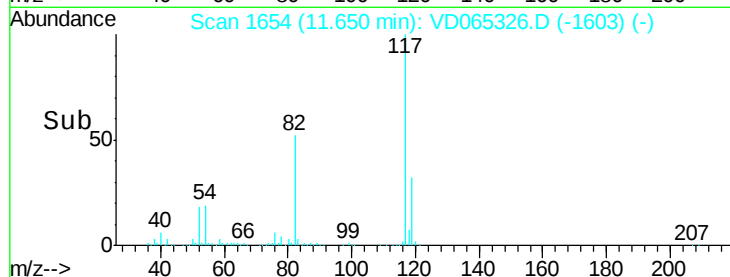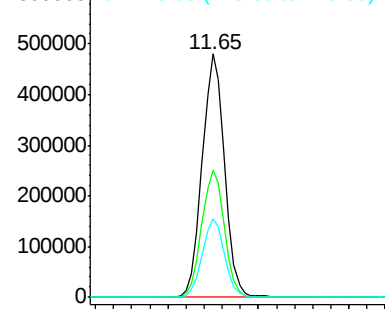

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.00 min

Lab File: VD065326.D

Acq: 26 Feb 2020 14:21


Tgt Ion:152 Resp: 336260

Ion Ratio Lower Upper

152 100

115 55.2 27.6 82.8

150 157.3 0.0 347.4

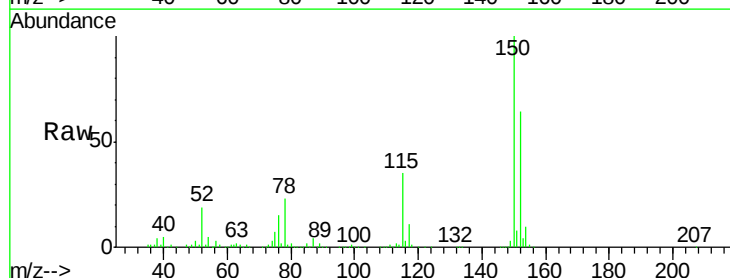

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

