

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022621\
 Data File : VD068460.D
 Acq On : 26 Feb 2021 16:57
 Operator : VA/SY
 Sample : M1477-01
 Misc : 5.07G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 72-11995

Quant Time: Feb 26 21:48:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.979	168	364480	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	676286	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	629037	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	286289	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	188078	51.65	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.30%
35) Dibromofluoromethane	7.920	113	111102	27.27	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	54.54%
50) Toluene-d8	10.338	98	851808	52.49	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.98%
62) 4-Bromofluorobenzene	12.632	95	269886	51.61	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	103.22%
Target Compounds						
16) Acetone	4.162	43	17116	29.59	ug/l	96
20) Methylene Chloride	4.967	84	55242	9.39	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022621\
Data File : VD068460.D
Acq On : 26 Feb 2021 16:57
Operator : VA/SY
Sample : M1477-01
Misc : 5.07G/5.00ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
72-11995

Quant Time: Feb 26 21:48:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration




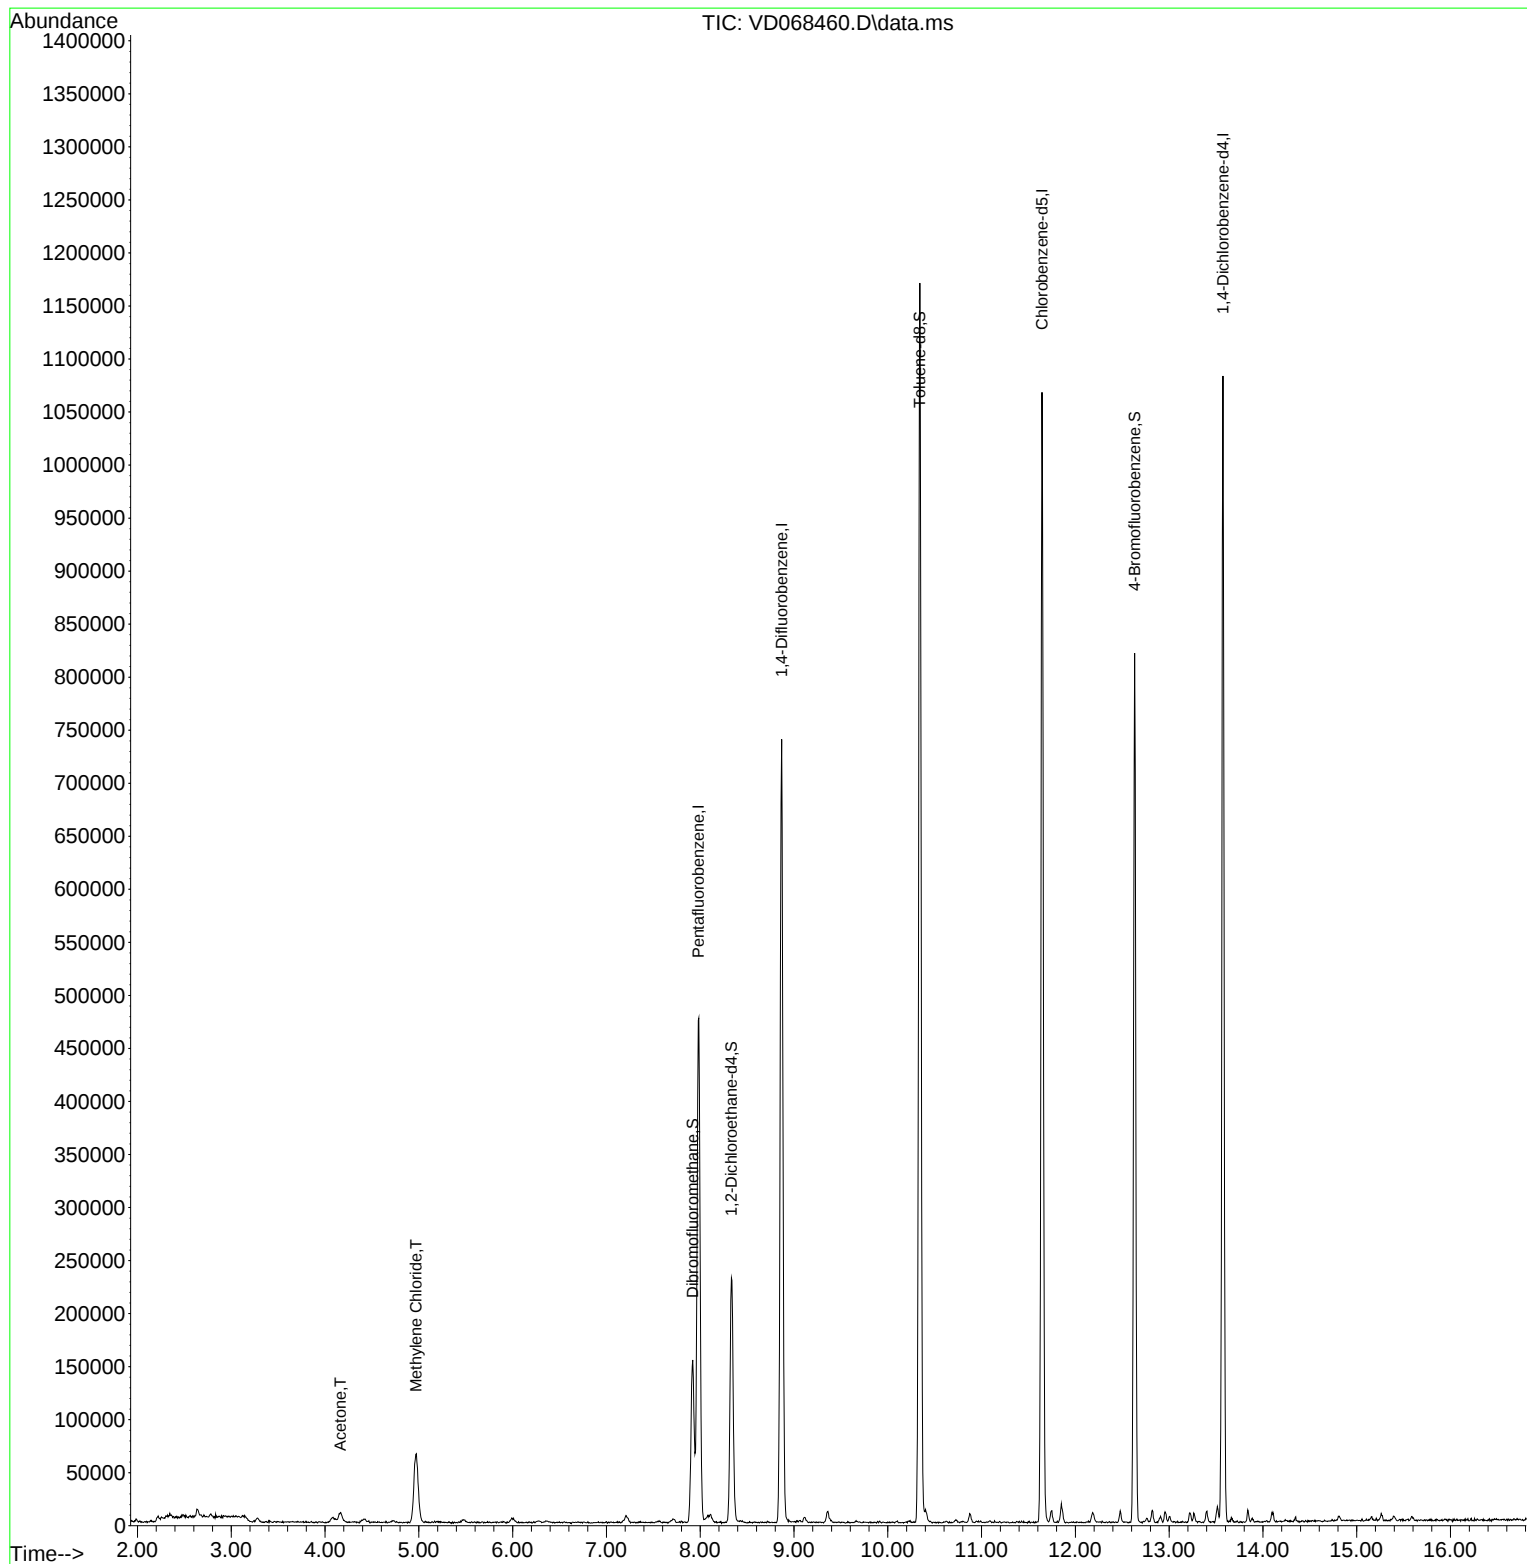


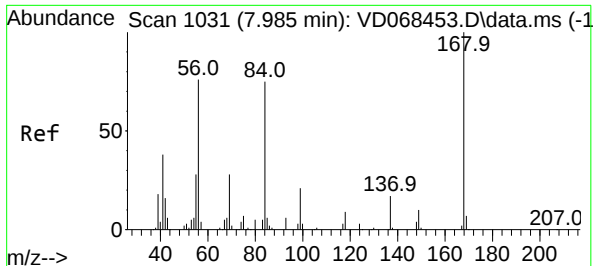

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57




Instrument :
MSVOA_D
ClientSampleId :
72-11995


Tgt Ion:168 Resp: 364480
Ion Ratio Lower Upper
168 100
99 55.7 43.5 65.3

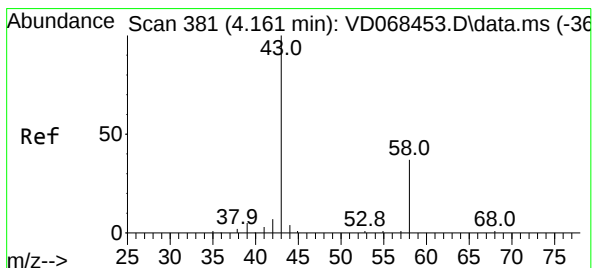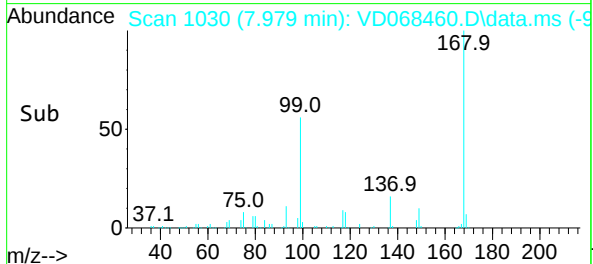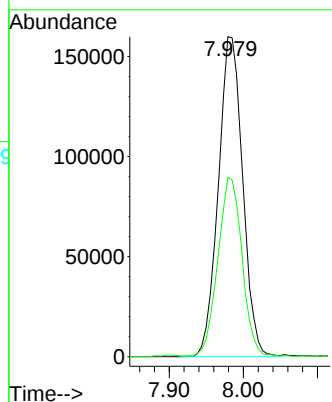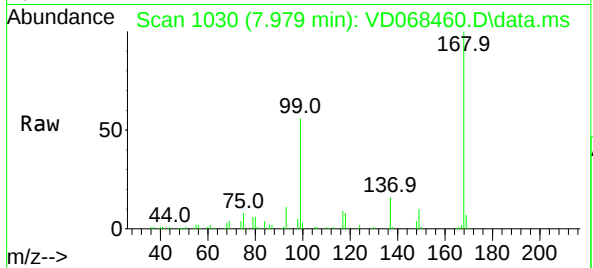

#16
Acetone
Concen: 29.59 ug/l
RT: 4.162 min Scan# 381
Delta R.T. 0.000 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57


Tgt Ion: 43 Resp: 17116
Ion Ratio Lower Upper
43 100
58 28.1 24.2 36.4

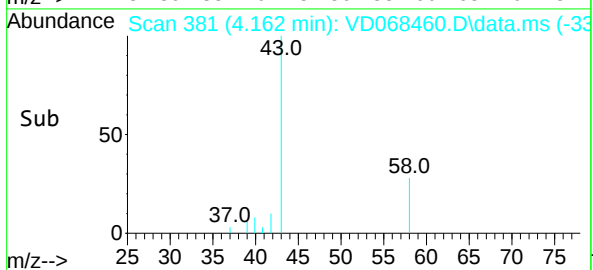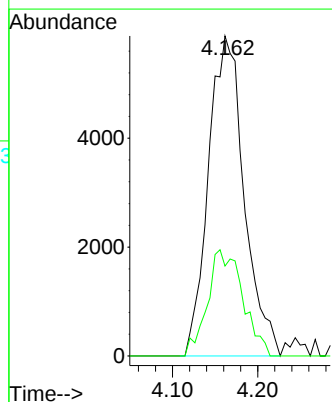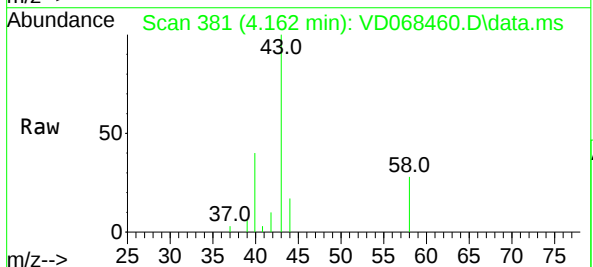



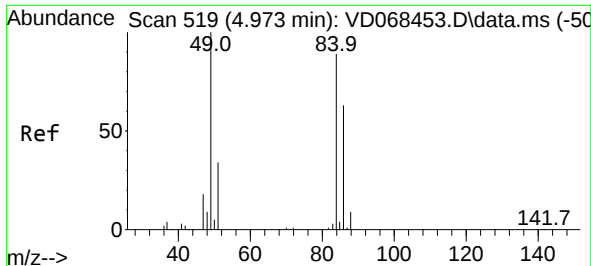


#20
Methylene Chloride
Concen: 9.39 ug/l
RT: 4.967 min Scan# 518
Delta R.T. -0.006 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Instrument :
MSVOA_D
ClientSampleId :
72-11995



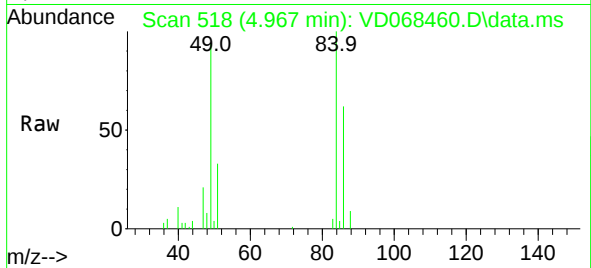



Tgt Ion:	84	Resp:	55242
Ion	Ratio	Lower	Upper
84	100		
49	93.9	77.4	116.2
51	32.5	26.1	39.1
86	61.5	51.8	77.8

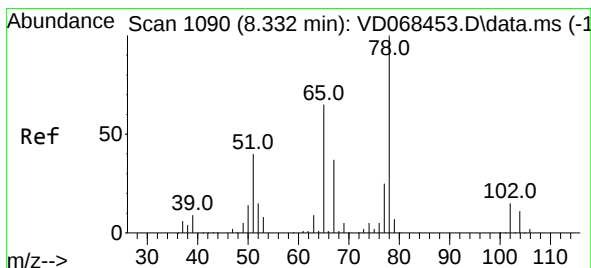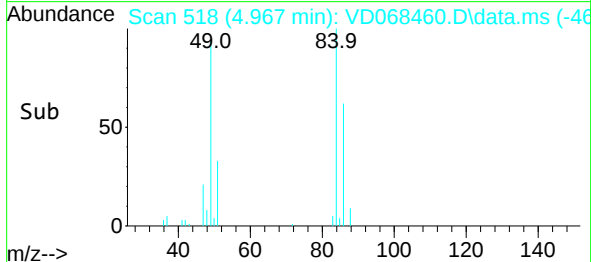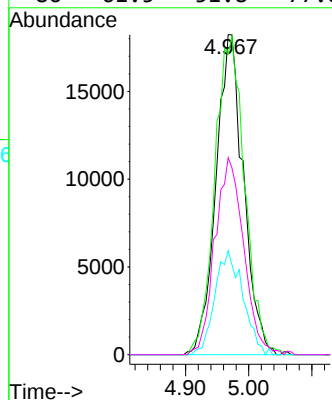

#33
1,2-Dichloroethane-d4
Concen: 51.65 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Tgt Ion:	65	Resp:	188078
Ion	Ratio	Lower	Upper
65	100		
67	53.2	0.0	105.0

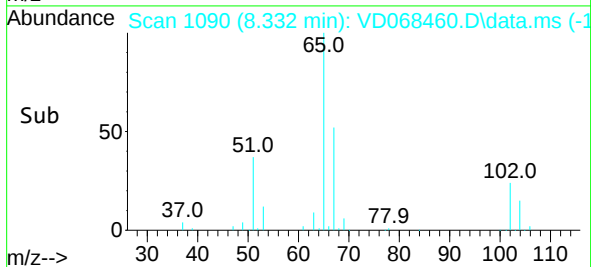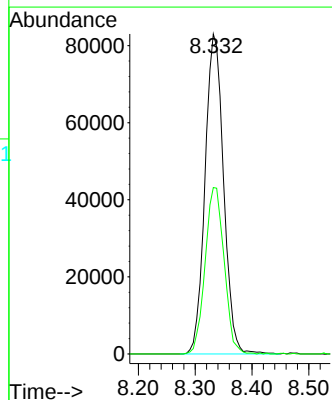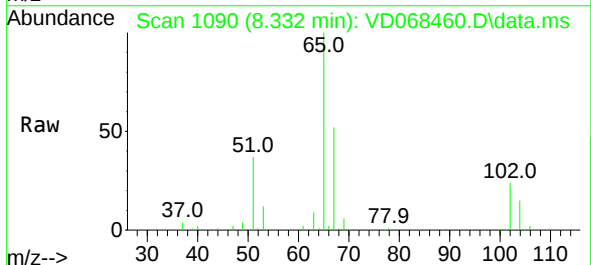




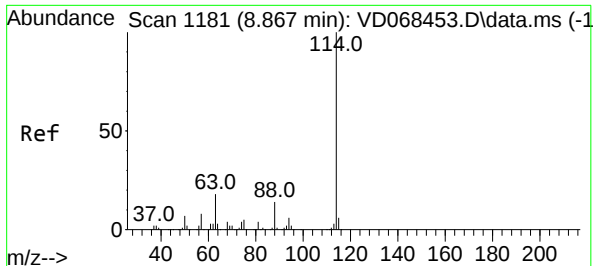


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Instrument :
MSVOA_D
ClientSampleId :
72-11995




Tgt Ion:114 Resp: 676286
Ion Ratio Lower Upper
114 100
63 19.1 0.0 34.8
88 14.2 0.0 31.6

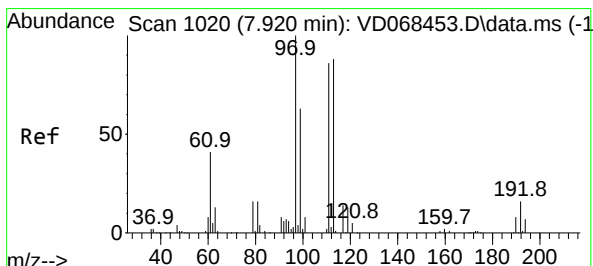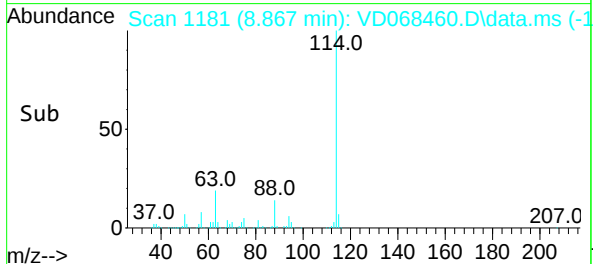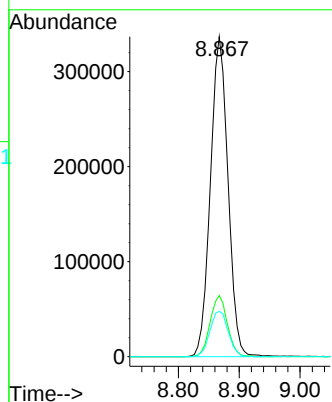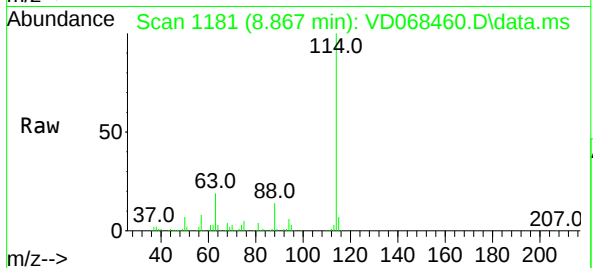


#35

Dibromofluoromethane
Concen: 27.27 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Tgt Ion:113 Resp: 111102
Ion Ratio Lower Upper
113 100
111 103.1 81.4 122.0
192 18.8 16.1 24.1


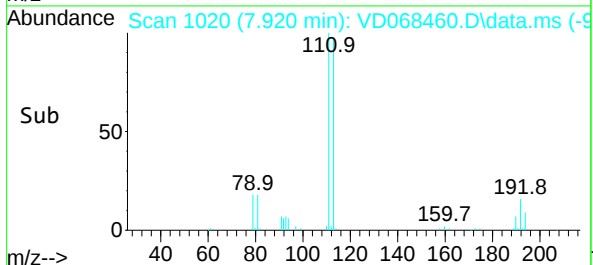
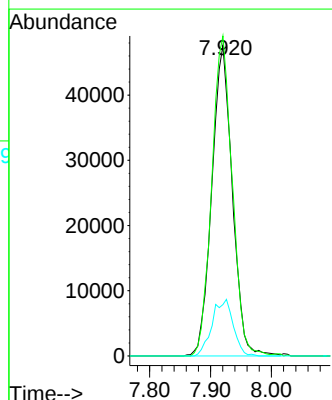
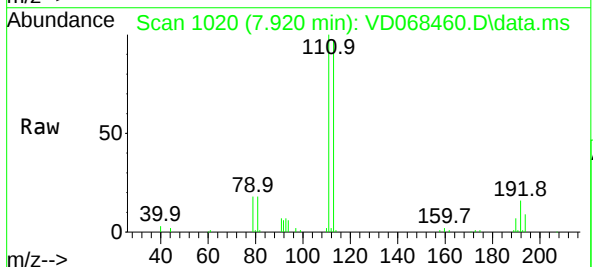


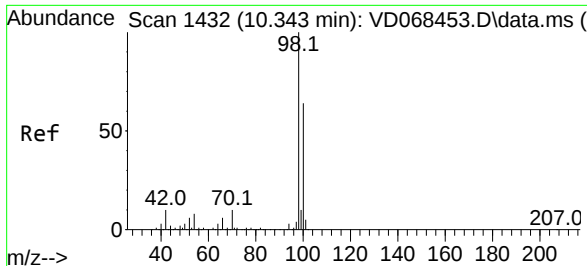

#50
Toluene-d8
Concen: 52.49 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57




Instrument :
MSVOA_D
ClientSampleId :
72-11995


Tgt Ion: 98 Resp: 851808
Ion Ratio Lower Upper
98 100
100 63.3 53.0 79.4

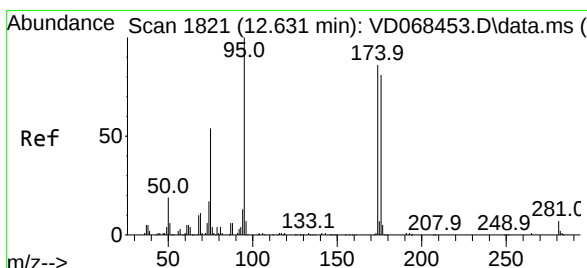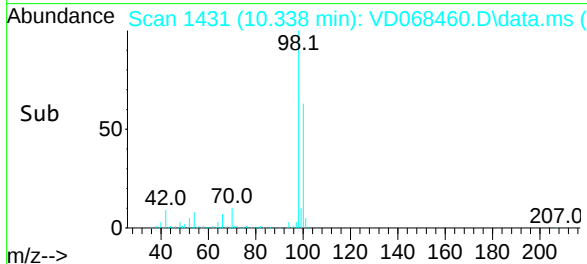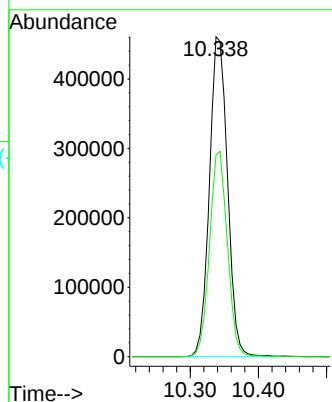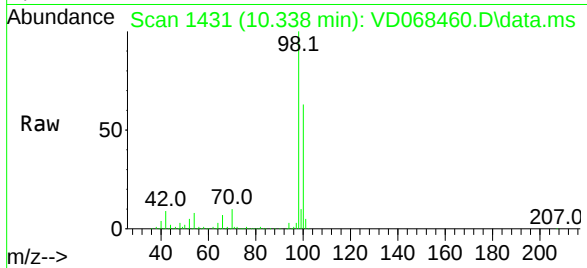

#62
4-Bromofluorobenzene
Concen: 51.61 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Tgt Ion: 95 Resp: 269886
Ion Ratio Lower Upper
95 100
174 81.1 0.0 172.4
176 78.9 0.0 168.4


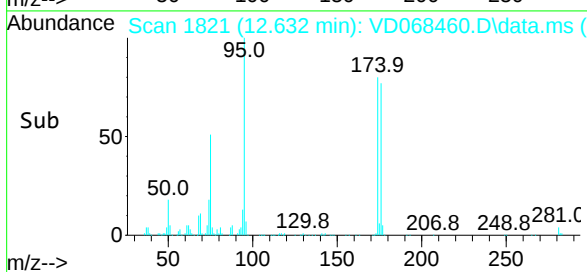
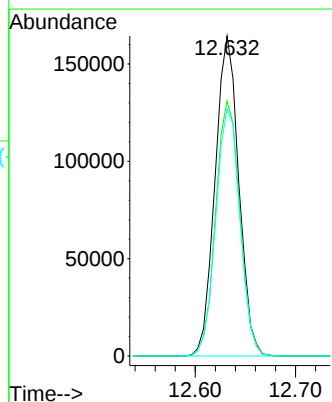
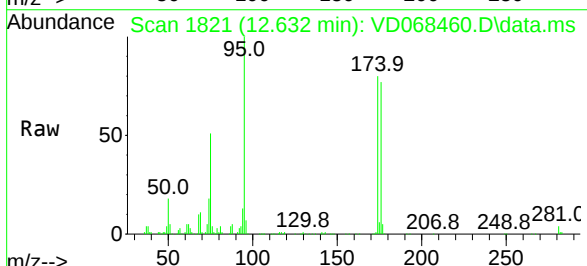


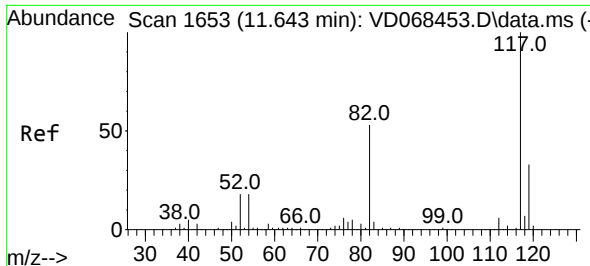

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Instrument :
MSVOA_D
ClientSampleId :
72-11995

Tgt Ion:117 Resp: 629037
Ion Ratio Lower Upper
117 100
82 56.3 41.4 62.0
119 32.2 26.1 39.1

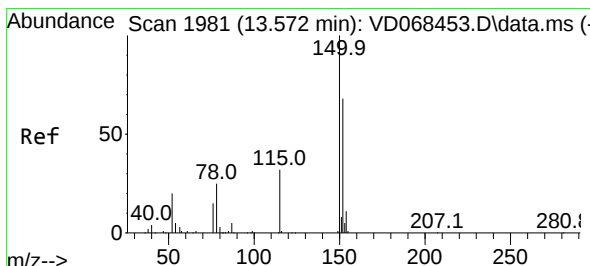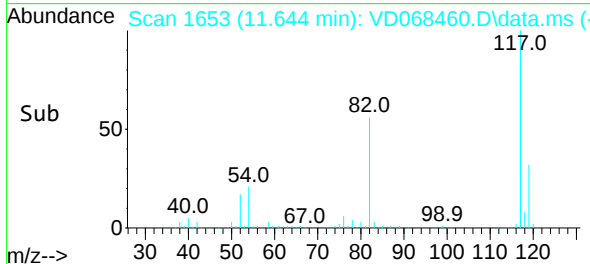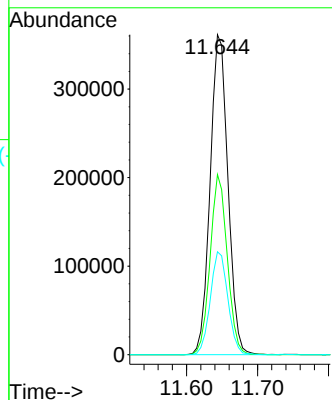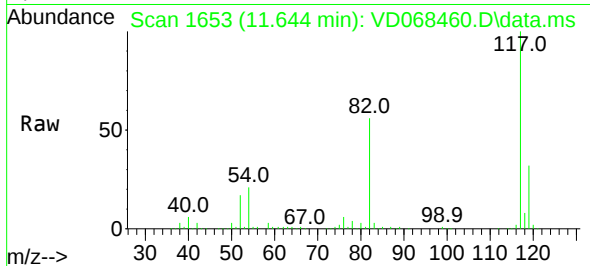

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.001 min
Lab File: VD068460.D
Acq: 26 Feb 2021 16:57

Tgt Ion:152 Resp: 286289
Ion Ratio Lower Upper
152 100
115 58.6 28.9 86.8
150 156.9 0.0 344.4

